

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
 Data File : BP003869.D
 Acq On : 09 Nov 2020 15:40
 Operator : CG/JU
 Sample : L4665-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-8-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003869.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.934	4	8	16	rVB	2495674	2983645	100.00%	10.839%
2	3.105	32	37	46	rVB	65714	100551	3.37%	0.365%
3	3.187	46	51	57	rVB	184023	216929	7.27%	0.788%
4	5.816	491	498	507	rBV	1029416	1499769	50.27%	5.449%
5	7.463	766	778	788	rBV	940100	1516731	50.83%	5.510%
6	8.299	913	920	928	rBV	218046	352071	11.80%	1.279%
7	9.463	1109	1118	1129	rBV	578602	978886	32.81%	3.556%
8	11.134	1394	1402	1409	rBV	262099	448205	15.02%	1.628%
9	13.540	1804	1811	1824	rBV	1285699	1865549	62.53%	6.777%
10	14.340	1942	1947	1955	rBV	142436	188022	6.30%	0.683%
11	14.916	2039	2045	2055	rVB	378734	556657	18.66%	2.022%
12	15.316	2106	2113	2114	rBV6	16994	33956	1.14%	0.123%
13	15.692	2173	2177	2182	rVB	24971	34914	1.17%	0.127%
14	16.392	2290	2296	2308	rBV	1004510	1476038	49.47%	5.362%
15	17.004	2395	2400	2410	rVB4	43904	86539	2.90%	0.314%
16	17.645	2503	2509	2515	rBV	450203	626257	20.99%	2.275%
17	18.480	2646	2651	2654	rBV2	64314	90606	3.04%	0.329%
18	18.545	2658	2662	2663	rVV	46579	62140	2.08%	0.226%
19	18.575	2664	2667	2674	rVB2	74197	145863	4.89%	0.530%
20	18.745	2691	2696	2699	rBV2	103718	156177	5.23%	0.567%
21	18.780	2699	2702	2716	rVB	158233	274153	9.19%	0.996%
22	19.333	2788	2796	2805	rBV2	124879	340233	11.40%	1.236%
23	19.445	2805	2815	2820	rBV3	335971	838559	28.11%	3.046%
24	19.504	2820	2825	2835	rVB	669421	1119968	37.54%	4.069%
25	19.645	2844	2849	2855	rVB	37813	71534	2.40%	0.260%
26	19.792	2868	2874	2884	rVB	129087	224757	7.53%	0.817%
27	20.139	2927	2933	2938	rBV	1954676	2468622	82.74%	8.968%
28	20.210	2938	2945	2951	rVV	314958	542001	18.17%	1.969%
29	20.874	3052	3058	3069	rBV	497188	787136	26.38%	2.860%
30	21.216	3113	3116	3120	rBV4	37658	48686	1.63%	0.177%
31	21.321	3130	3134	3141	rBV	269640	351703	11.79%	1.278%
32	21.474	3155	3160	3166	rBV	544725	770605	25.83%	2.800%
33	21.669	3185	3193	3199	rBV	544005	769636	25.80%	2.796%
34	21.769	3207	3210	3215	rVB2	121998	136089	4.56%	0.494%
35	22.104	3261	3267	3274	rBV	506975	846817	28.38%	3.076%
36	22.233	3285	3289	3298	rVB	172907	254317	8.52%	0.924%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
 Data File : BP003869.D
 Acq On : 09 Nov 2020 15:40
 Operator : CG/JU
 Sample : L4665-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-8-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	22.739	3371	3375	3378	rBV	213477	294363	9.87%	1.069%
38	22.786	3378	3383	3392	rVB	394527	790229	26.49%	2.871%
39	23.298	3465	3470	3476	rVB	166380	264914	8.88%	0.962%
40	23.563	3508	3515	3525	rVB	346395	725460	24.31%	2.636%
41	23.927	3572	3577	3583	rBV2	113641	198873	6.67%	0.722%
42	24.145	3608	3614	3629	rVB2	354306	744644	24.96%	2.705%
43	24.445	3658	3665	3674	rVB	257283	612986	20.54%	2.227%
44	24.645	3696	3699	3707	rVB2	66065	122998	4.12%	0.447%
45	25.457	3830	3837	3849	rVB2	159151	507115	17.00%	1.842%




Sum of corrected areas: 27525903

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003869.D
Acq On : 09 Nov 2020 15:40
Operator : CG/JU
Sample : L4665-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-8-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

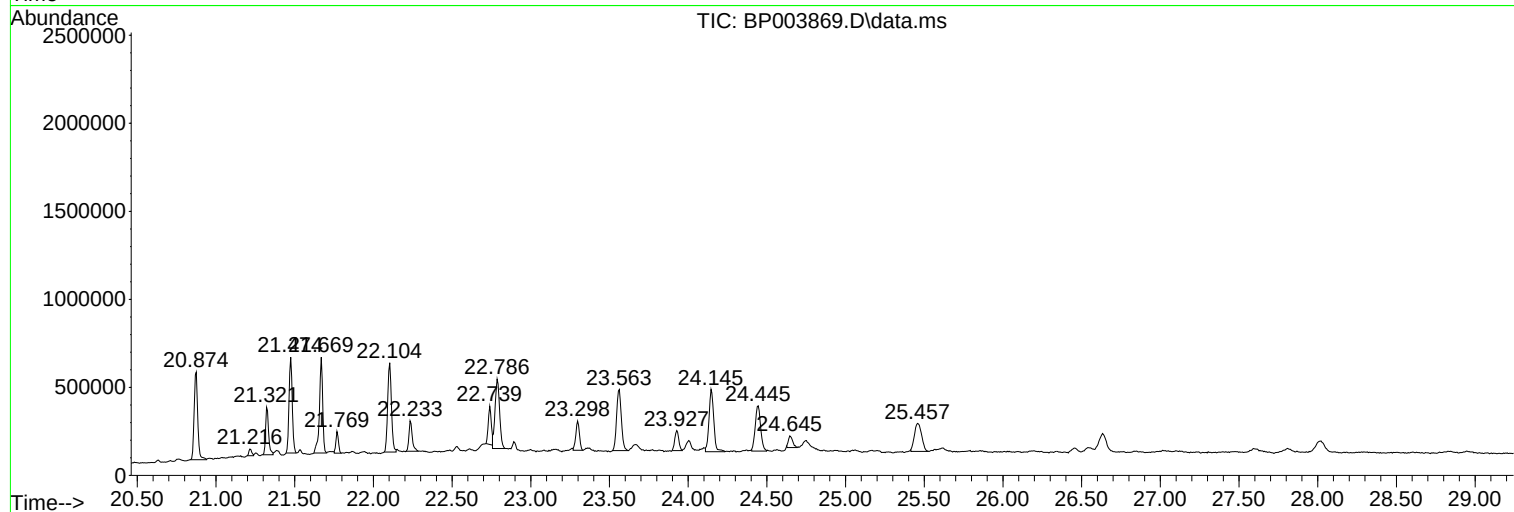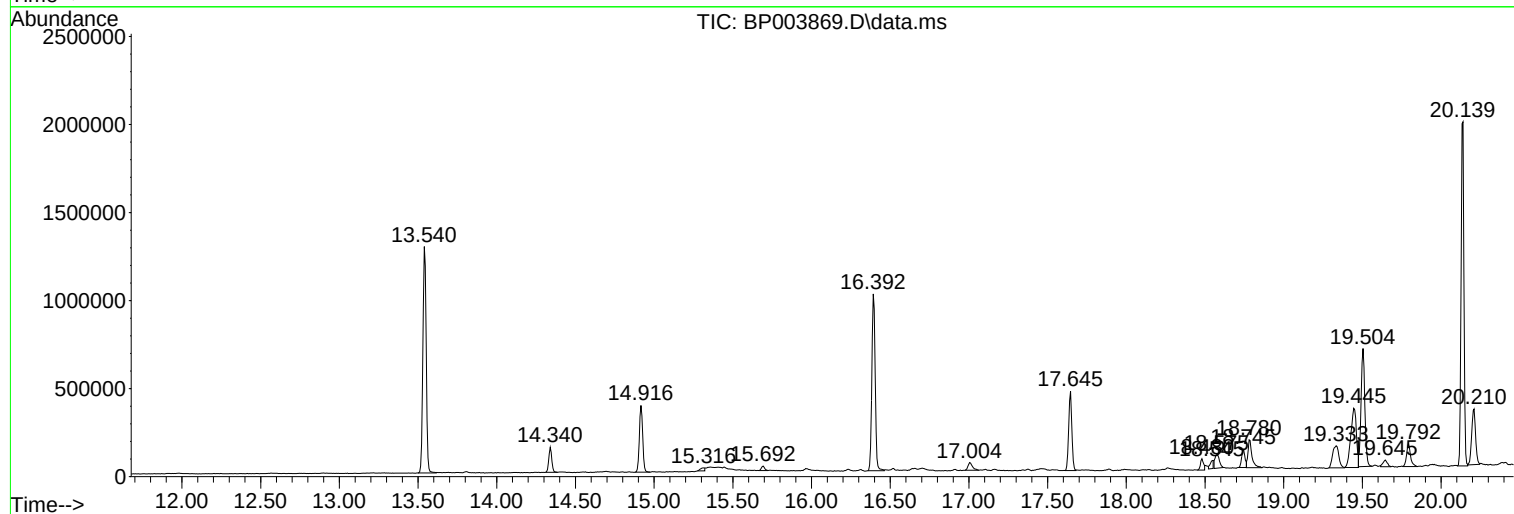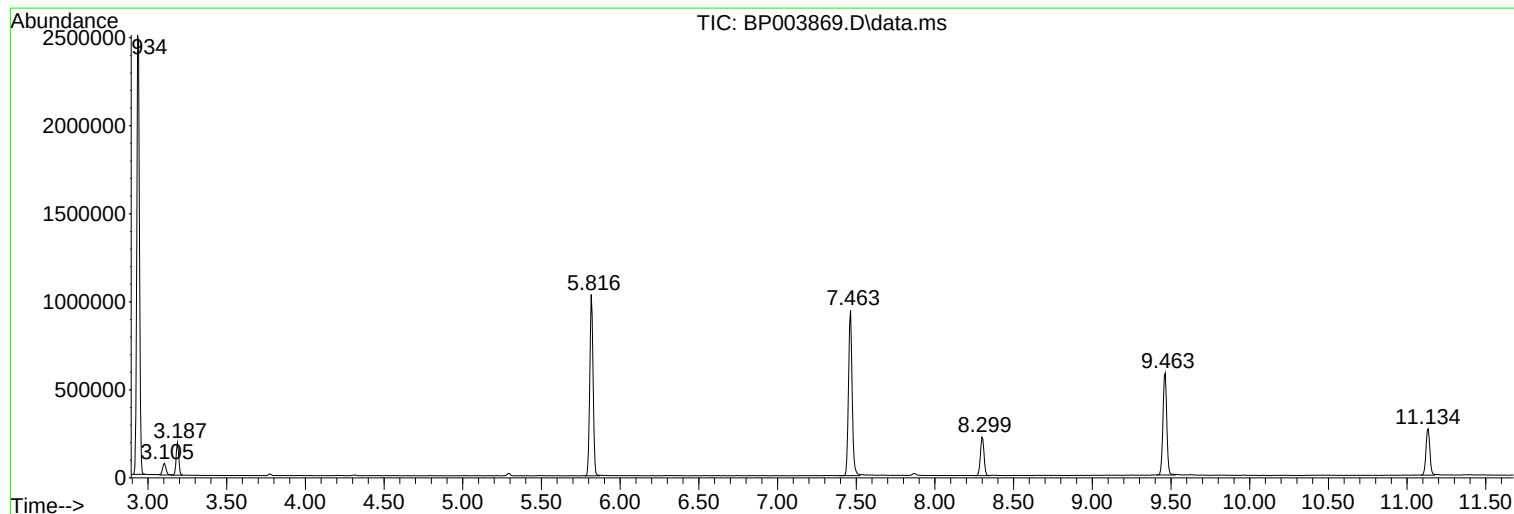

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003869.D
Acq On : 09 Nov 2020 15:40
Operator : CG/JU
Sample : L4665-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-8-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003869.D
Acq On : 09 Nov 2020 15:40
Operator : CG/JU
Sample : L4665-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-8-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
