

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
 Data File : BP003872.D
 Acq On : 09 Nov 2020 17:23
 Operator : CG/JU
 Sample : L4658-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 361-CL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003872.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.946	5	10	25	rVB	4758669	5707477	100.00%	17.925%
2	3.105	31	37	47	rVV2	136371	269638	4.72%	0.847%
3	3.193	47	52	64	rVB	276561	360747	6.32%	1.133%
4	5.822	491	499	508	rBV	1581760	2340015	41.00%	7.349%
5	7.463	770	778	791	rBV	1481224	2392907	41.93%	7.515%
6	8.299	909	920	927	rBV	487114	779259	13.65%	2.447%
7	9.463	1108	1118	1128	rBV	918873	1528989	26.79%	4.802%
8	11.134	1394	1402	1412	rBV	614697	1011497	17.72%	3.177%
9	13.540	1804	1811	1826	rBV	2128896	3106119	54.42%	9.755%
10	14.339	1940	1947	1954	rBV	178839	251583	4.41%	0.790%
11	14.916	2038	2045	2056	rBV	890912	1300744	22.79%	4.085%
12	16.392	2290	2296	2313	rBV	1658063	2447628	42.88%	7.687%
13	17.645	2503	2509	2520	rBV	1107106	1527646	26.77%	4.798%
14	18.480	2647	2651	2659	rBV	38085	67402	1.18%	0.212%
15	20.139	2927	2933	2938	rBV	3802368	4590710	80.43%	14.418%
16	21.321	3130	3134	3144	rBV	538553	666674	11.68%	2.094%
17	21.669	3188	3193	3199	rBV	1303951	1726970	30.26%	5.424%
18	24.151	3607	3615	3624	rVB2	859317	1764729	30.92%	5.542%




Sum of corrected areas: 31840734

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003872.D
Acq On : 09 Nov 2020 17:23
Operator : CG/JU
Sample : L4658-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
361-CL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

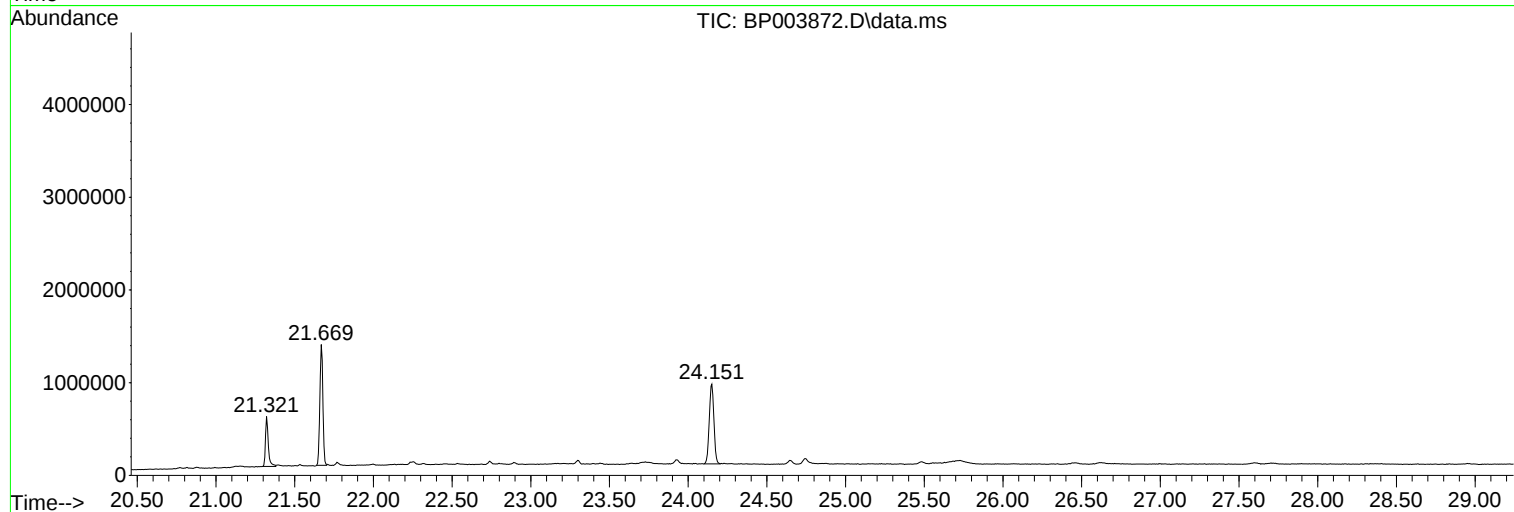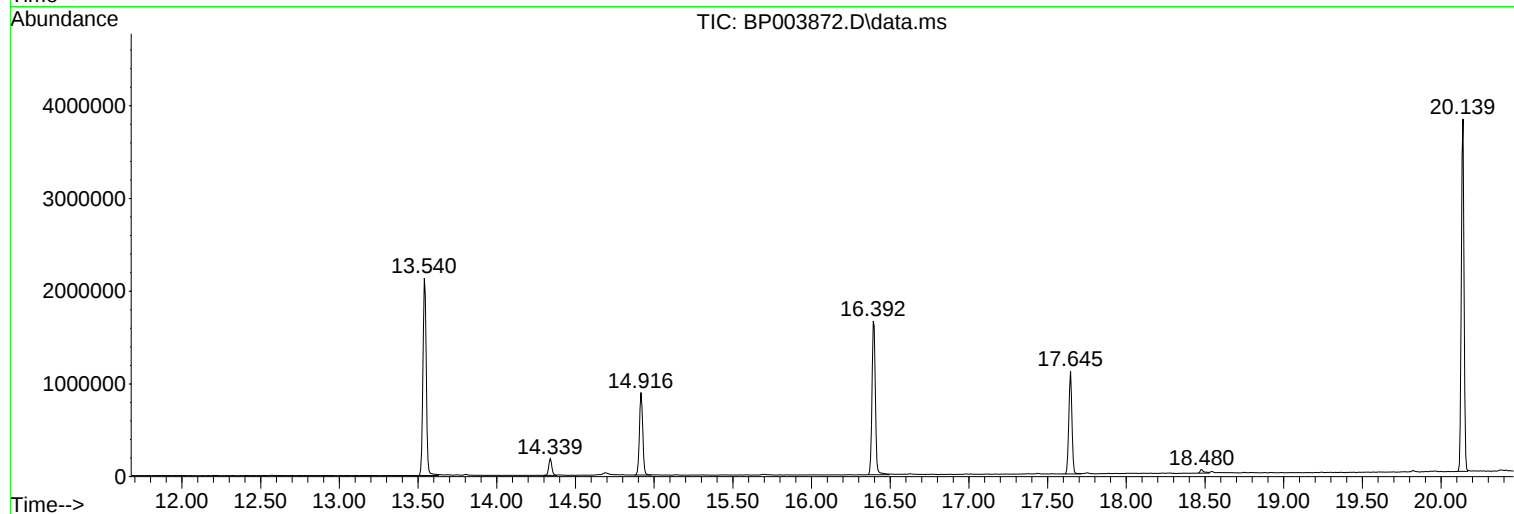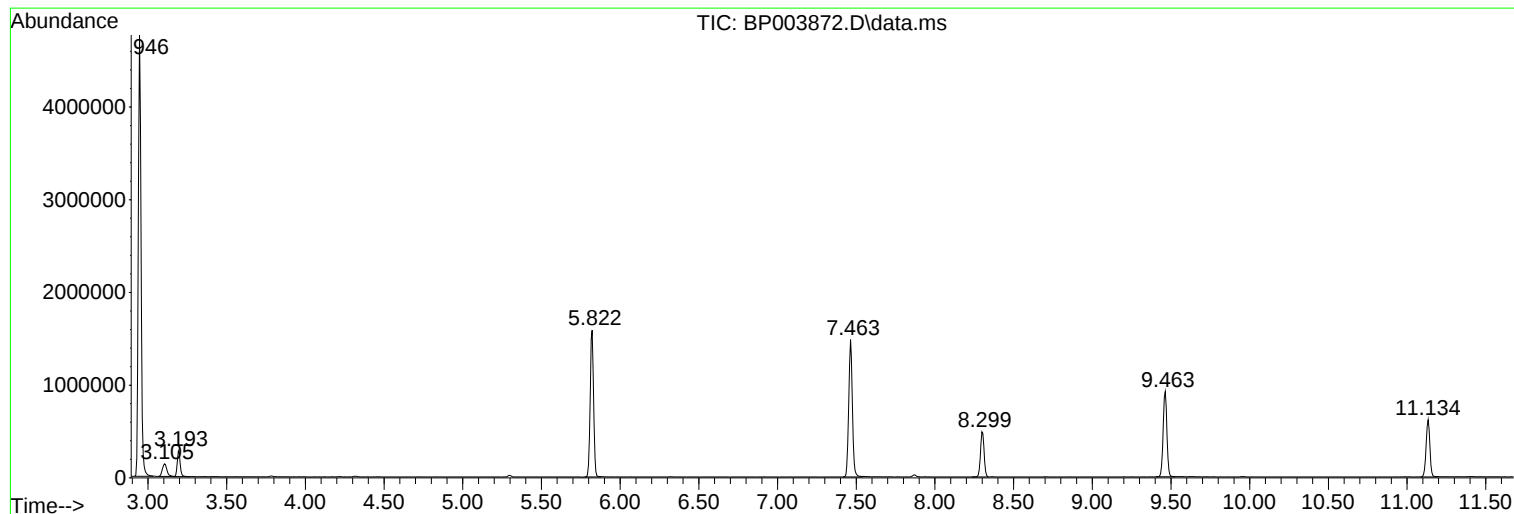

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003872.D
Acq On : 09 Nov 2020 17:23
Operator : CG/JU
Sample : L4658-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
361-CL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003872.D
Acq On : 09 Nov 2020 17:23
Operator : CG/JU
Sample : L4658-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
361-CL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------