

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
 Data File : BP003874.D
 Acq On : 09 Nov 2020 18:31
 Operator : CG/JU
 Sample : L4658-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 361-OS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.946	5	10	29	rVB	6433418	7142458	100.00%	16.313%
2	3.105	30	37	47	rVB	116590	244505	3.42%	0.558%
3	3.193	47	52	59	rBV	369060	429210	6.01%	0.980%
4	5.822	491	499	508	rBV	2212163	3307664	46.31%	7.554%
5	7.463	769	778	798	rBV	2097422	3464526	48.51%	7.913%
6	8.298	912	920	928	rBV	744596	1175898	16.46%	2.686%
7	9.463	1109	1118	1127	rBV	1372982	2227419	31.19%	5.087%
8	11.134	1394	1402	1410	rBV	919195	1549951	21.70%	3.540%
9	13.545	1803	1812	1833	rBV	3104423	4784686	66.99%	10.928%
10	13.804	1850	1856	1863	rVB	169331	249358	3.49%	0.570%
11	14.339	1941	1947	1954	rBV	195827	273921	3.84%	0.626%
12	14.916	2038	2045	2057	rBV	1329992	1995894	27.94%	4.558%
13	16.392	2291	2296	2302	rBV	2239551	3328140	46.60%	7.601%
14	16.622	2331	2335	2341	rBV	264561	389324	5.45%	0.889%
15	17.645	2504	2509	2517	rBV	1572886	2518501	35.26%	5.752%
16	20.139	2928	2933	2940	rVB	4668957	5719287	80.07%	13.062%
17	21.321	3131	3134	3145	rVB	532141	786409	11.01%	1.796%
18	21.668	3189	3193	3205	rVB	1431637	2075509	29.06%	4.740%
19	23.298	3466	3470	3475	rVB	149250	215252	3.01%	0.492%
20	24.145	3607	3614	3623	rVB	837255	1716170	24.03%	3.920%
21	24.645	3694	3699	3706	rVB2	94927	190756	2.67%	0.436%




Sum of corrected areas: 43784838

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003874.D
Acq On : 09 Nov 2020 18:31
Operator : CG/JU
Sample : L4658-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
361-OS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

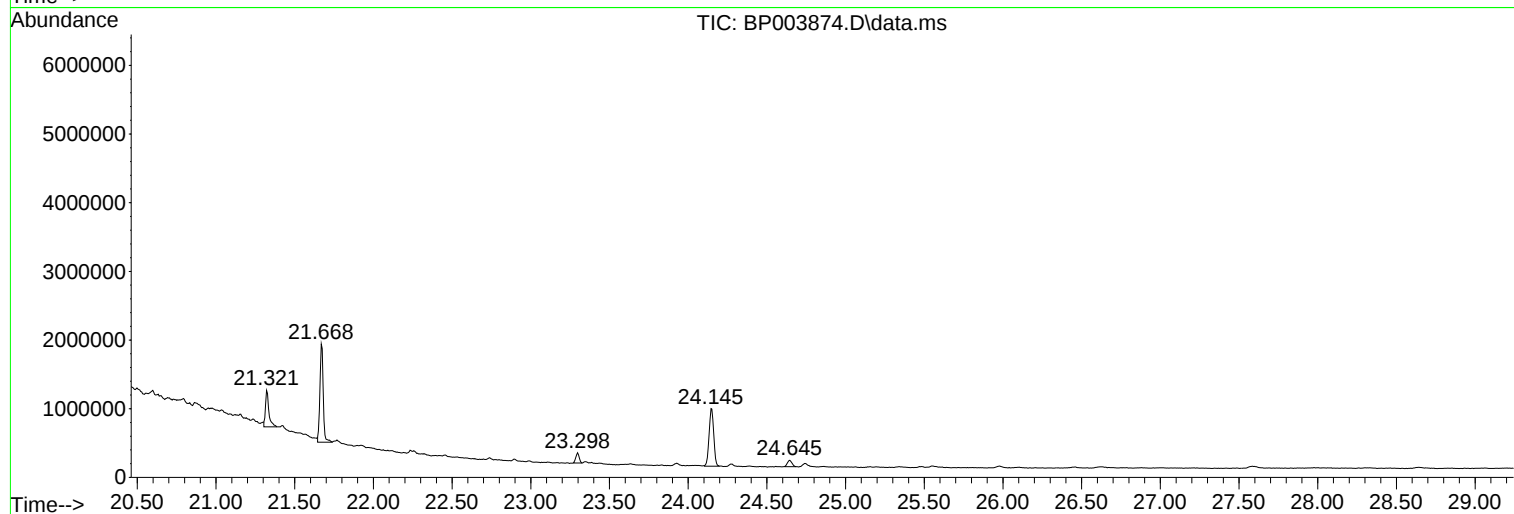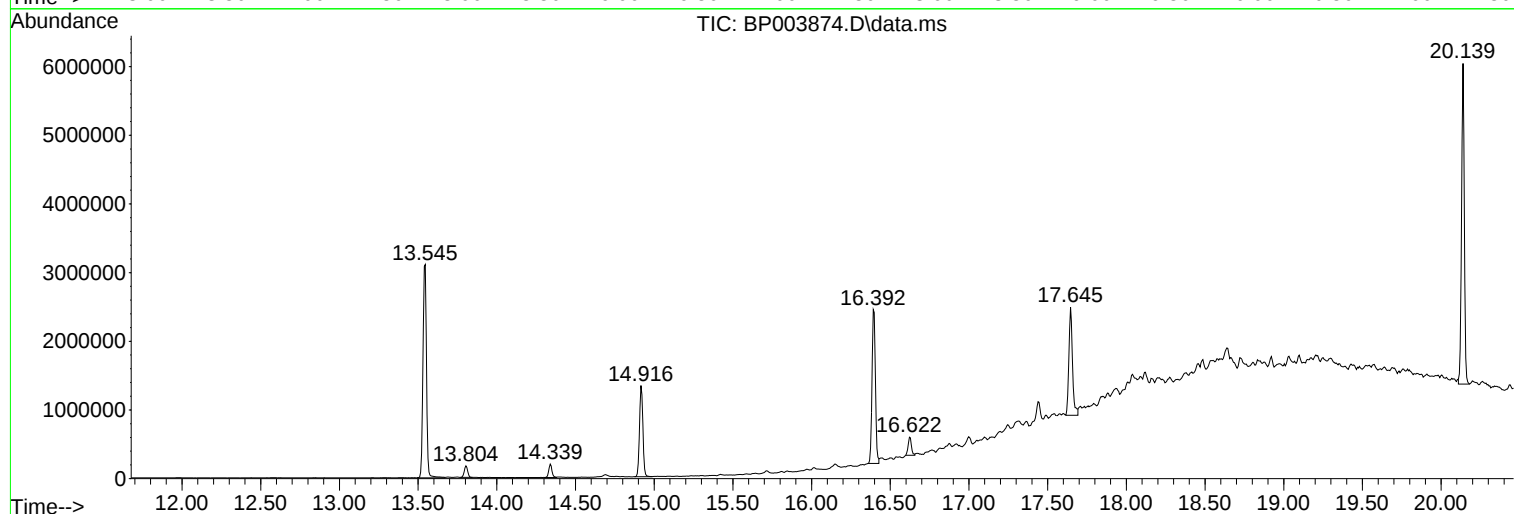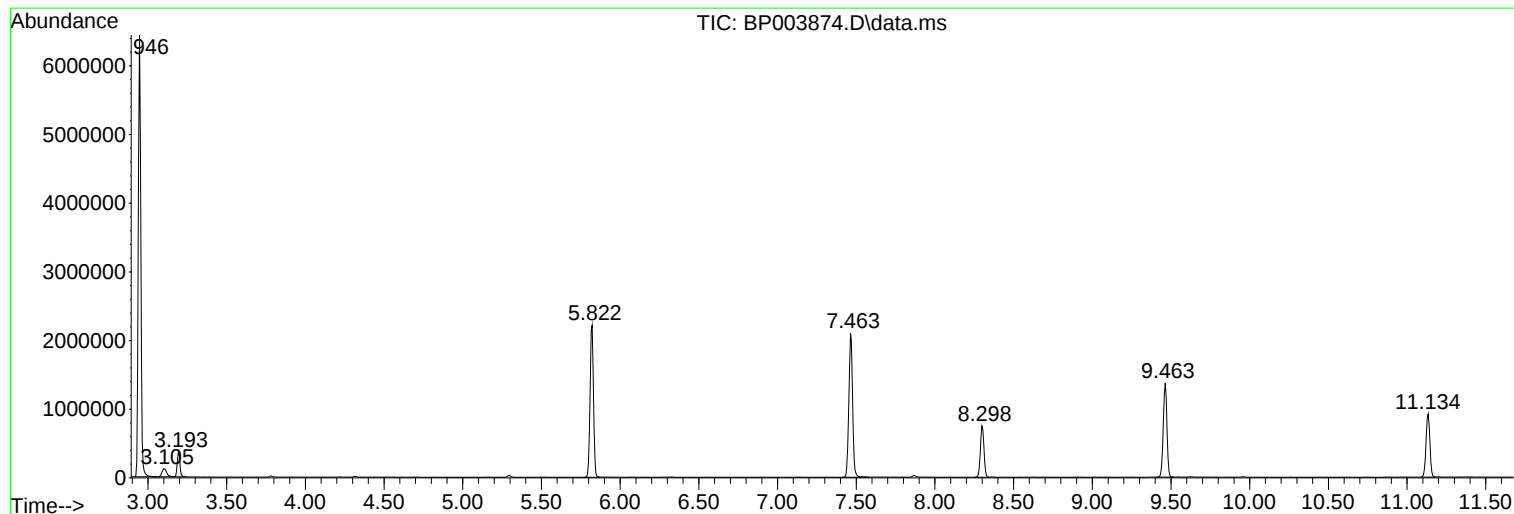

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003874.D
Acq On : 09 Nov 2020 18:31
Operator : CG/JU
Sample : L4658-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
361-OS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003874.D
Acq On : 09 Nov 2020 18:31
Operator : CG/JU
Sample : L4658-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
361-OS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
