

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
 Data File : BP003877.D
 Acq On : 09 Nov 2020 20:13
 Operator : CG/JU
 Sample : L4589-01 2X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CL-02-110620

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.952	6	11	30	rVB	2736361	3736259	17.90%	1.729%
2	3.105	31	37	48	rVV	117880	263558	1.26%	0.122%
3	3.199	48	53	65	rVB	157181	227919	1.09%	0.105%
4	5.822	492	499	508	rBV	1164888	1760950	8.44%	0.815%
5	7.469	771	779	792	rBV	1138629	1830715	8.77%	0.847%
6	8.305	914	921	929	rBV	1006618	1598752	7.66%	0.740%
7	9.463	1108	1118	1129	rBV	651403	1108925	5.31%	0.513%
8	11.140	1394	1403	1407	rBV	1233506	2102352	10.07%	0.973%
9	11.187	1407	1411	1419	rVB	560706	917119	4.39%	0.424%
10	12.769	1674	1680	1687	rVB	449261	669225	3.21%	0.310%
11	12.987	1708	1717	1724	rVB	291756	458294	2.20%	0.212%
12	13.546	1805	1812	1820	rBV	1620428	2290327	10.97%	1.060%
13	13.751	1841	1847	1852	rBV	133977	212862	1.02%	0.099%
14	14.245	1925	1931	1936	rBV	245901	413951	1.98%	0.192%
15	14.645	1990	1999	2005	rBV	583216	986484	4.73%	0.457%
16	14.922	2041	2046	2052	rVB	1580572	2293367	10.99%	1.061%
17	14.987	2052	2057	2062	rVB	675784	984814	4.72%	0.456%
18	15.310	2106	2112	2119	rVB	681540	993982	4.76%	0.460%
19	15.957	2216	2222	2229	rBV	1266960	1872078	8.97%	0.866%
20	16.251	2267	2272	2277	rVB	267801	371551	1.78%	0.172%
21	16.398	2288	2297	2304	rBV	1250169	1972498	9.45%	0.913%
22	16.622	2327	2335	2346	rBV3	179948	406663	1.95%	0.188%
23	16.957	2384	2392	2397	rBV2	268051	517275	2.48%	0.239%
24	17.004	2397	2400	2406	rVB2	145774	212451	1.02%	0.098%
25	17.104	2413	2417	2422	rVB4	125146	211305	1.01%	0.098%
26	17.186	2423	2431	2434	rBV2	182387	350527	1.68%	0.162%
27	17.228	2434	2438	2445	rVV2	193689	377033	1.81%	0.174%
28	17.298	2445	2450	2459	rVB2	208138	388087	1.86%	0.180%
29	17.381	2459	2464	2470	rBV2	197917	339885	1.63%	0.157%
30	17.469	2475	2479	2488	rVB	413421	602089	2.88%	0.279%
31	17.651	2504	2510	2513	rBV	1531304	2278397	10.91%	1.054%
32	17.698	2513	2518	2523	rVV	7796686	10980445	52.60%	5.081%
33	17.781	2523	2532	2537	rVV	2955318	4175001	20.00%	1.932%
34	17.834	2537	2541	2547	rVB3	195954	339207	1.62%	0.157%
35	18.028	2570	2574	2579	rVB	435833	612849	2.94%	0.284%
36	18.145	2591	2594	2598	rVB	233534	299086	1.43%	0.138%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
 Data File : BP003877.D
 Acq On : 09 Nov 2020 20:13
 Operator : CG/JU
 Sample : L4589-01 2X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CL-02-110620

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.216	2603	2606	2610	rVB2	184808	211669	1.01%	0.098%
38	18.498	2649	2654	2658	rBV	1098528	1503658	7.20%	0.696%
39	18.545	2658	2662	2667	rVB	1592568	2096855	10.04%	0.970%
40	18.616	2669	2674	2680	rBV	733217	1088941	5.22%	0.504%
41	18.692	2680	2687	2696	rBV2	2208372	4621308	22.14%	2.139%
42	18.963	2728	2733	2736	rBV	954329	1248407	5.98%	0.578%
43	18.998	2736	2739	2744	rVB	411820	523186	2.51%	0.242%
44	19.204	2770	2774	2777	rVB	236152	293361	1.41%	0.136%
45	19.251	2779	2782	2785	rVV	285320	334368	1.60%	0.155%
46	19.286	2785	2788	2792	rVB	260288	326351	1.56%	0.151%
47	19.369	2797	2802	2807	rBV2	602343	1097781	5.26%	0.508%
48	19.504	2821	2825	2837	rBV	818357	1319510	6.32%	0.611%
49	19.633	2839	2847	2851	rBV	14256906	20874650	100.00%	9.660%
50	19.710	2857	2860	2865	rVB3	329256	440075	2.11%	0.204%
51	19.769	2866	2870	2872	rBV2	269127	356879	1.71%	0.165%
52	19.863	2882	2886	2895	rVB2	452120	784057	3.76%	0.363%
53	19.945	2895	2900	2901	rBV	2353425	3055550	14.64%	1.414%
54	19.980	2901	2906	2912	rVV	11811028	17674576	84.67%	8.179%
55	20.033	2912	2915	2921	rVB2	597357	844711	4.05%	0.391%
56	20.139	2929	2933	2938	rVB2	2427220	3107032	14.88%	1.438%
57	20.198	2939	2943	2950	rVB	448082	679043	3.25%	0.314%
58	20.286	2951	2958	2962	rBV3	936738	2272466	10.89%	1.052%
59	20.445	2976	2985	2989	rVB	2311774	4027874	19.30%	1.864%
60	20.539	2997	3001	3005	rBV	1736067	2138520	10.24%	0.990%
61	20.598	3005	3011	3015	rVB2	1211570	1934483	9.27%	0.895%
62	20.733	3031	3034	3038	rBV	629943	878454	4.21%	0.407%
63	20.775	3038	3041	3048	rVB	747851	1064994	5.10%	0.493%
64	21.163	3103	3107	3113	rVB	1254063	1697462	8.13%	0.786%
65	21.327	3128	3135	3137	rBV2	1359446	2484394	11.90%	1.150%
66	21.357	3137	3140	3144	rVV	1329988	1869158	8.95%	0.865%
67	21.404	3144	3148	3152	rVV	1771114	2502740	11.99%	1.158%
68	21.445	3152	3155	3165	rVB2	1404453	2099514	10.06%	0.972%
69	21.669	3188	3193	3198	rBV2	8424843	13921516	66.69%	6.443%
70	21.727	3198	3203	3211	rVB	6340867	9773543	46.82%	4.523%
71	21.851	3220	3224	3228	rBV	1564059	2367376	11.34%	1.096%
72	21.898	3229	3232	3236	rVB2	511974	755605	3.62%	0.350%
73	22.010	3247	3251	3256	rBV2	867093	1591561	7.62%	0.737%
74	22.269	3290	3295	3300	rVB	1106630	1862283	8.92%	0.862%
75	22.498	3330	3334	3337	rBV3	632012	944782	4.53%	0.437%
76	23.421	3483	3491	3496	rBV	4899119	13279207	63.61%	6.145%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003877.D
Acq On : 09 Nov 2020 20:13
Operator : CG/JU
Sample : L4589-01 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-110620

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	23.604	3518	3522	3529	rVB	1313395	2316092	11.10%	1.072%
78	23.957	3576	3582	3592	rVB	3114594	6725415	32.22%	3.112%
79	24.068	3593	3601	3608	rVV	4826167	9891904	47.39%	4.578%
80	24.168	3614	3618	3623	rBV	761473	1509531	7.23%	0.699%
81	24.227	3623	3628	3635	rVB2	1478468	3121110	14.95%	1.444%
82	26.751	4047	4057	4065	rVB2	2289435	7534485	36.09%	3.487%
83	27.545	4184	4192	4210	rVB	1632269	5884241	28.19%	2.723%




Sum of corrected areas: 216086960

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003877.D
Acq On : 09 Nov 2020 20:13
Operator : CG/JU
Sample : L4589-01 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-110620

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

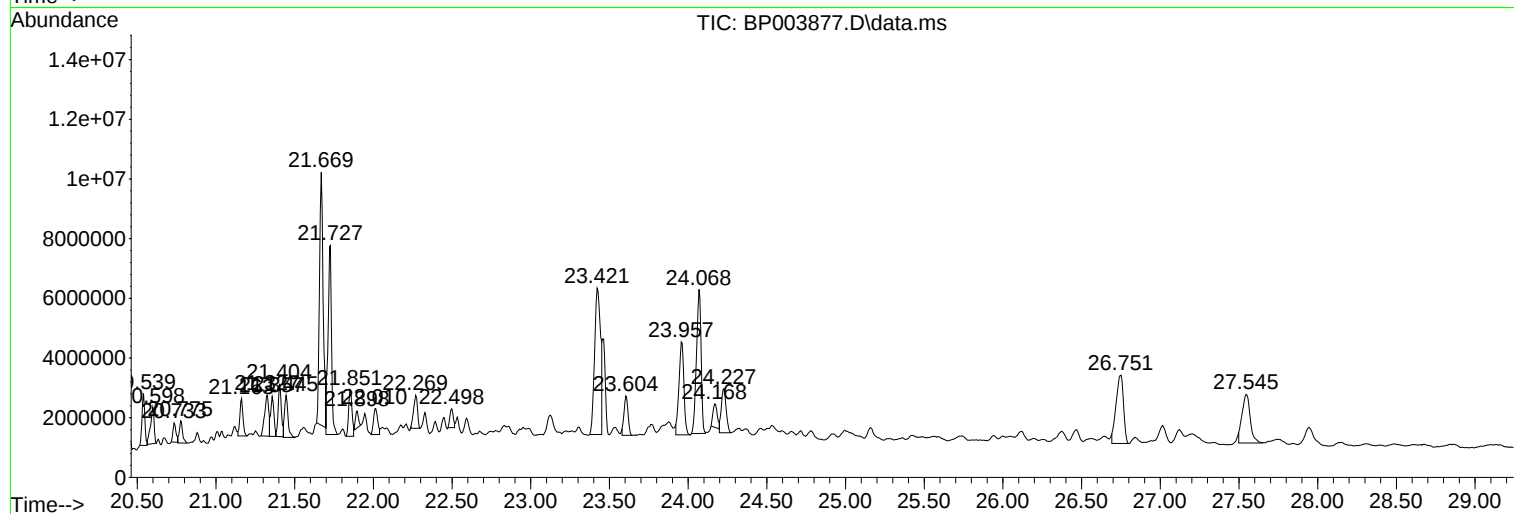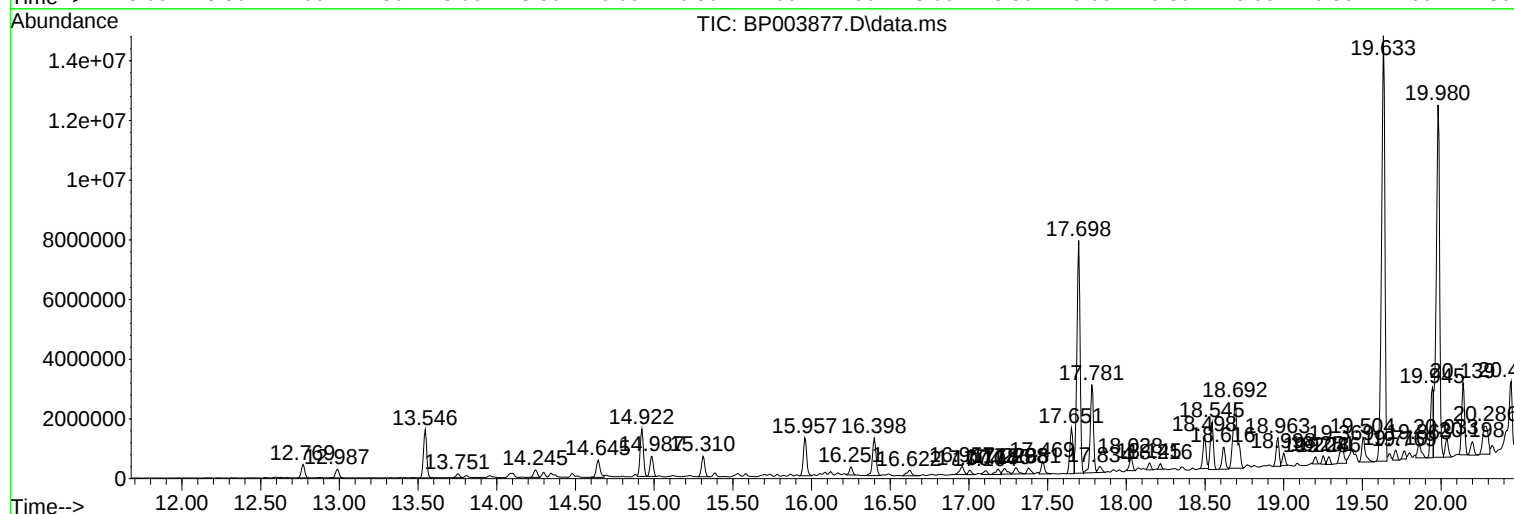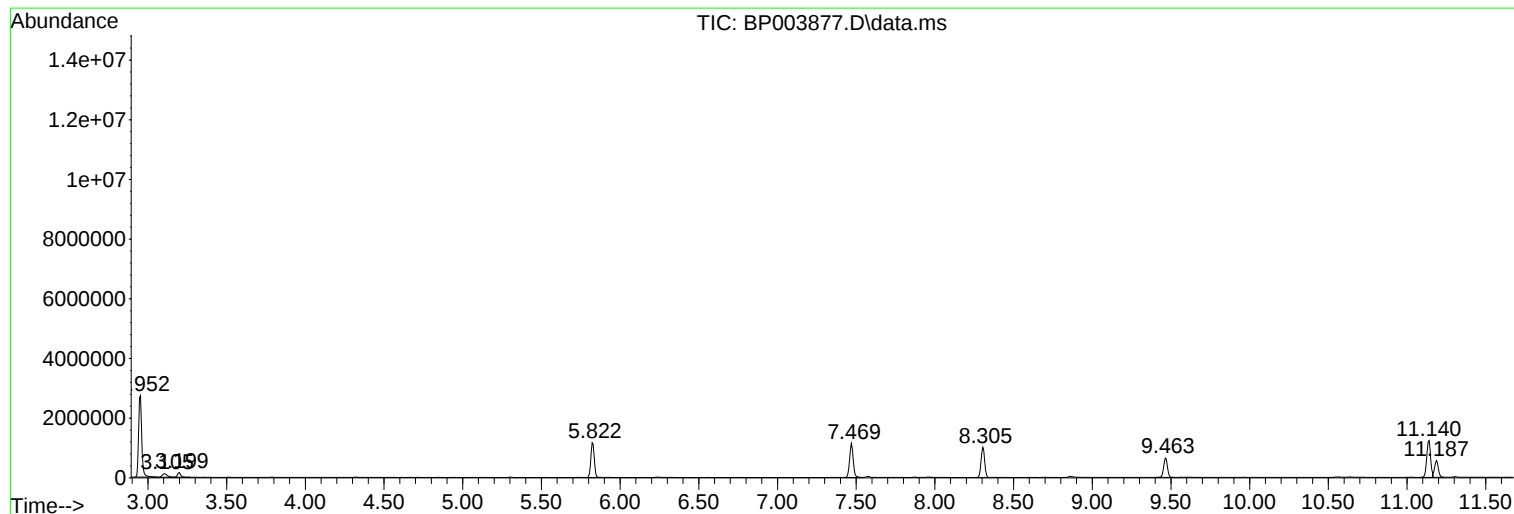

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003877.D
Acq On : 09 Nov 2020 20:13
Operator : CG/JU
Sample : L4589-01 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-110620

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
Data File : BP003877.D
Acq On : 09 Nov 2020 20:13
Operator : CG/JU
Sample : L4589-01 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-110620

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc