
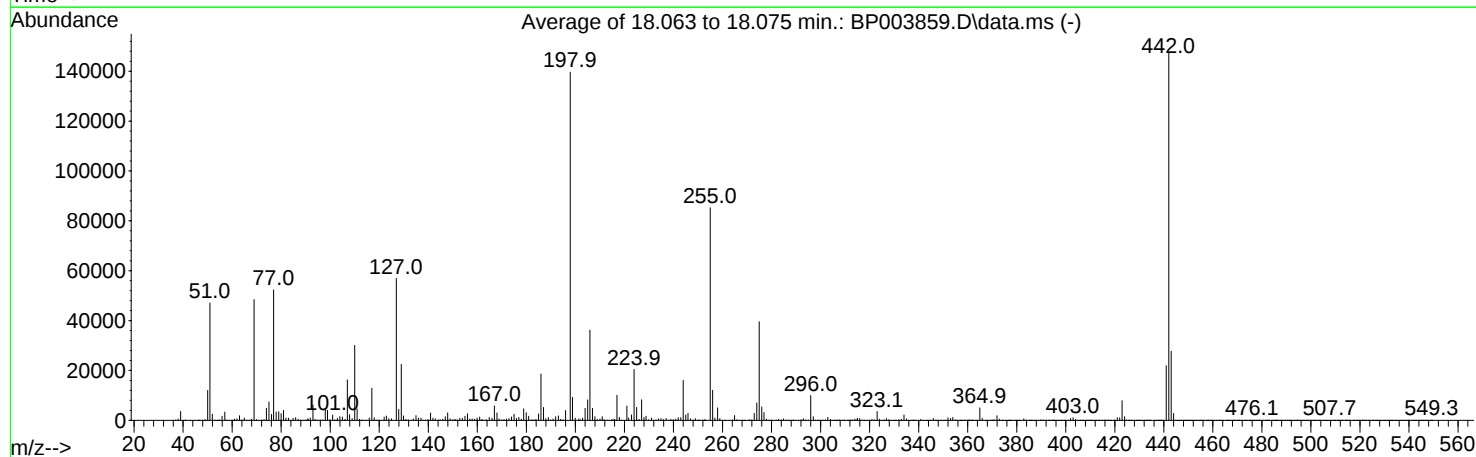


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110920\
 Data File : BP003859.D
 Acq On : 09 Nov 2020 09:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 10 13:41:24 2020

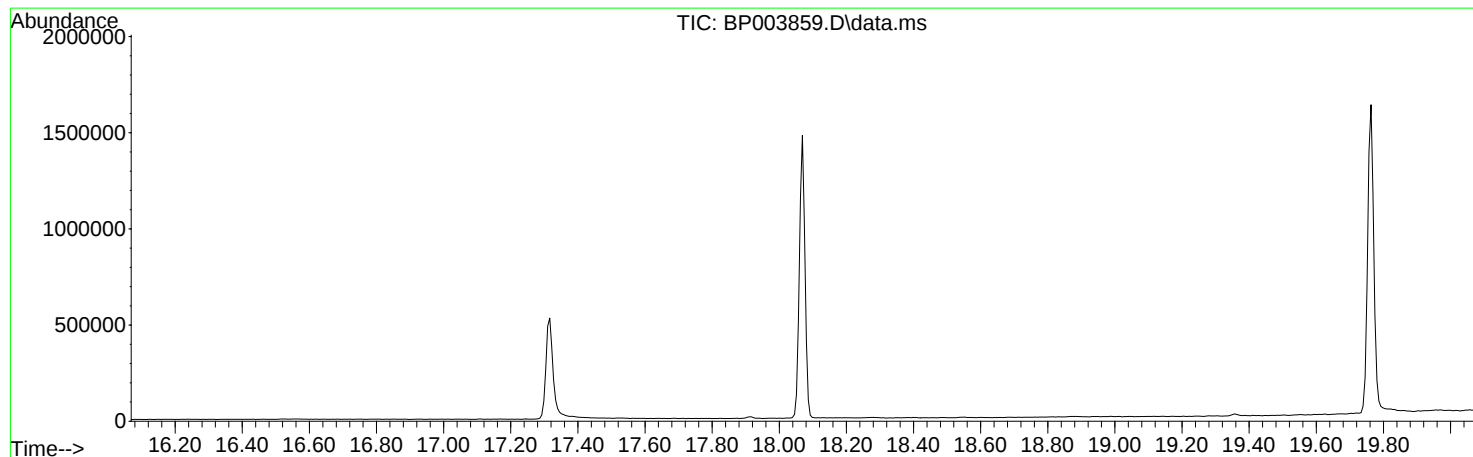

AutoFind: Scans 2580, 2581, 2582; Background Corrected with Scan 2572

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	47093	PASS
68	69	0.00	2	1.0	507	PASS
69	198	0.00	100	34.7	48433	PASS
70	69	0.00	2	0.6	304	PASS
127	198	10	80	40.7	56893	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	139645	PASS
199	198	5	9	6.6	9265	PASS
275	198	10	60	28.3	39571	PASS
365	198	1	100	3.6	4985	PASS
441	198	0.01	100	15.7	21973	PASS
442	442	100	100	100.0	147509	PASS
443	442	15	24	18.8	27725	PASS