
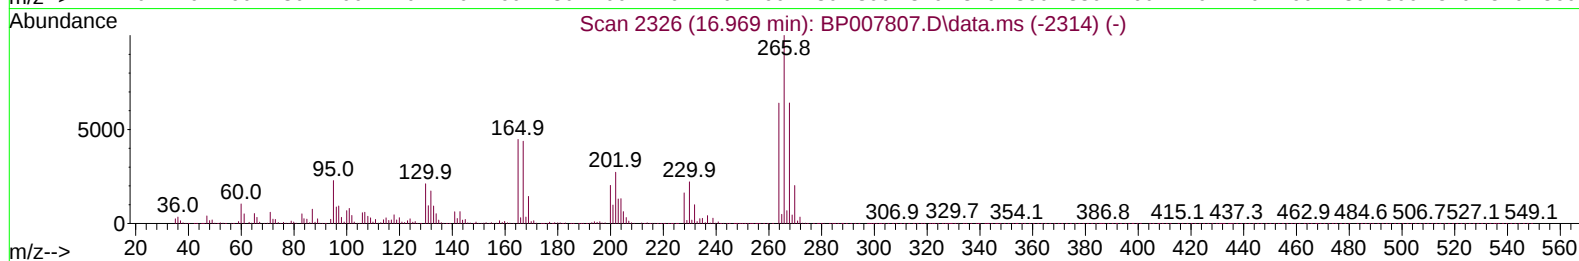
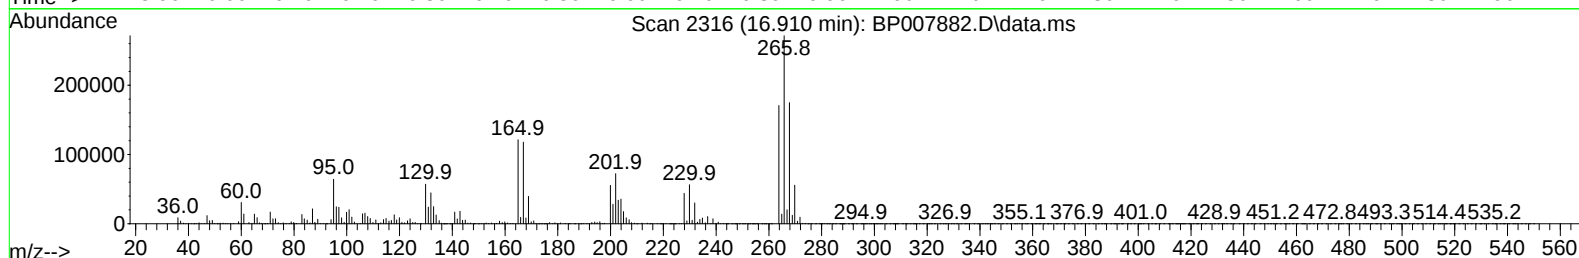


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
 Data File : BP007882.D
 Acq On : 09 Nov 2021 09:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 10:30:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 08 16:36:40 2021
 Response via : Initial Calibration

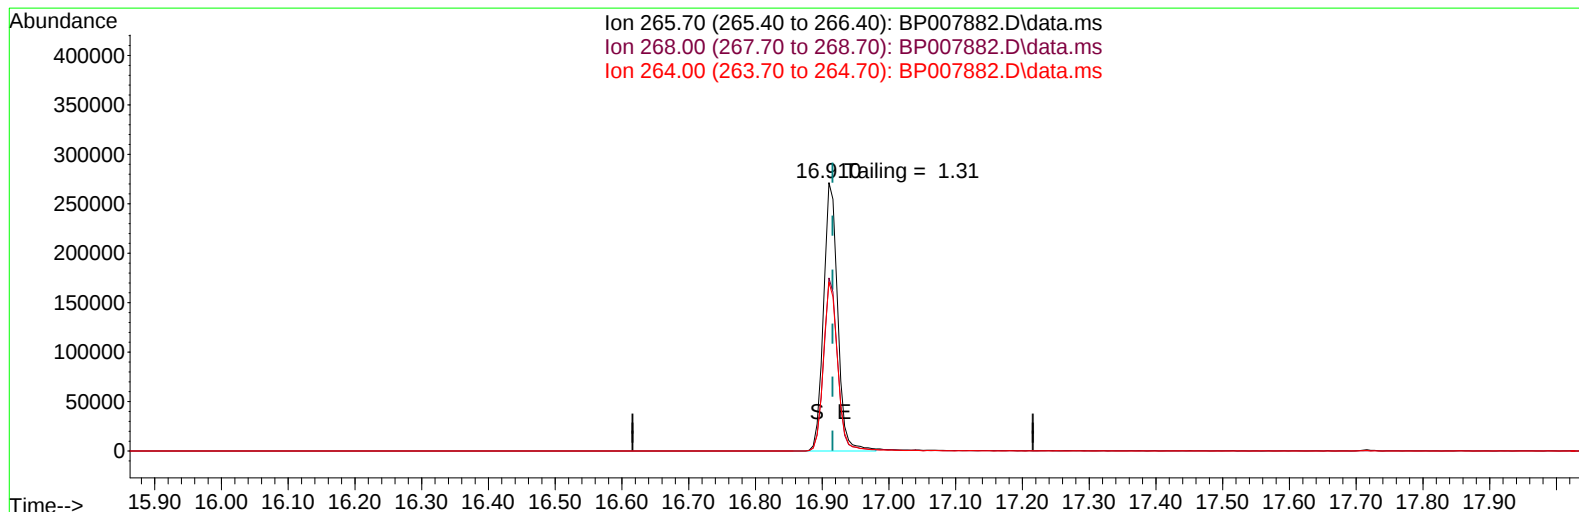

TIC: BP007882.D\data.ms

(70) Pentachlorophenol (C)




16.910min (-0.006) 767408.37 ng

response 402415

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	64.47
264.00	60.90	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
Data File : BP007882.D
Acq On : 09 Nov 2021 09:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 10:30:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 08 16:36:40 2021
Response via : Initial Calibration

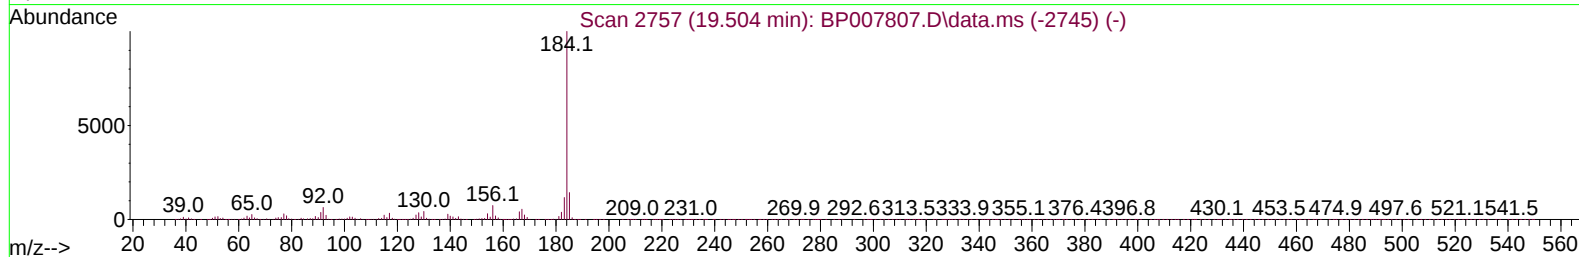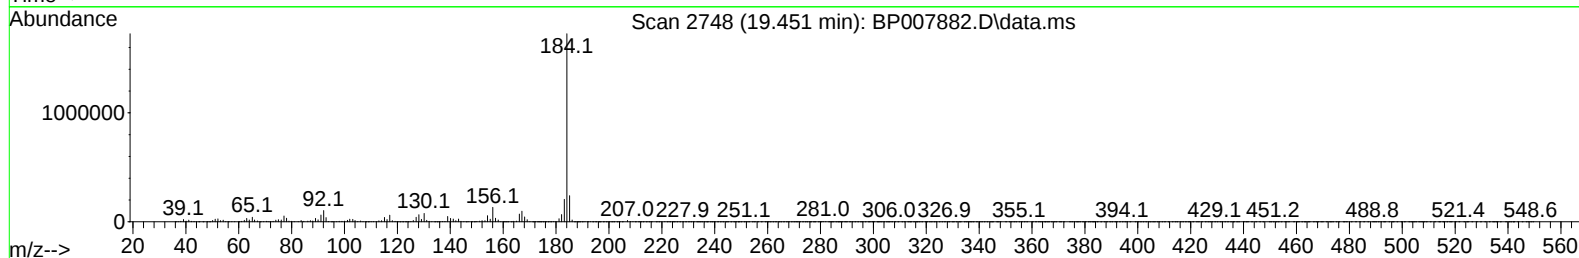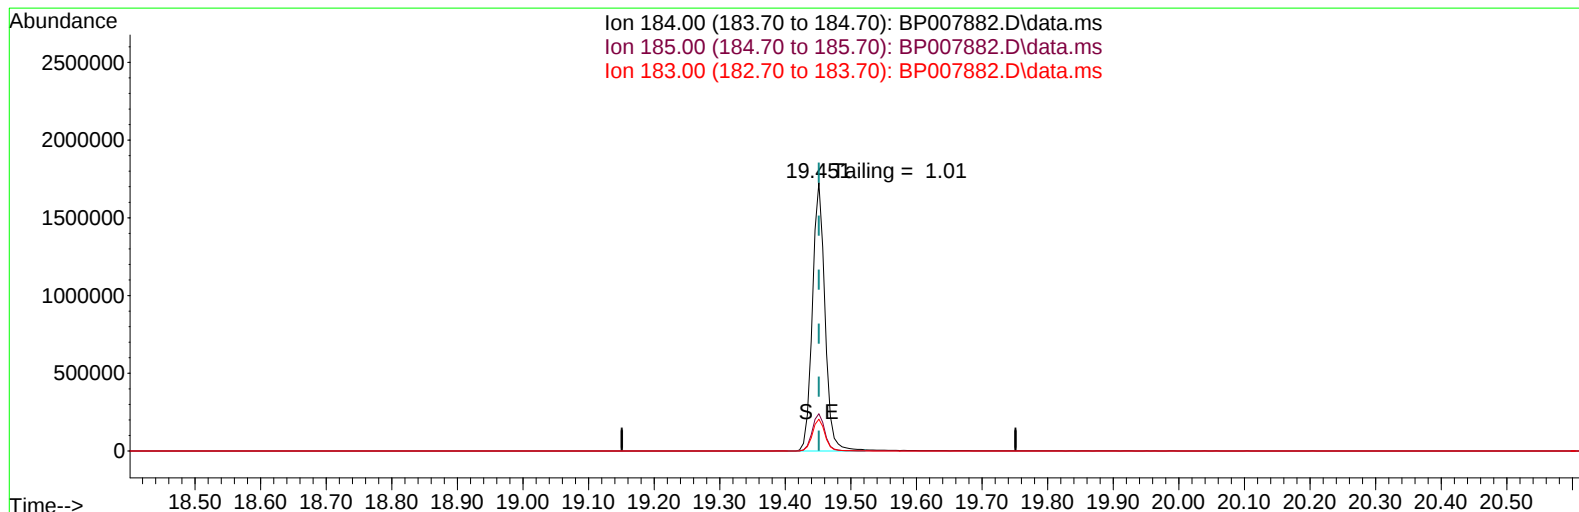

TIC: BP007882.D\data.ms

(77) Benzidine**19.451min (+ 0.000) 871503.86 ng****response 2328230**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.90
183.00	11.40	11.91
0.00	0.00	0.00