
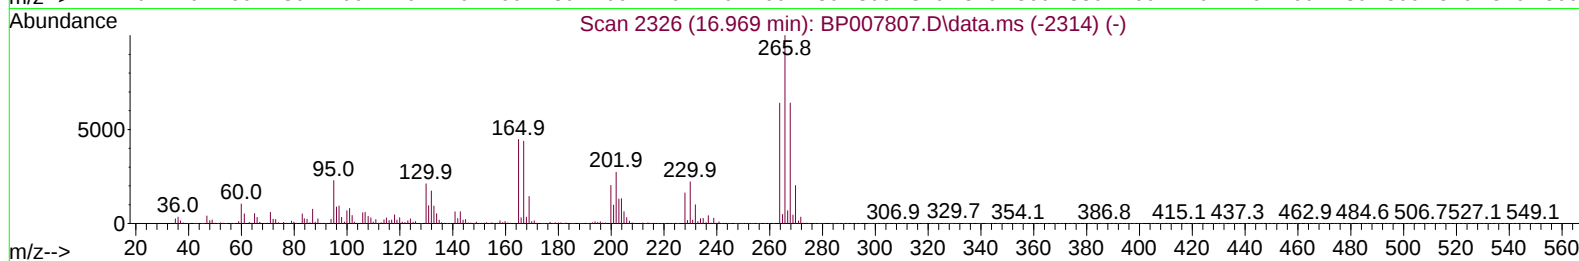
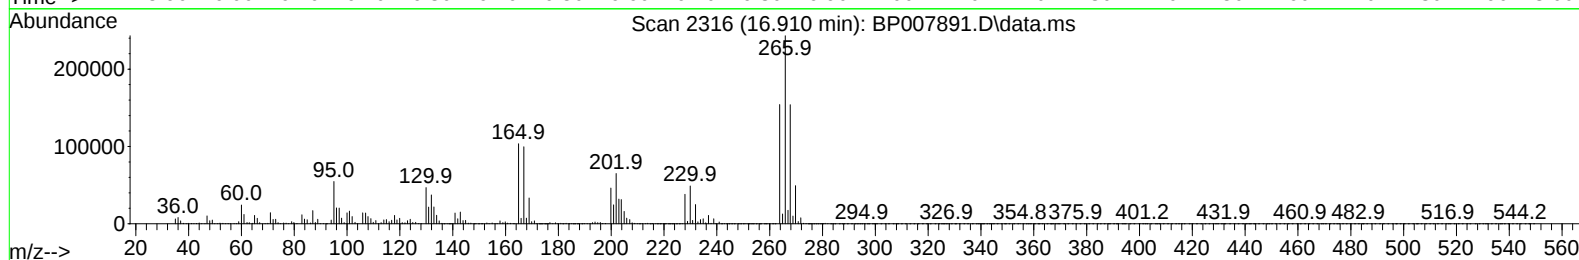


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
Data File : BP007891.D
Acq On : 09 Nov 2021 14:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 15:36:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 10:45:24 2021
Response via : Initial Calibration

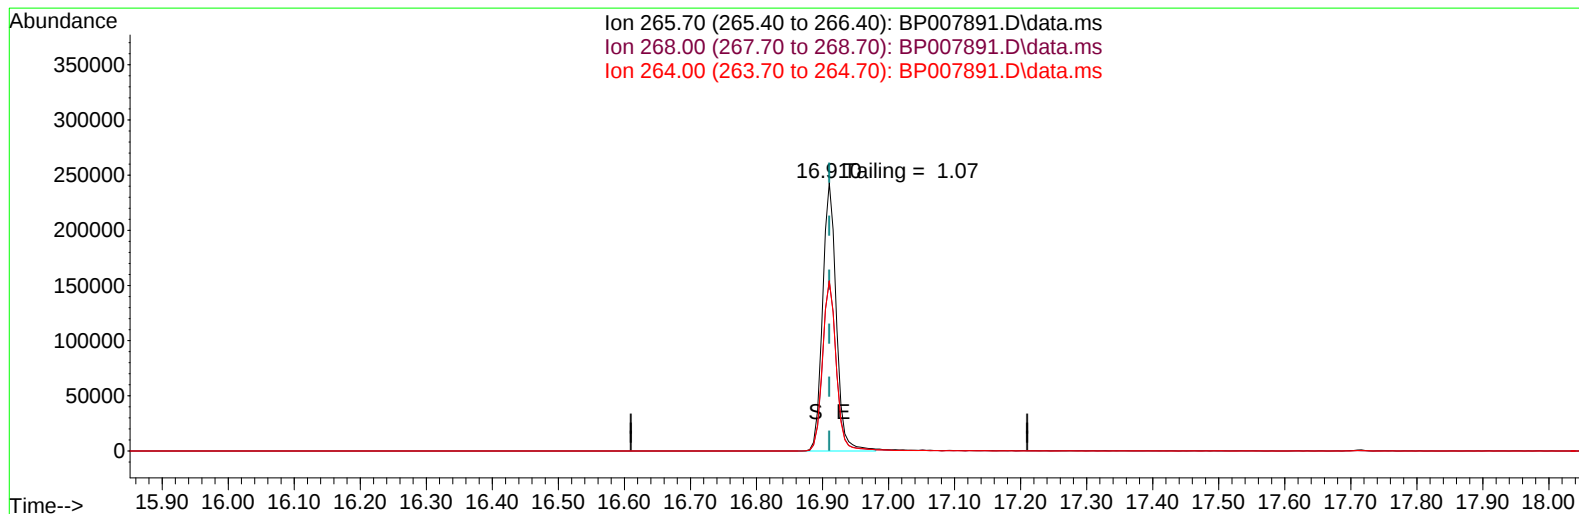

TIC: BP007891.D\data.ms

(70) Pentachlorophenol (C)




16.910min (+ 0.000) 580329.04 ng

response 355033

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	63.29
264.00	60.90	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
 Data File : BP007891.D
 Acq On : 09 Nov 2021 14:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 15:36:58 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 10:45:24 2021
 Response via : Initial Calibration

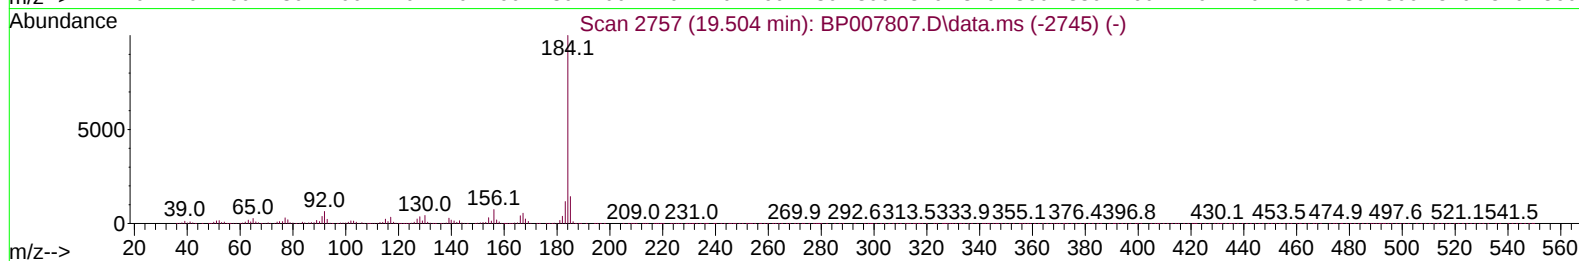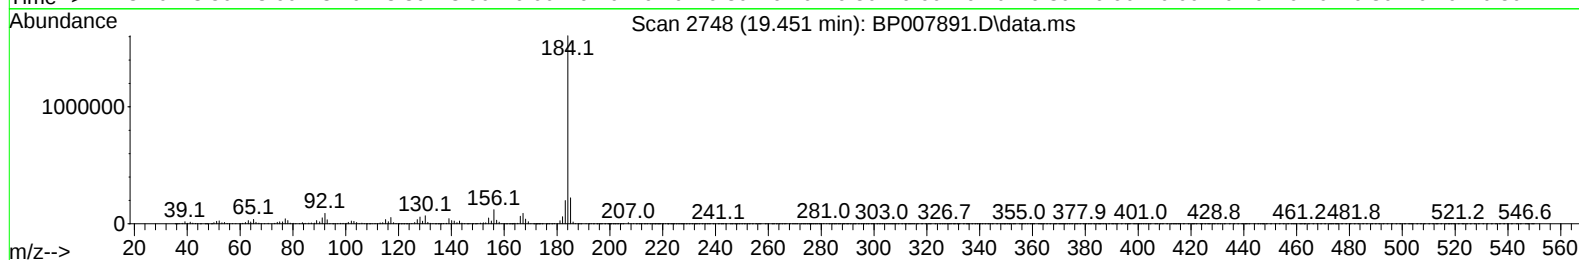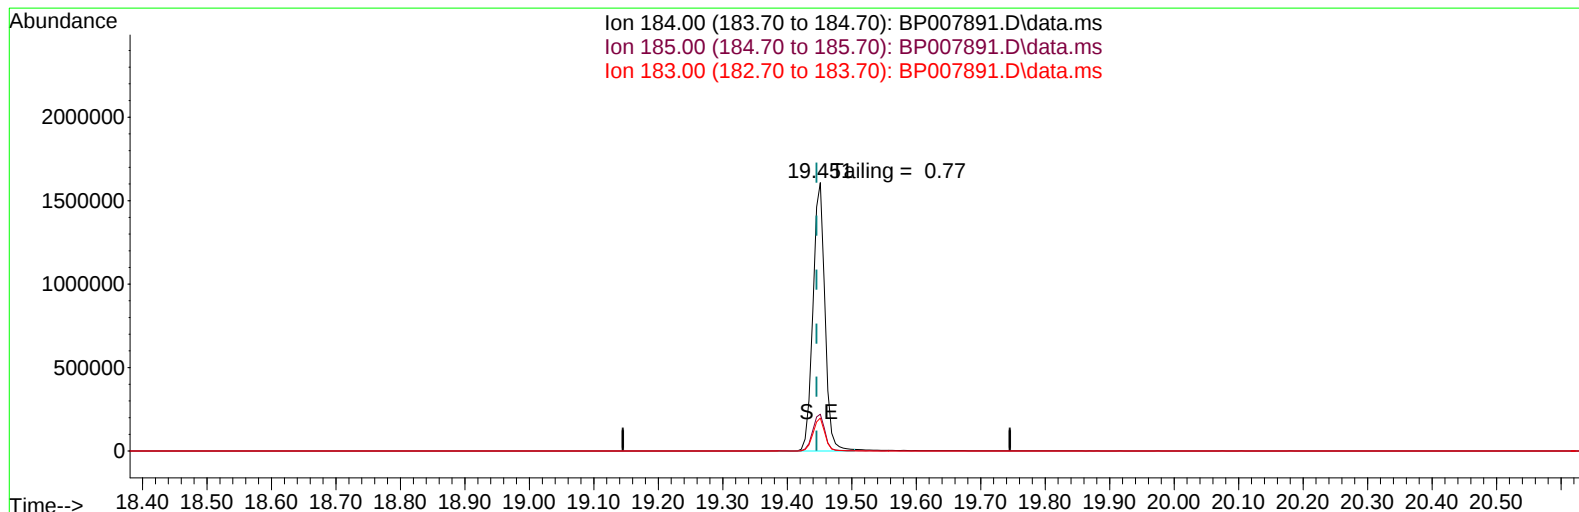

TIC: BP007891.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 760902.73 ng

response 2109466

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.76
183.00	11.40	12.31
0.00	0.00	0.00