

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
 Data File : BP007884.D
 Acq On : 09 Nov 2021 10:41
 Operator : CG/JU
 Sample : PB140520BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB140520BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	361	368	378	rBV	2840732	4171103	34.12%	8.671%
2	7.046	630	639	653	rBV	2564348	4029189	32.95%	8.376%
3	7.869	771	779	788	rBV	537015	850641	6.96%	1.768%
4	9.028	965	976	990	rBV	1491046	2537631	20.76%	5.275%
5	10.669	1246	1255	1265	rBV	684291	1181517	9.66%	2.456%
6	13.128	1665	1673	1683	rBV	4341878	6486835	53.06%	13.485%
7	14.504	1897	1907	1924	rBV	1189060	1766586	14.45%	3.672%
8	15.998	2154	2161	2175	rBV	3963445	5884932	48.13%	12.234%
9	17.257	2368	2375	2387	rBV	1640415	2352392	19.24%	4.890%
10	19.822	2805	2811	2821	rBV	9895361	12226417	100.00%	25.416%
11	21.351	3066	3071	3078	rBV	2408544	3135629	25.65%	6.518%
12	23.768	3475	3482	3491	rVB2	1677993	3481475	28.48%	7.237%




Sum of corrected areas: 48104347

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
Data File : BP007884.D
Acq On : 09 Nov 2021 10:41
Operator : CG/JU
Sample : PB140520BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140520BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

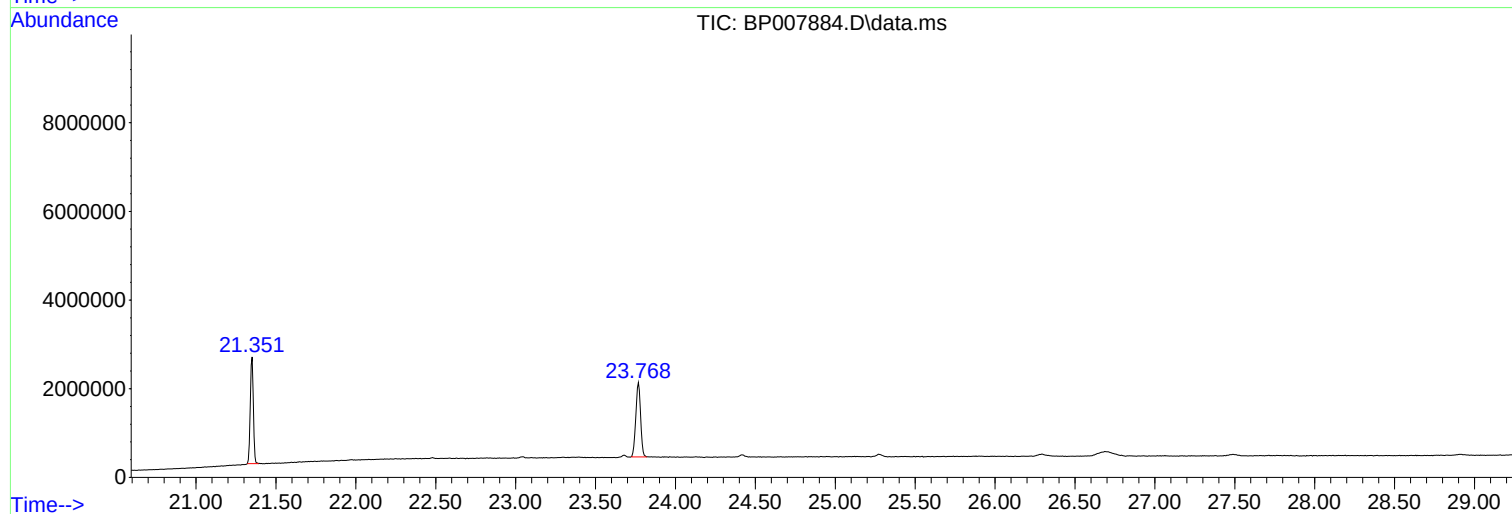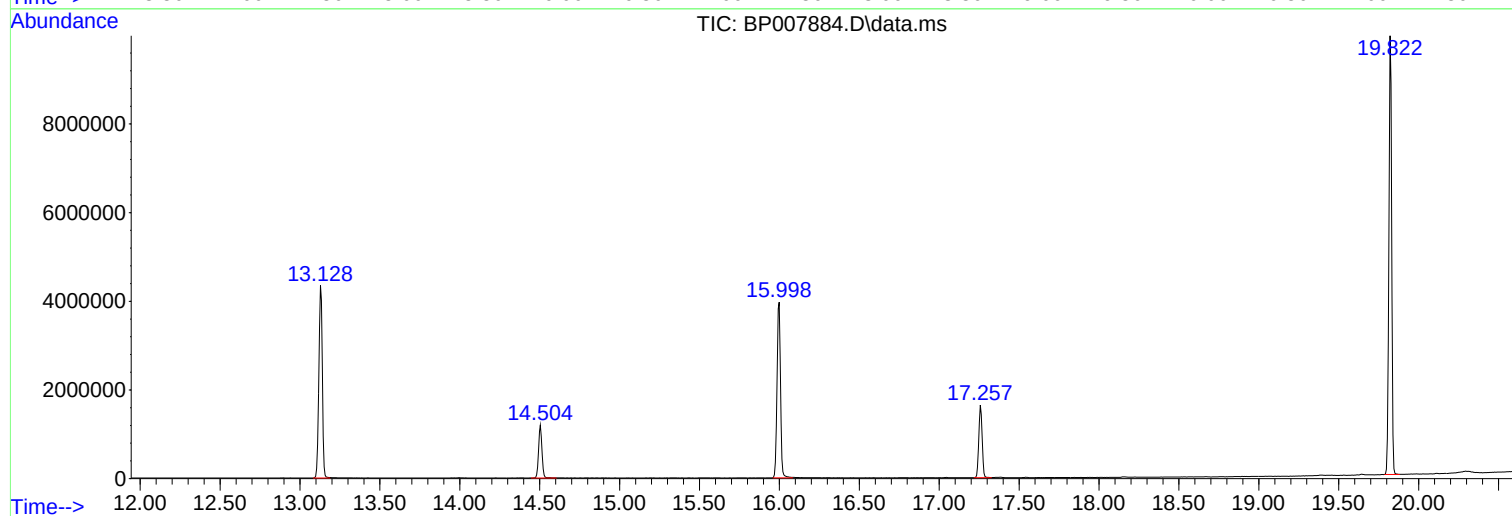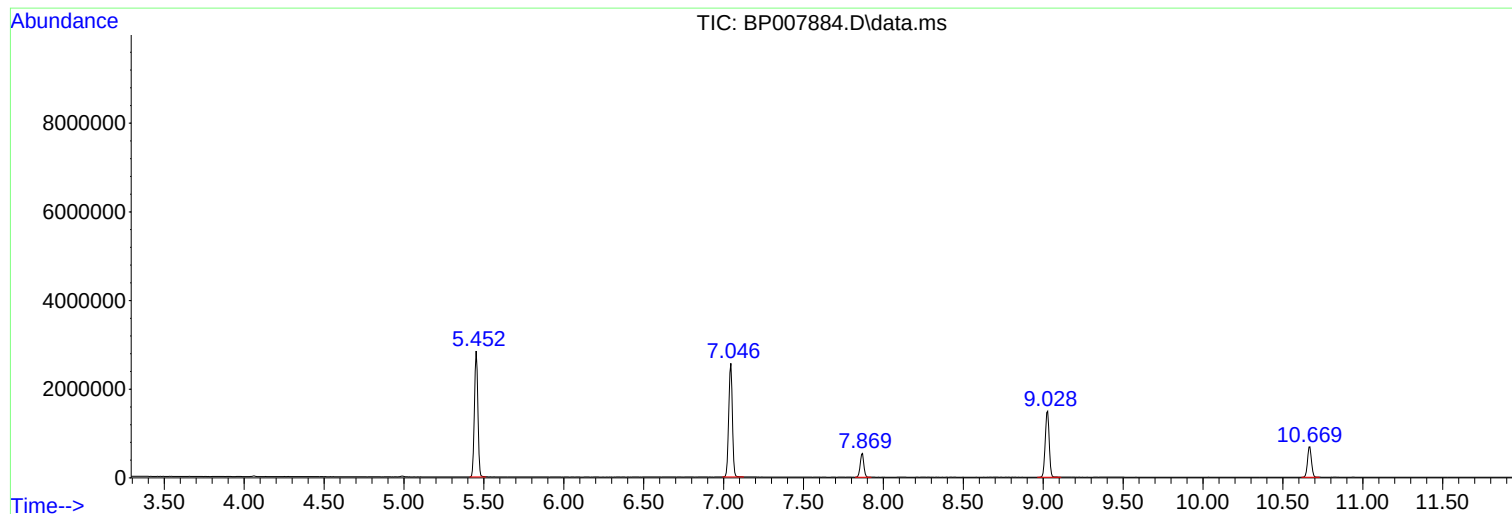

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
Data File : BP007884.D
Acq On : 09 Nov 2021 10:41
Operator : CG/JU
Sample : PB140520BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140520BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
Data File : BP007884.D
Acq On : 09 Nov 2021 10:41
Operator : CG/JU
Sample : PB140520BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140520BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------