

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
Data File : BP007893.D
Acq On : 09 Nov 2021 16:08
Operator : CG/JU
Sample : PB140580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140580BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	361	368	379	rBV	1982769	2926608	24.59%	7.038%
2	7.040	631	638	657	rBV	1955363	3138220	26.37%	7.547%
3	7.863	772	778	785	rBV	351547	557991	4.69%	1.342%
4	9.022	966	975	986	rBV	1087264	1792877	15.07%	4.311%
5	10.663	1244	1254	1264	rBV	495968	828308	6.96%	1.992%
6	13.128	1665	1673	1694	rBV	3486641	5122567	43.05%	12.318%
7	14.498	1898	1906	1920	rBV	906517	1409569	11.85%	3.390%
8	15.992	2152	2160	2181	rBV	3588066	5390298	45.30%	12.962%
9	17.257	2368	2375	2387	rBV	1460860	2116543	17.79%	5.090%
10	19.822	2805	2811	2816	rBV	9432524	11900022	100.00%	28.616%
11	21.345	3065	3070	3079	rBV	2356898	3087915	25.95%	7.426%
12	23.763	3474	3481	3490	rVB2	1597813	3313674	27.85%	7.969%




Sum of corrected areas: 41584592

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
Data File : BP007893.D
Acq On : 09 Nov 2021 16:08
Operator : CG/JU
Sample : PB140580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140580BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

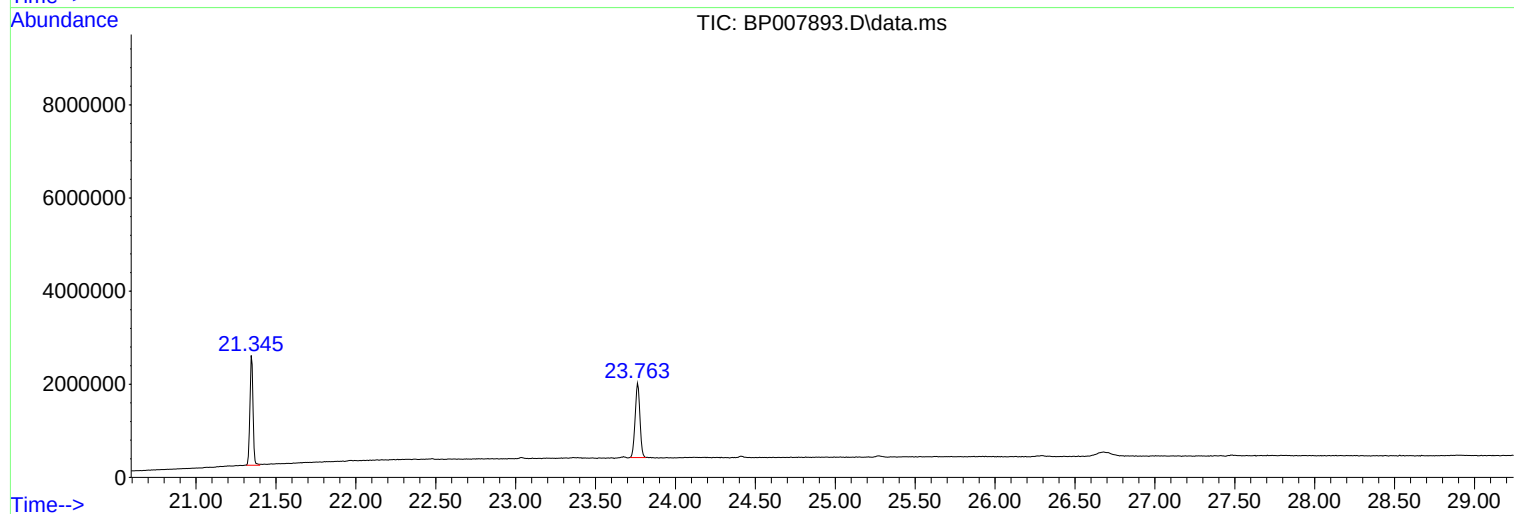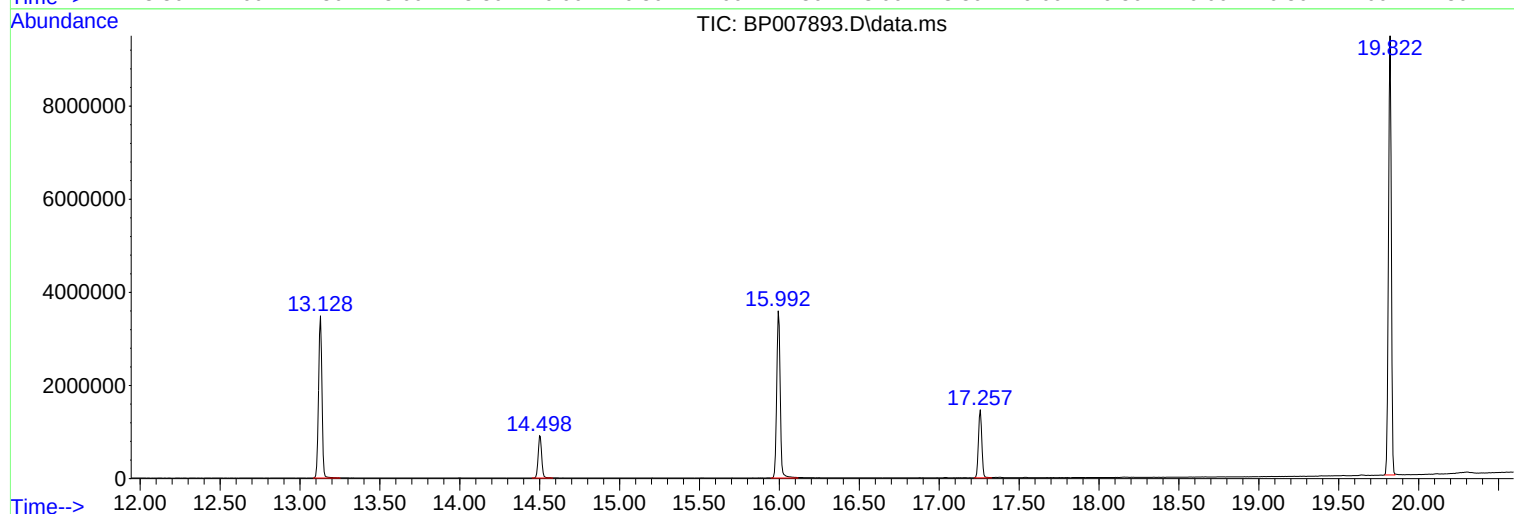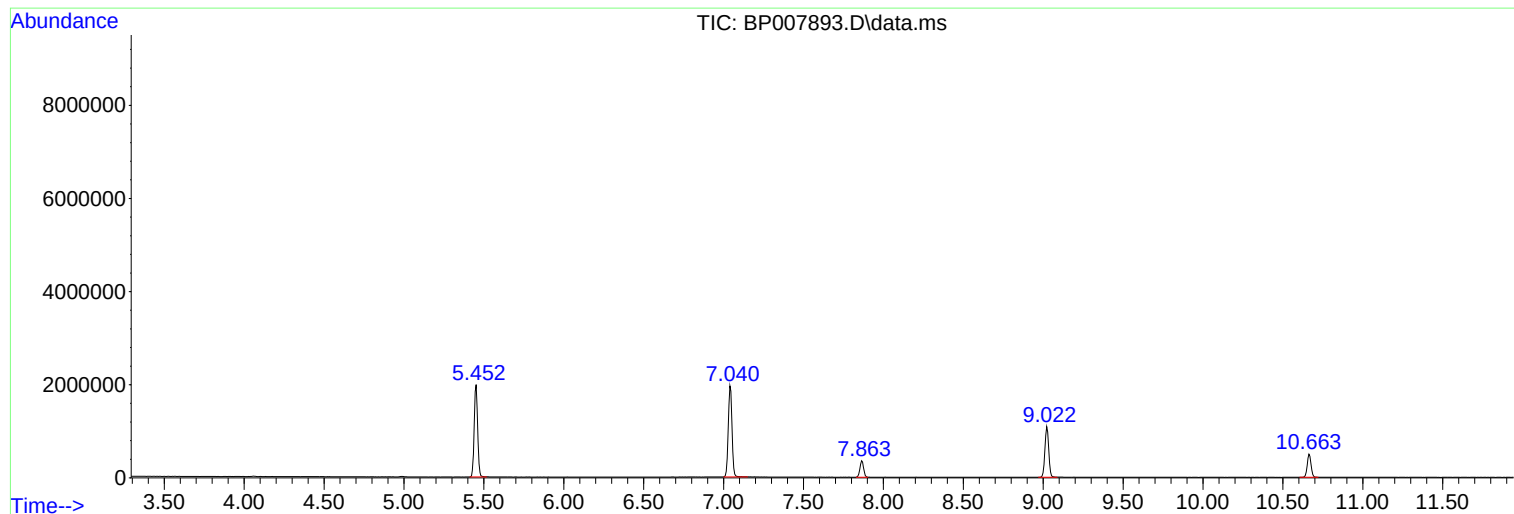

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
Data File : BP007893.D
Acq On : 09 Nov 2021 16:08
Operator : CG/JU
Sample : PB140580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140580BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
Data File : BP007893.D
Acq On : 09 Nov 2021 16:08
Operator : CG/JU
Sample : PB140580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140580BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------