
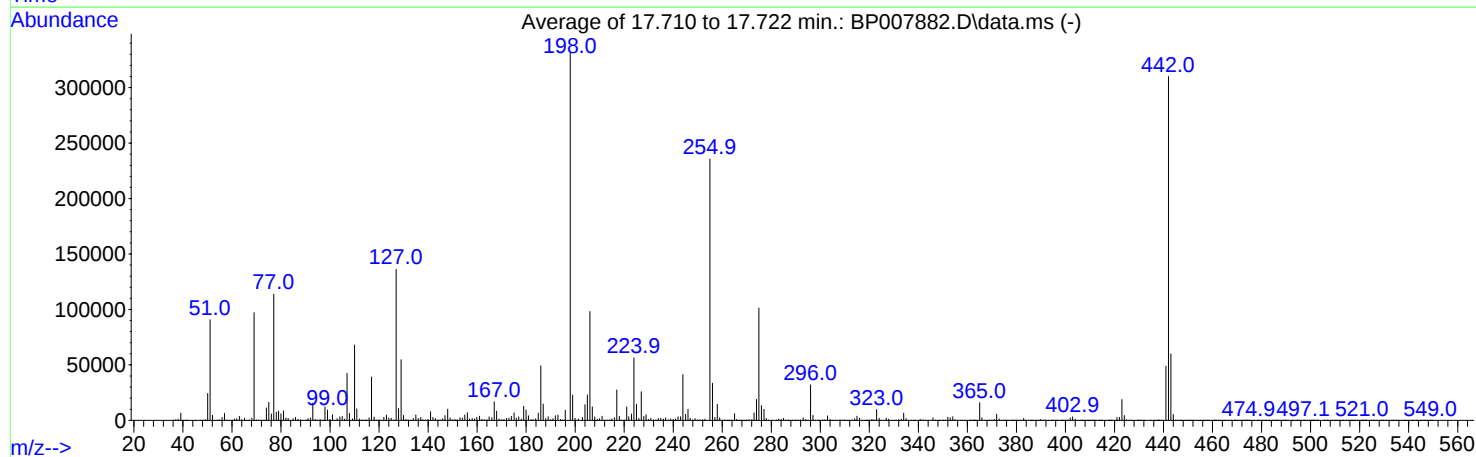


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
 Data File : BP007882.D
 Acq On : 09 Nov 2021 09:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 09 10:45:24 2021

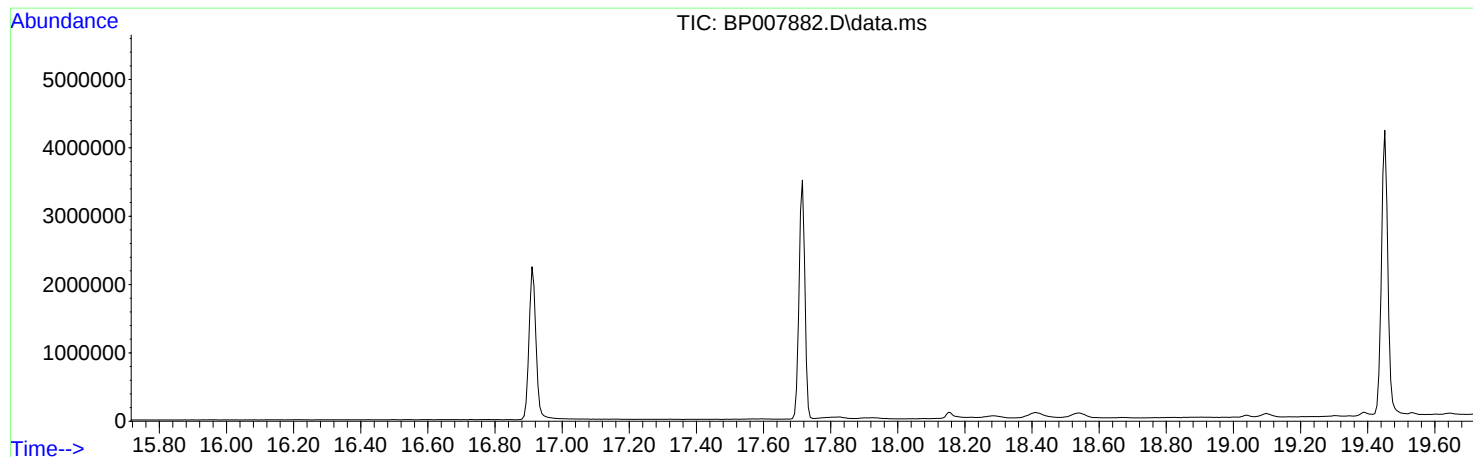




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	90728	PASS
68	69	0.00	2	2.0	1928	PASS
69	198	0.00	100	29.3	97160	PASS
70	69	0.00	2	0.5	506	PASS
127	198	10	80	41.1	136237	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	331633	PASS
199	198	5	9	6.8	22611	PASS
275	198	10	60	30.5	101290	PASS
365	198	1	100	4.8	15990	PASS
441	198	0.01	100	14.7	48915	PASS
442	442	100	100	100.0	309952	PASS
443	442	15	24	19.3	59964	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
 Data File : BP007882.D
 Acq On : 09 Nov 2021 09:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 09 10:30:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 08 16:36:40 2021
 Response via : Initial Calibration

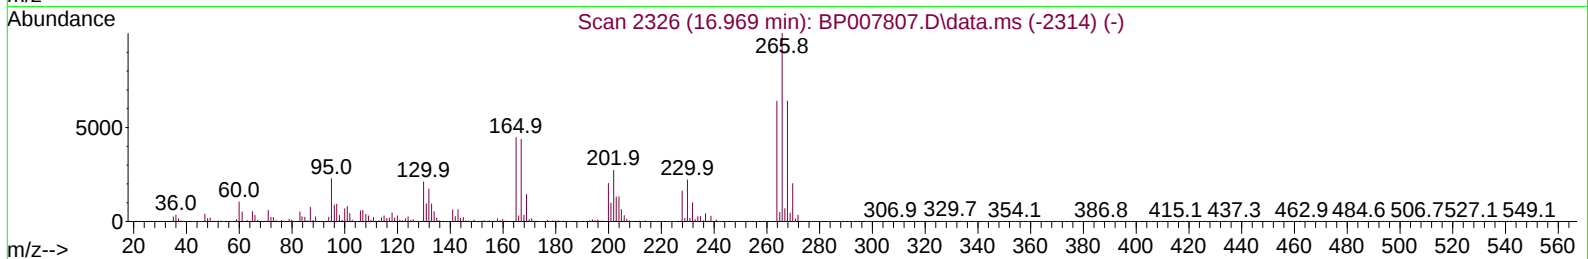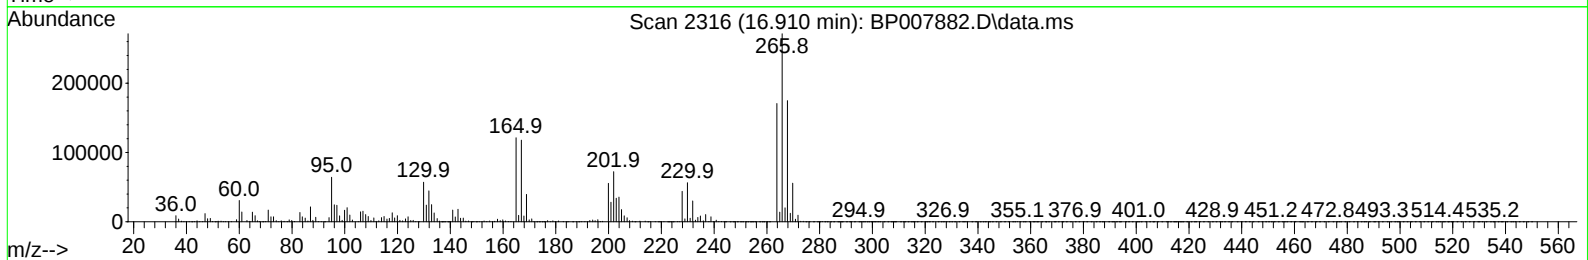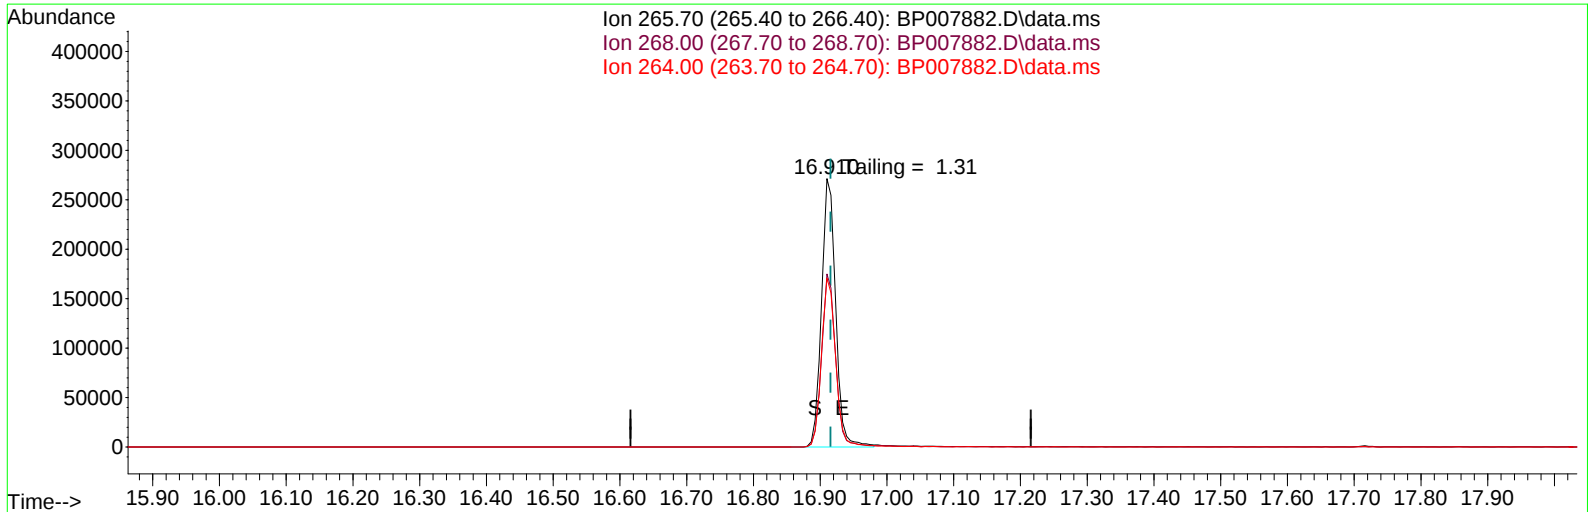

TIC: BP007882.D\data.ms

(70) Pentachlorophenol (C)

16.910min (-0.006) 767408.37 ng




response 402415

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	64.47
264.00	60.90	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
 Data File : BP007882.D
 Acq On : 09 Nov 2021 09:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 09 10:30:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 08 16:36:40 2021
 Response via : Initial Calibration

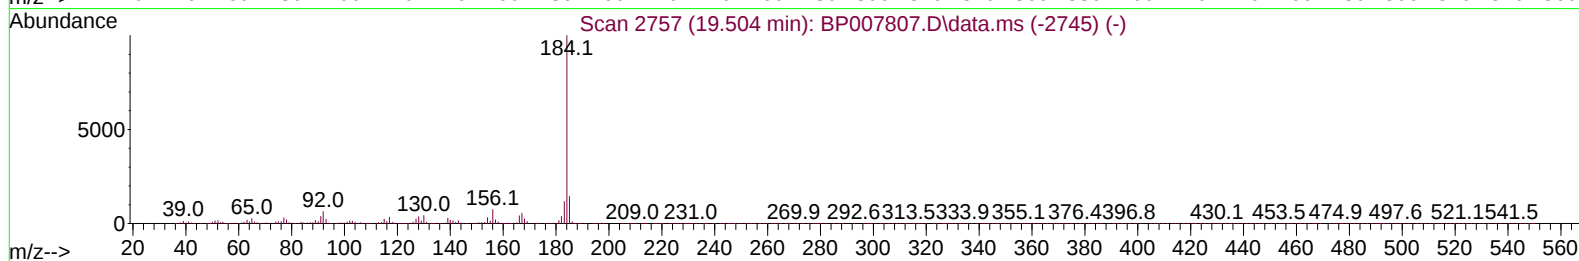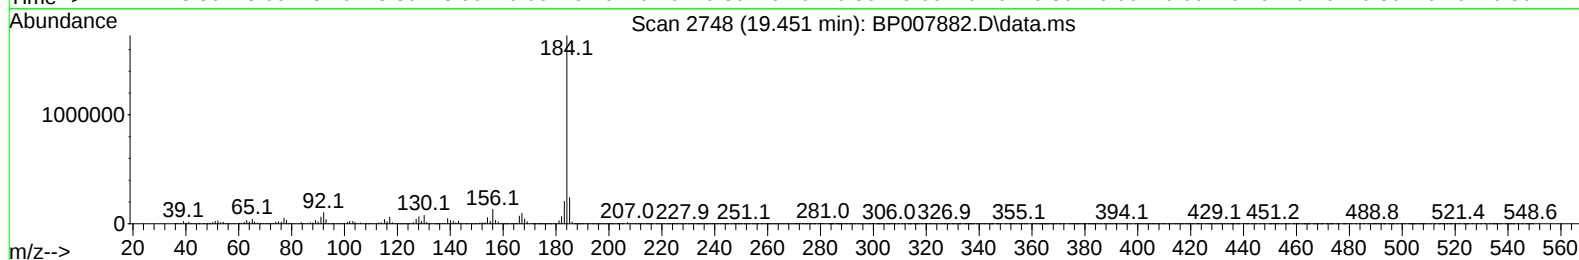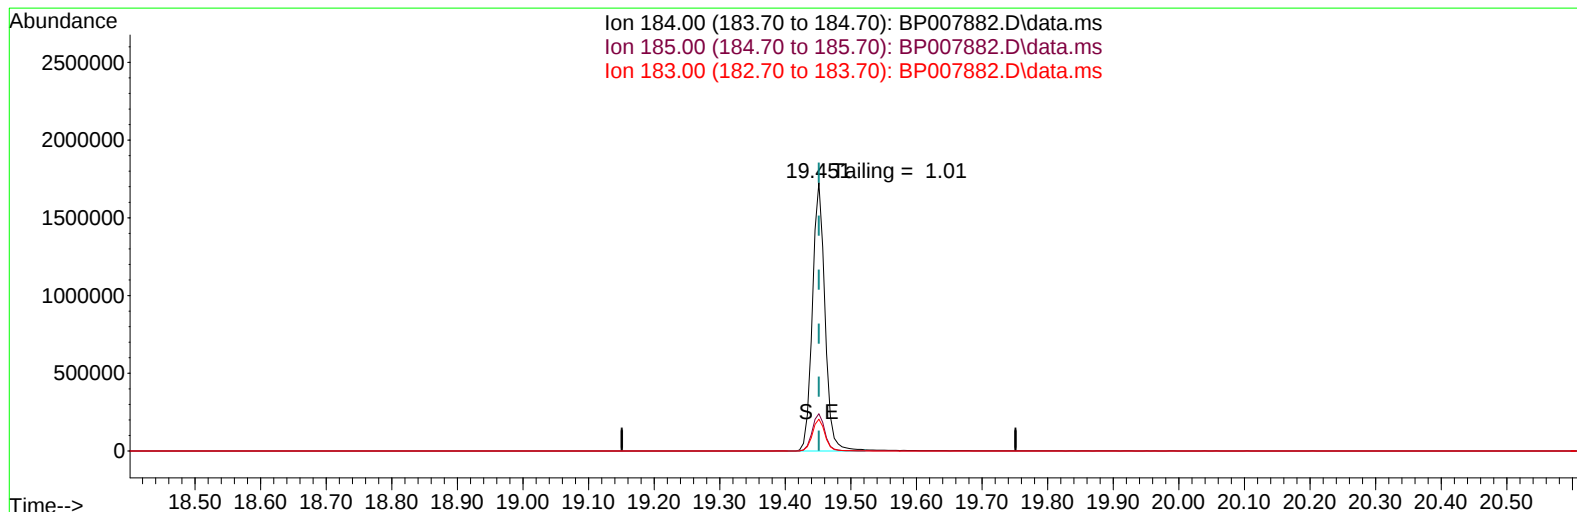

TIC: BP007882.D\data.ms

(77) Benzidine

19.451min (+ 0.000) 871503.86 ng

response 2328230

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.90
183.00	11.40	11.91
0.00	0.00	0.00

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/9/2021	BNA_P	<u>BP007882.D</u>
Compound Name	Response	Retention Time
DDT	1310896	20.65
DDD	35347	20.22
DDE	2358	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37705	1348601	2.80