
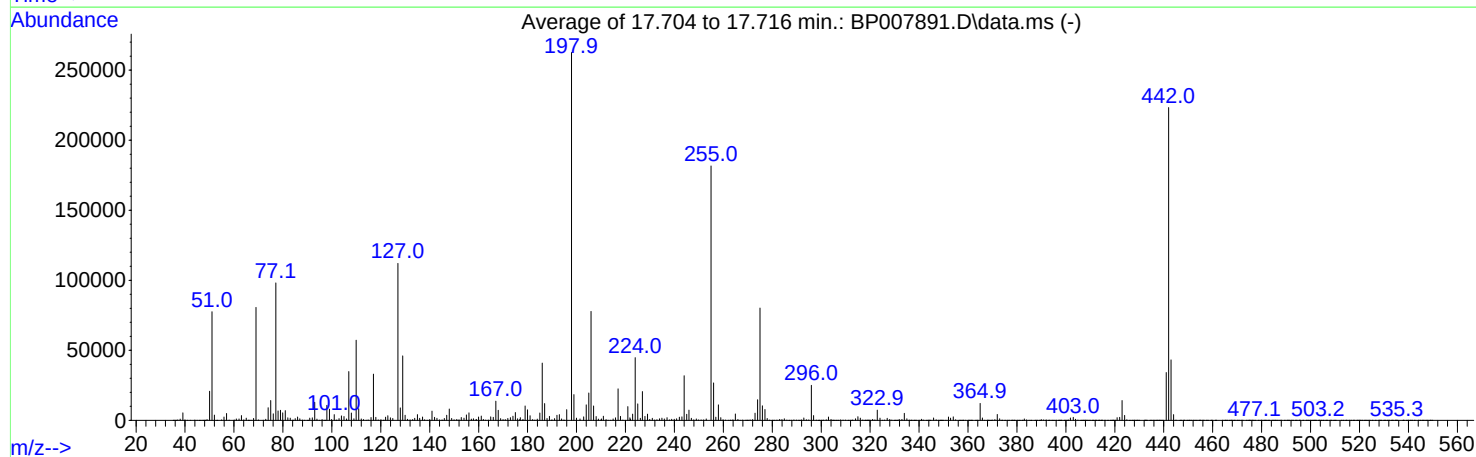


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
 Data File : BP007891.D
 Acq On : 09 Nov 2021 14:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 09 10:45:24 2021

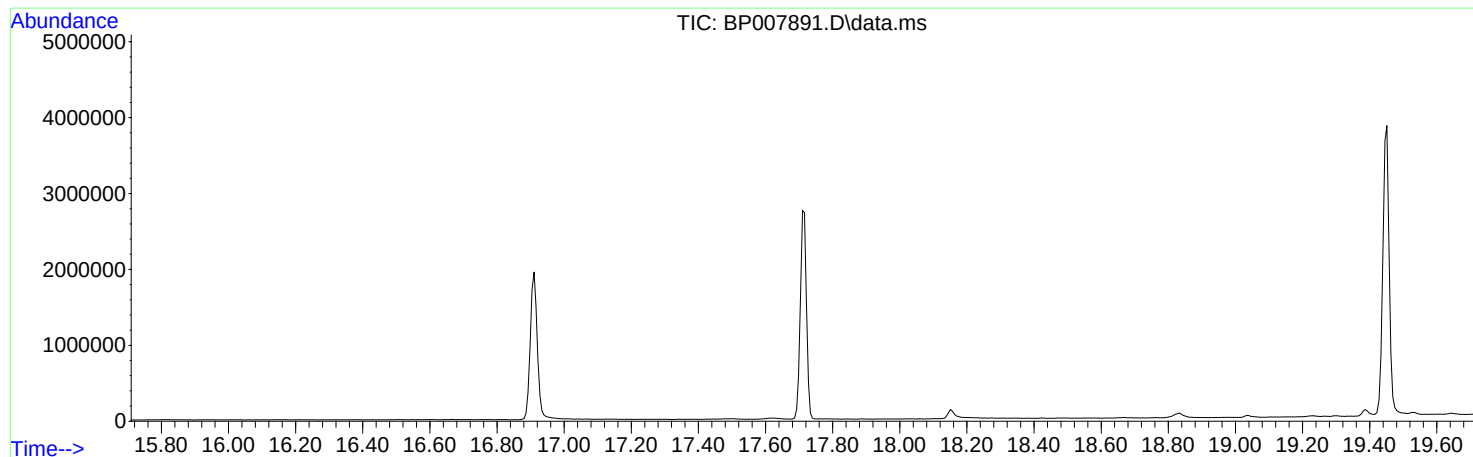




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	77586	PASS
68	69	0.00	2	1.7	1375	PASS
69	198	0.00	100	30.7	80692	PASS
70	69	0.00	2	0.5	371	PASS
127	198	10	80	42.7	112078	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	262617	PASS
199	198	5	9	7.0	18461	PASS
275	198	10	60	30.6	80253	PASS
365	198	1	100	4.6	12134	PASS
441	198	0.01	100	13.0	34217	PASS
442	442	100	100	100.0	223347	PASS
443	442	15	24	19.4	43224	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
Data File : BP007891.D
Acq On : 09 Nov 2021 14:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 09 15:36:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 10:45:24 2021
Response via : Initial Calibration

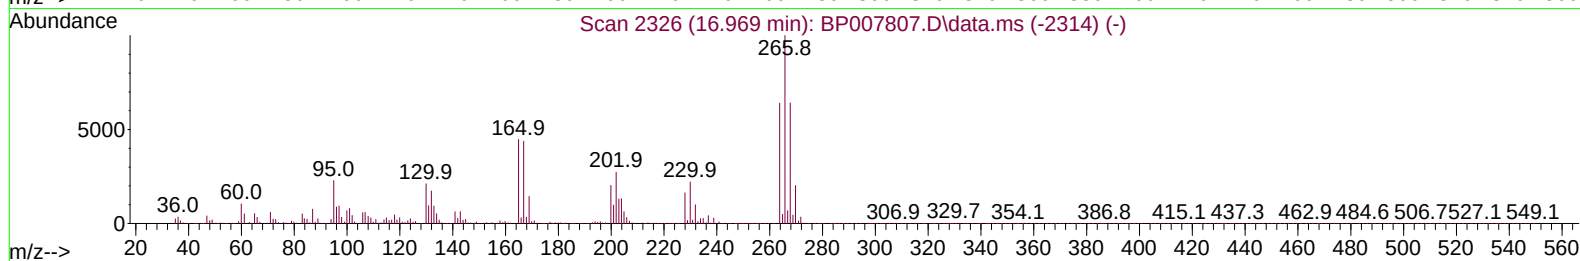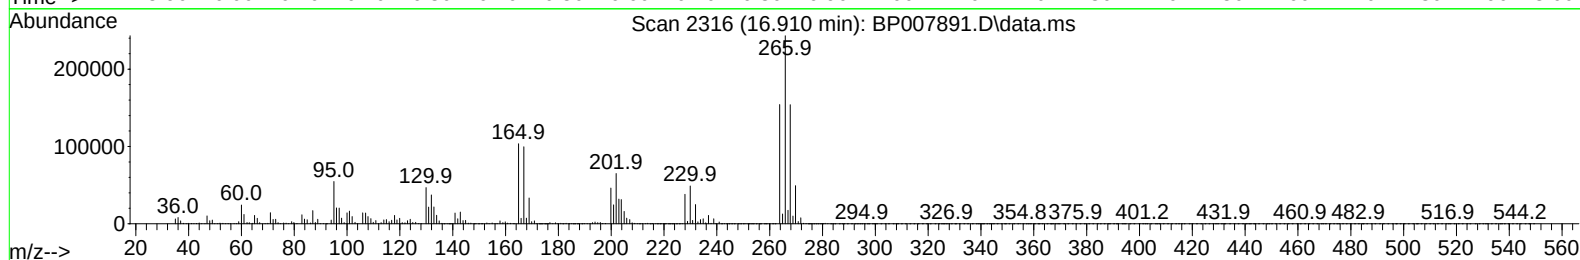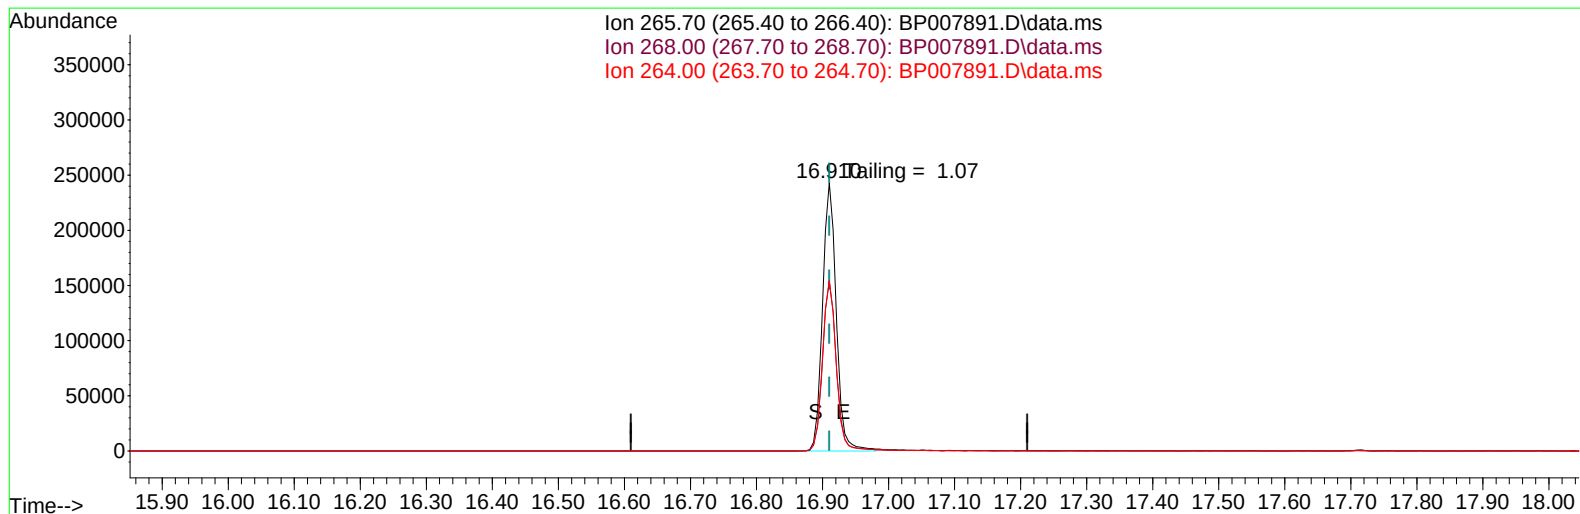

TIC: BP007891.D\data.ms

(70) Pentachlorophenol (C)

16.910min (+ 0.000) 580329.04 ng




response 355033

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	63.29
264.00	60.90	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110921\
 Data File : BP007891.D
 Acq On : 09 Nov 2021 14:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 09 15:36:58 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 10:45:24 2021
 Response via : Initial Calibration

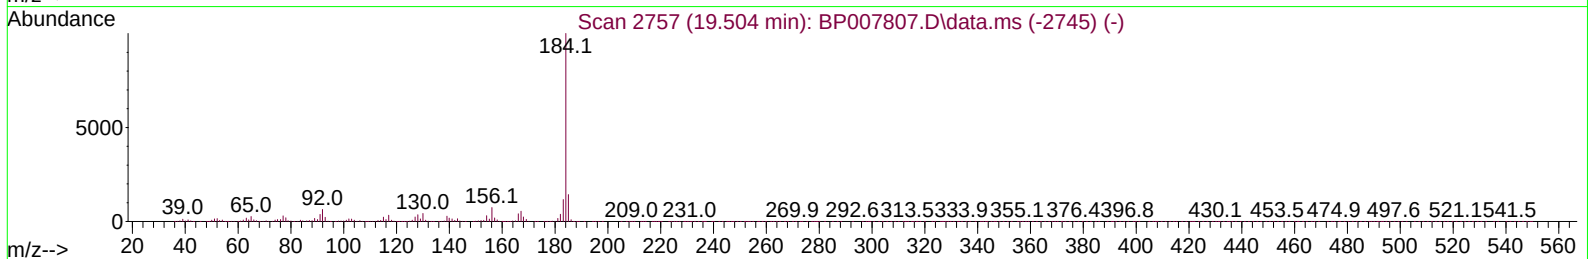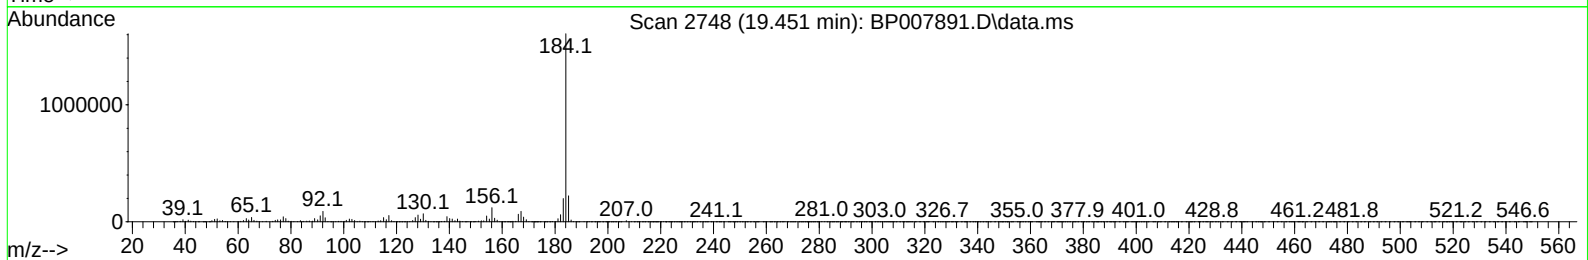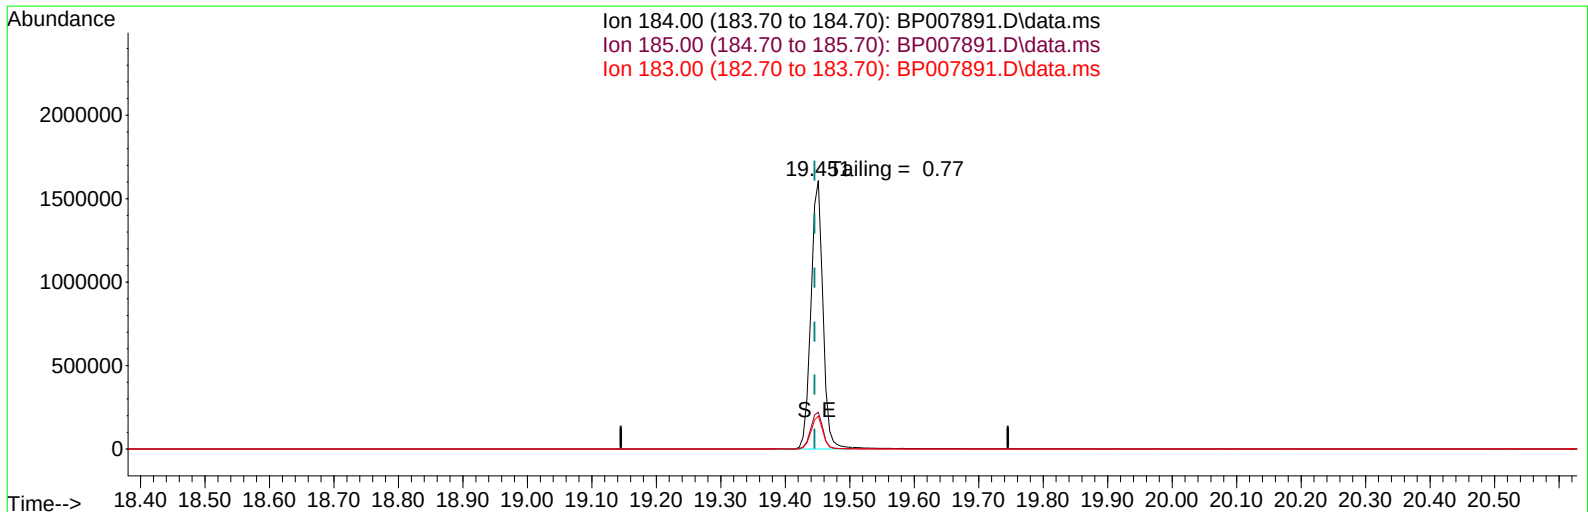

TIC: BP007891.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 760902.73 ng

response 2109466

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.76
183.00	11.40	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/9/2021	BNA_P	BP007891.D
Compound Name	Response	Retention Time
DDT	1122675	20.65
DDD	27762	20.22
DDE	2271	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30033	1152708	2.61