

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110922\
 Data File : BP012592.D
 Acq On : 09 Nov 2022 17:07
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV616

Quant Time: Nov 09 23:30:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 09 23:28:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.764	152	328223	20.000	ng/u1	0.00
20) Naphthalene-d8	10.563	136	1483432	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.416	164	943871	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.181	188	1914877	20.000	ng/u1	0.00
79) Chrysene-d12	21.280	240	1503671	20.000	ng/u1	0.00
88) Perylene-d12	23.651	264	1370135	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	55158	6.849	ng/uL	0.00
4) Pyridine-d5	3.640	84	409977	18.015	ng/u1	0.00
7) Phenol-d5	6.952	99	546731	19.760	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	356588	21.540	ng/u1	0.00
11) 2-Chlorophenol-d4	7.299	132	434679	20.415	ng/u1	0.00
15) 4-Methylphenol-d8	8.493	113	443498	20.263	ng/u1	0.00
21) Nitrobenzene-d5	8.934	128	224267	20.432	ng/u1	0.00
24) 2-Nitrophenol-d4	9.652	143	254818	21.137	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	456623	21.024	ng/u1	0.00
31) 4-Chloroaniline-d4	10.716	131	625482	20.445	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	1351374	20.772	ng/u1	0.00
49) Acenaphthylene-d8	14.110	160	1537898	20.896	ng/u1	0.00
54) 4-Nitrophenol-d4	14.663	143	199142	19.441	ng/u1	0.00
60) Fluorene-d10	15.416	176	1132404	20.528	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	222081	20.969	ng/u1	0.00
73) Anthracene-d10	17.281	188	1691685	20.343	ng/u1	0.00
81) Pyrene-d10	19.522	212	1798121	21.339	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.498	264	1351491	20.009	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.258	88	57041	6.631	ng/uL	96
5) Pyridine	3.664	79	370576	16.843	ng/u1	97
6) Benzaldehyde	6.911	77	356977	27.600	ng/u1	99
8) Phenol	6.981	94	545097	19.079	ng/u1	100
10) Bis(2-Chloroethyl)ether	7.199	93	445328	19.296	ng/u1	98
12) 2-Chlorophenol	7.328	128	443070	19.401	ng/u1	99
13) 2-Methylphenol	8.222	108	424952	19.254	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.299	45	568546	18.822	ng/u1	98
16) Acetophenone	8.599	105	699243	20.902	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.581	70	346838	20.147	ng/u1	99
18) 4-Methylphenol	8.558	108	457614	19.506	ng/u1	100
19) Hexachloroethane	8.828	117	176104	19.132	ng/u1	100
22) Nitrobenzene	8.975	77	510692	19.381	ng/u1	99
23) Isophorone	9.499	82	982039	19.230	ng/u1	99
25) 2-Nitrophenol	9.687	139	265571	19.742	ng/u1	97
26) 2,4-Dimethylphenol	9.752	107	509015	19.243	ng/u1	100
27) Bis(2-Chloroethoxy)met...	9.987	93	623759	19.177	ng/u1	100
29) 2,4-Dichlorophenol	10.222	162	441892	19.689	ng/u1	99
30) Naphthalene	10.610	128	1465288	19.085	ng/u1	100
32) 4-Chloroaniline	10.740	127	638508	20.308	ng/u1	100
33) Hexachlorobutadiene	10.881	225	299884	20.179	ng/u1	98
34) Caprolactam	11.546	113	129385	18.291	ng/u1	93
35) 4-Chloro-3-methylphenol	11.881	107	484660	19.726	ng/u1	99
36) 2-Methylnaphthalene	12.228	142	1042649	19.744	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110922\
 Data File : BP012592.D
 Acq On : 09 Nov 2022 17:07
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV616


Quant Time: Nov 09 23:30:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 09 23:28:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.446	142	994164	18.796	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.593	216	562588	19.945	ng/ul	99
40) Hexachlorocyclopentadiene	12.563	237	272379	19.851	ng/ul	98
41) 2,4,6-Trichlorophenol	12.851	196	366619	20.112	ng/ul	98
42) 2,4,5-Trichlorophenol	12.934	196	389275	20.213	ng/ul	96
43) 1,1'-Biphenyl	13.246	154	1376472	20.269	ng/ul	99
44) 2-Chloronaphthalene	13.287	162	1053980	19.552	ng/ul	99
45) 2-Nitroaniline	13.510	65	298752	20.347	ng/ul	97
47) Dimethylphthalate	13.887	163	1324778	19.505	ng/ul	99
48) 2,6-Dinitrotoluene	14.010	165	286427	21.468	ng/ul	96
50) Acenaphthylene	14.140	152	1655198	20.432	ng/ul	100
51) 3-Nitroaniline	14.346	138	295682	21.860	ng/ul	100
52) Acenaphthene	14.481	153	1112172	19.377	ng/ul	99
53) 2,4-Dinitrophenol	14.557	184	140422	18.230	ng/ul	98
55) 4-Nitrophenol	14.681	109	153715	18.499	ng/ul	94
56) Dibenzofuran	14.816	168	1580189	20.364	ng/ul	99
57) 2,4-Dinitrotoluene	14.804	165	380886	20.623	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.051	232	341960	20.343	ng/ul	97
59) Diethylphthalate	15.251	149	1302556	19.316	ng/ul	99
61) Fluorene	15.469	166	1224125	19.762	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.469	204	624569	19.932	ng/ul	99
63) 4-Nitroaniline	15.516	138	272187	24.082	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.569	198	215466	19.520	ng/ul	97
67) N-Nitrosodiphenylamine	15.687	169	1083696	20.178	ng/ul	99
68) 4-Bromophenyl-phenylether	16.369	248	409639	20.059	ng/ul	97
69) Hexachlorobenzene	16.475	284	486267	20.002	ng/ul	97
70) Atrazine	16.651	200	367575	19.215	ng/ul	100
71) Pentachlorophenol	16.834	266	261057	19.122	ng/ul	99
72) Phenanthrene	17.222	178	1925150	19.303	ng/ul	99
74) Anthracene	17.316	178	1931376	18.919	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.210	216	536988	19.144	ng/ul	98
76) Pentachlorobenzene	14.734	250	540287	17.873	ng/ul	100
77) Carbazole	17.598	167	1736382	20.389	ng/ul	100
78) Di-n-butylphthalate	18.139	149	2163633	18.899	ng/ul	100
80) Fluoranthene	19.198	202	2127178	20.442	ng/ul	98
82) Pyrene	19.551	202	2159284	20.355	ng/ul	96
83) Butylbenzylphthalate	20.428	149	851411	19.981	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.204	252	648710	21.955	ng/ul	99
85) Benzo(a)anthracene	21.263	228	1813511	19.024	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.186	149	1154841	19.564	ng/ul	99
87) Chrysene	21.316	228	1716616	19.179	ng/ul	100
89) Di-n-octyl phthalate	22.098	149	1695957	17.147	ng/ul	100
90) Benzo(b)fluoranthene	22.927	252	1647254	17.941	ng/ul	99
91) Benzo(k)fluoranthene	22.974	252	1618698	18.498	ng/ul	99
93) Benzo(a)pyrene	23.545	252	1447655	19.208	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.115	276	1981084	22.889	ng/ul	97
95) Dibenzo(a,h)anthracene	26.127	278	1747364	22.256	ng/ul	98
96) Benzo(g,h,i)perylene	26.874	276	1727509	22.255	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 09 23:30:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 09 23:28:28 2022
Response via : Initial Calibration







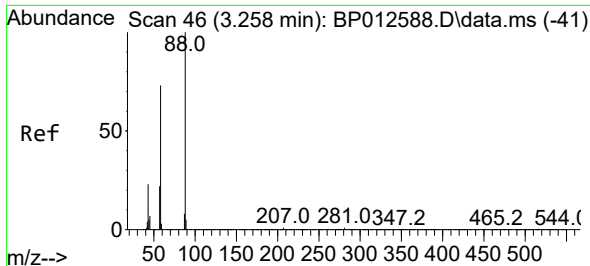

#2
1,4-Dioxane
Concen: 6.631 ng/uL
RT: 3.258 min Scan# 41
Delta R.T. -0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:	88	Resp:	57041
Ion	Ratio	Lower	Upper
88	100		
43	26.6	18.9	28.3
58	69.8	57.8	86.8

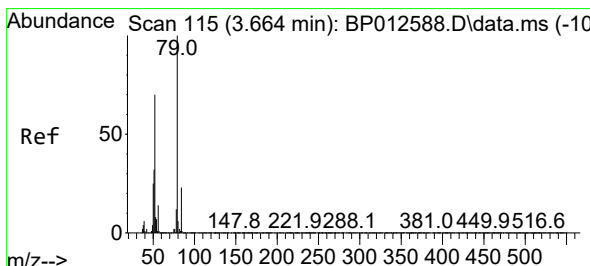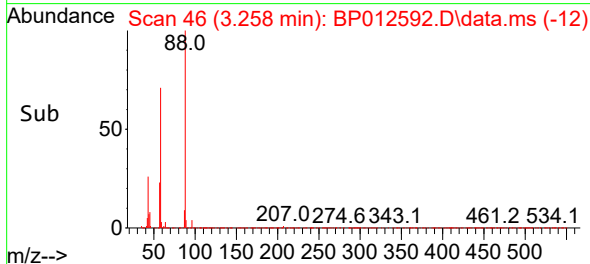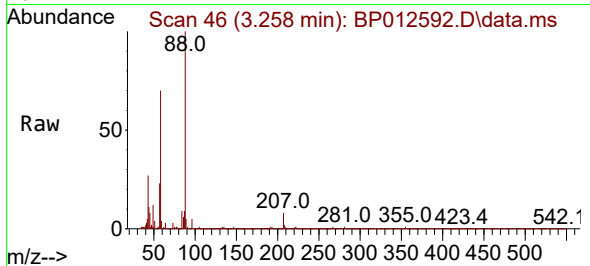

#5
Pyridine
Concen: 16.843 ng/uL
RT: 3.664 min Scan# 115
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:	79	Resp:	370576
Ion	Ratio	Lower	Upper
79	100		
52	73.5	55.8	83.6
51	32.8	25.8	38.8


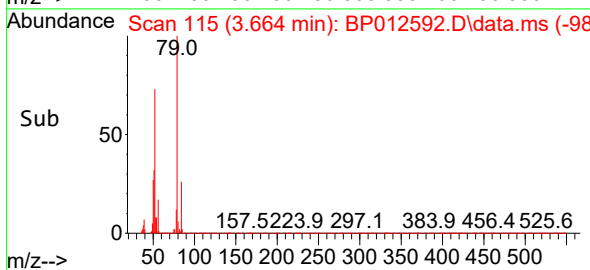

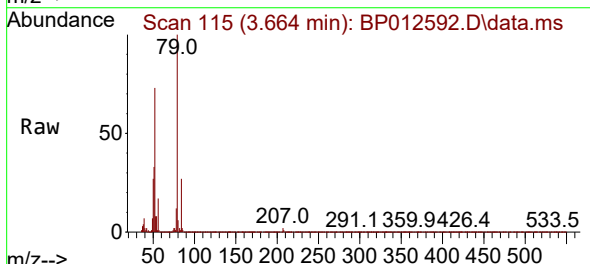


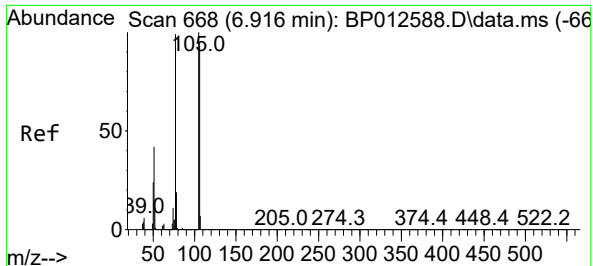

#6
Benzaldehyde
Concen: 27.600 ng/ul
RT: 6.911 min Scan# 609
Delta R.T. -0.006 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion: 77 Resp: 356977
Ion Ratio Lower Upper
77 100
105 99.8 80.7 121.1
106 95.8 76.7 115.1

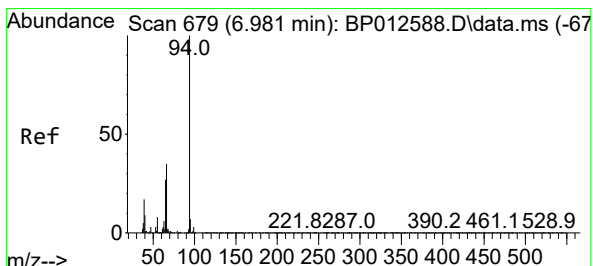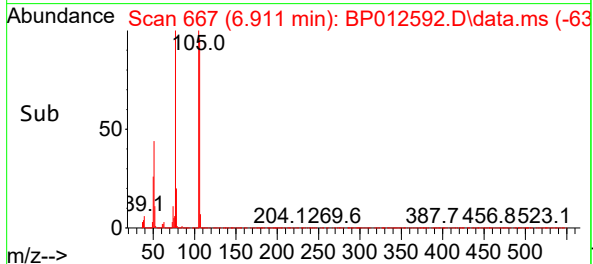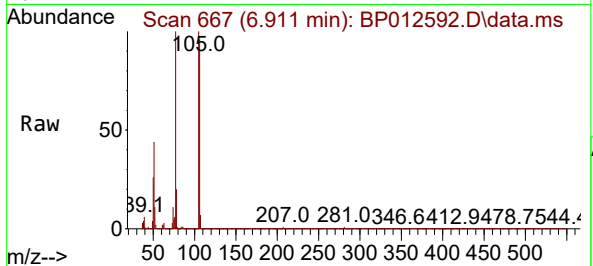

#8
Phenol
Concen: 19.079 ng/ul
RT: 6.981 min Scan# 679
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion: 94 Resp: 545097
Ion Ratio Lower Upper
94 100
65 26.8 21.4 32.2
66 35.5 28.2 42.2

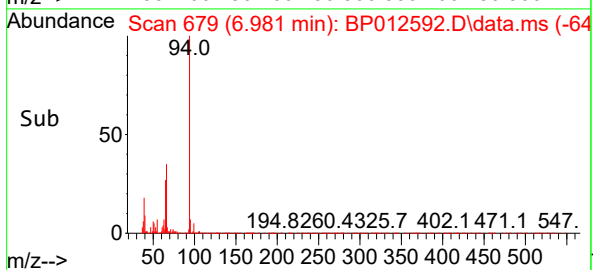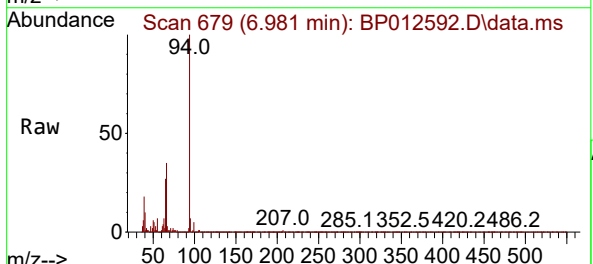



#10

Bis(2-Chloroethyl)ether

Concen: 19.296 ng/ul

RT: 7.199 min Scan# 716

Delta R.T. 0.000 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07

Instrument :

BNA_P

ClientSampleId :

SICV616





Tgt Ion: 93 Resp: 445328

Ion Ratio Lower Upper

93 100

63 72.1 59.1 88.7

95 33.0 26.5 39.7

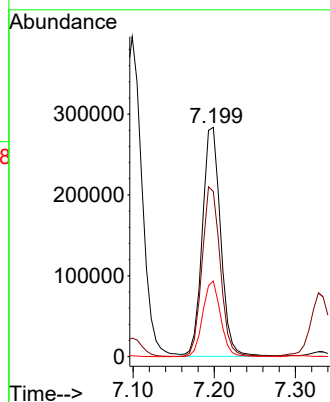

#12

2-Chlorophenol

Concen: 19.401 ng/ul

RT: 7.328 min Scan# 738

Delta R.T. -0.006 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07




Tgt Ion:128 Resp: 443070


Ion Ratio Lower Upper

128 100

64 45.3 35.3 52.9

130 32.0 25.8 38.6





#13

2-Methylphenol

Concen: 19.254 ng/ul

RT: 8.222 min Scan# 890

Delta R.T. 0.000 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07

Instrument :

BNA_P

ClientSampleId :





SICV616

Tgt Ion:108 Resp: 424952

Ion Ratio Lower Upper

108 100

107 88.8 70.2 105.4

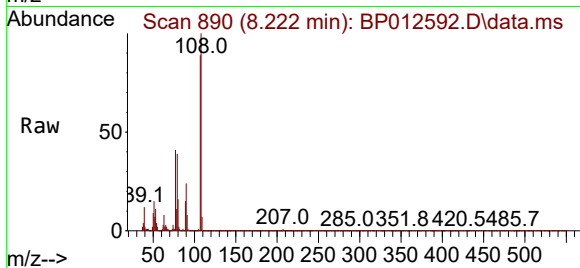

#14

2,2'-oxybis(1-Chloropropane)

Concen: 18.822 ng/ul

RT: 8.299 min Scan# 903

Delta R.T. 0.000 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07




Tgt Ion: 45 Resp: 568546


Ion Ratio Lower Upper

45 100

77 16.7 12.4 18.6

79 12.4 10.2 15.4









#16
Acetophenone
Concen: 20.902 ng/ul
RT: 8.599 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:105 Resp: 699243
Ion Ratio Lower Upper
105 100
77 75.3 60.5 90.7
51 24.4 20.1 30.1

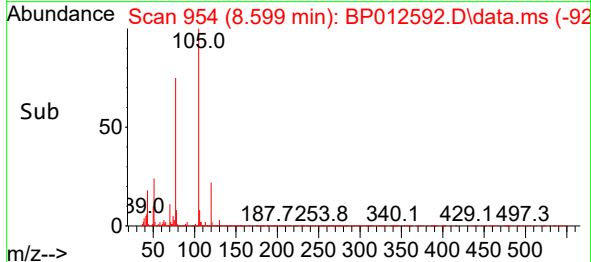

#17
N-Nitroso-di-n-propylamine
Concen: 20.147 ng/ul
RT: 8.581 min Scan# 951
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion: 70 Resp: 346838
Ion Ratio Lower Upper
70 100
42 51.7 41.2 61.8
101 10.2 8.0 12.0
130 22.8 17.7 26.5


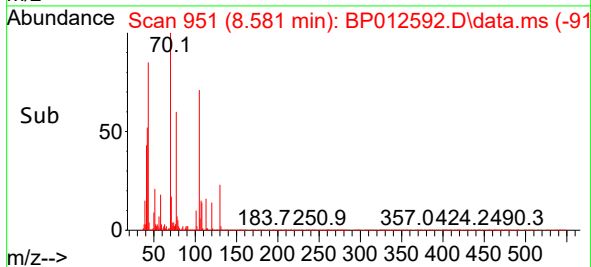

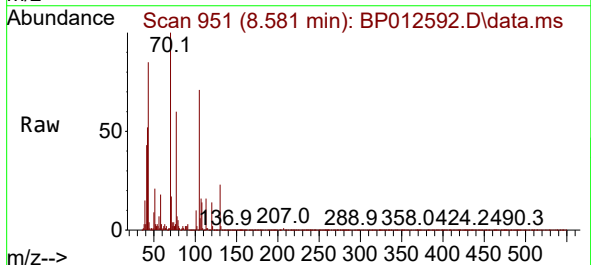




#18
4-Methylphenol
Concen: 19.506 ng/ul
RT: 8.558 min Scan# 947
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:108 Resp: 457614
Ion Ratio Lower Upper
108 100
107 109.7 87.8 131.6

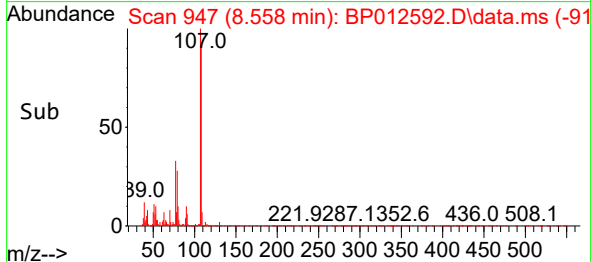

#19
Hexachloroethane
Concen: 19.132 ng/ul
RT: 8.828 min Scan# 993
Delta R.T. -0.006 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:117 Resp: 176104
Ion Ratio Lower Upper
117 100
201 105.4 84.6 127.0
199 64.3 51.5 77.3


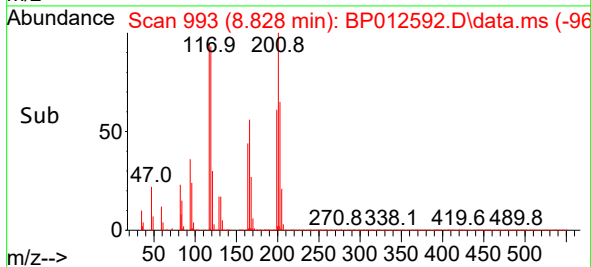

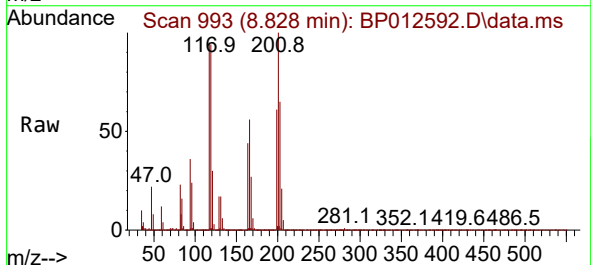




#22
Nitrobenzene
Concen: 19.381 ng/ul
RT: 8.975 min Scan# 1107
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion: 77 Resp: 510692
Ion Ratio Lower Upper
77 100
123 47.5 37.1 55.7
65 12.9 10.2 15.2



#23
Isophorone
Concen: 19.230 ng/ul
RT: 9.499 min Scan# 1107
Delta R.T. -0.006 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion: 82 Resp: 982039
Ion Ratio Lower Upper
82 100
95 7.2 5.7 8.5
138 17.5 14.6 21.8









#25
2-Nitrophenol
Concen: 19.742 ng/ul
RT: 9.687 min Scan# 1139
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:139 Resp: 265571
Ion Ratio Lower Upper
139 100
65 48.8 37.8 56.6
109 30.7 23.0 34.4



#26
2,4-Dimethylphenol
Concen: 19.243 ng/ul
RT: 9.752 min Scan# 1150
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:107 Resp: 509015
Ion Ratio Lower Upper
107 100
121 50.7 40.3 60.5
122 85.9 68.8 103.2









#27
 Bis(2-Chloroethoxy)methane
 Concen: 19.177 ng/ul
 RT: 9.987 min Scan# 1190
 Delta R.T. 0.000 min
 Lab File: BP012592.D
 Acq: 09 Nov 2022 17:07




Instrument :
 BNA_P
 ClientSampleId :
 SICV616


Tgt Ion:	93	Resp:	623759
Ion	Ratio	Lower	Upper
93	100		
95	32.6	26.1	39.1
123	11.3	9.1	13.7



#29
 2,4-Dichlorophenol
 Concen: 19.689 ng/ul
 RT: 10.222 min Scan# 1230
 Delta R.T. 0.000 min
 Lab File: BP012592.D
 Acq: 09 Nov 2022 17:07

Tgt Ion:	162	Resp:	441892
Ion	Ratio	Lower	Upper
162	100		
164	65.6	51.9	77.9
98	34.7	28.7	43.1









#30
Naphthalene
Concen: 19.085 ng/ul
RT: 10.610 min Scan# 1296
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:128 Resp: 1465288
Ion Ratio Lower Upper
128 100
129 11.0 8.8 13.2
127 13.0 10.3 15.5

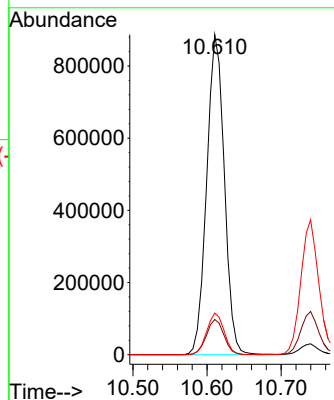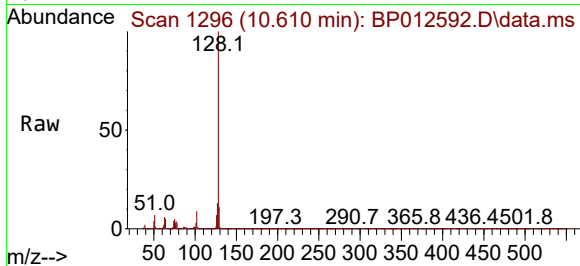

#32
4-Chloroaniline
Concen: 20.308 ng/ul
RT: 10.740 min Scan# 1318
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:127 Resp: 638508
Ion Ratio Lower Upper
127 100
129 32.0 25.4 38.2



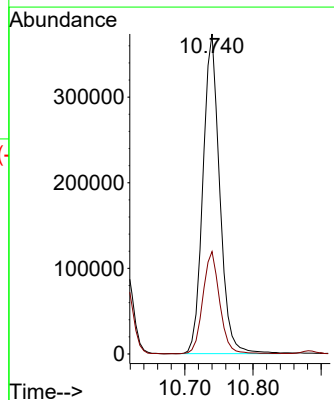





#33
Hexachlorobutadiene
Concen: 20.179 ng/ul
RT: 10.881 min Scan# 1342
Delta R.T. -0.006 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:225 Resp: 299884
Ion Ratio Lower Upper
225 100
223 62.8 51.3 76.9
227 64.3 50.4 75.6

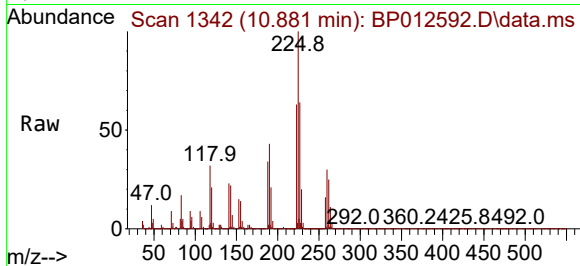

#34
Caprolactam
Concen: 18.291 ng/ul
RT: 11.546 min Scan# 1455
Delta R.T. 0.006 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:113 Resp: 129385
Ion Ratio Lower Upper
113 100
55 157.7 135.1 202.7
56 117.1 98.6 147.8









#35
4-Chloro-3-methylphenol
Concen: 19.726 ng/ul
RT: 11.881 min Scan# 1512
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:107 Resp: 484660
Ion Ratio Lower Upper
107 100
144 25.5 20.9 31.3
142 80.2 63.8 95.8

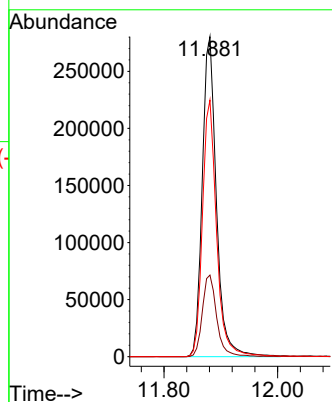

#36
2-Methylnaphthalene
Concen: 19.744 ng/ul
RT: 12.228 min Scan# 1571
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:142 Resp: 1042649
Ion Ratio Lower Upper
142 100
141 89.6 71.0 106.6





#37

1-Methylnaphthalene

Concen: 18.796 ng/ul

RT: 12.446 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07

Instrument :

BNA_P

ClientSampleId :

SICV616





Tgt Ion:142 Resp: 994164

Ion Ratio Lower Upper

142 100

141 91.8 73.4 110.2

116 4.0 3.0 4.6

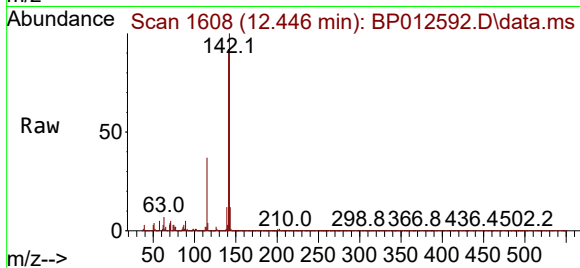

#39

1,2,4,5-Tetrachlorobenzene

Concen: 19.945 ng/ul

RT: 12.593 min Scan# 1633

Delta R.T. -0.006 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07

Tgt Ion:216 Resp: 562588




Ion Ratio Lower Upper


216 100

214 78.6 63.8 95.8

179 20.8 16.8 25.2

108 16.6 13.5 20.3







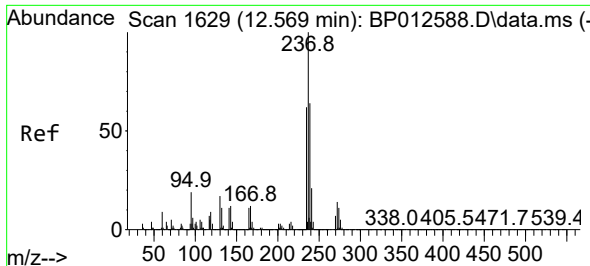

#40
Hexachlorocyclopentadiene
Concen: 19.851 ng/ul
RT: 12.563 min Scan# 1628
Delta R.T. -0.006 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:237 Resp: 272379
Ion Ratio Lower Upper
237 100
235 63.9 49.8 74.6
272 13.5 11.4 17.0

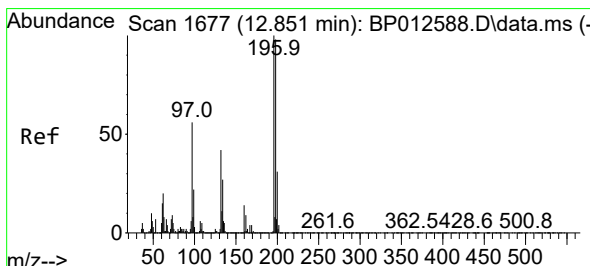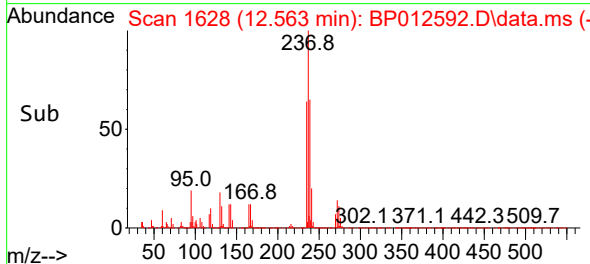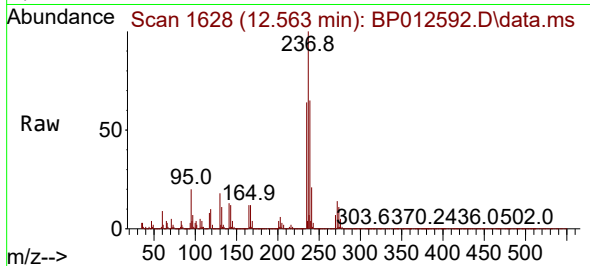

#41
2,4,6-Trichlorophenol
Concen: 20.112 ng/ul
RT: 12.851 min Scan# 1677
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:196 Resp: 366619
Ion Ratio Lower Upper
196 100
198 95.8 78.3 117.5
200 31.3 24.6 37.0


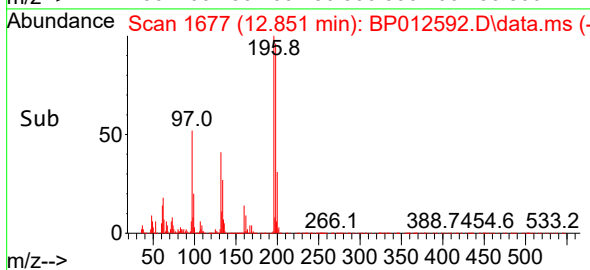

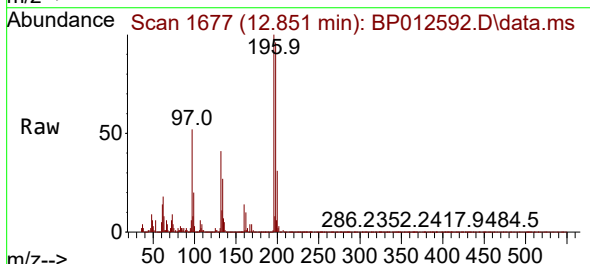




#42
2,4,5-Trichlorophenol
Concen: 20.213 ng/ul
RT: 12.934 min Scan# 1691
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:196 Resp: 389275
Ion Ratio Lower Upper
196 100
198 98.9 75.6 113.4
200 31.1 25.4 38.2

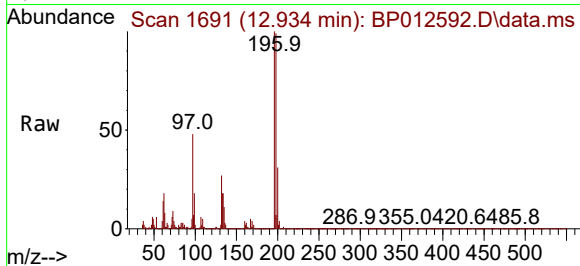

#43
1,1'-Biphenyl
Concen: 20.269 ng/ul
RT: 13.246 min Scan# 1744
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:154 Resp: 1376472
Ion Ratio Lower Upper
154 100
153 40.0 32.0 48.0
76 12.4 10.7 16.1









#44
2-Chloronaphthalene
Concen: 19.552 ng/ul
RT: 13.287 min Scan# 1751
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:162 Resp: 1053980
Ion Ratio Lower Upper
162 100
164 33.2 26.4 39.6
127 39.1 31.7 47.5

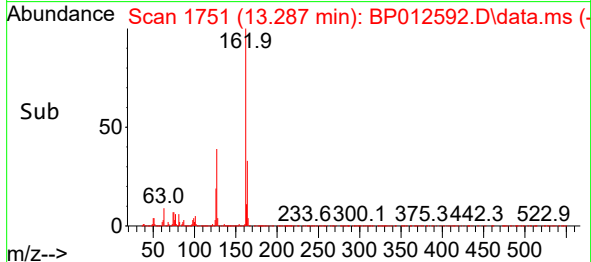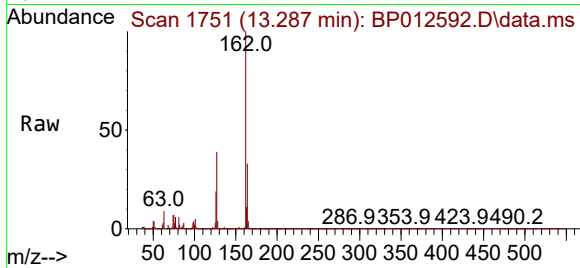

#45
2-Nitroaniline
Concen: 20.347 ng/ul
RT: 13.510 min Scan# 1789
Delta R.T. -0.006 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion: 65 Resp: 298752
Ion Ratio Lower Upper
65 100
92 70.6 57.6 86.4
138 109.9 91.2 136.8


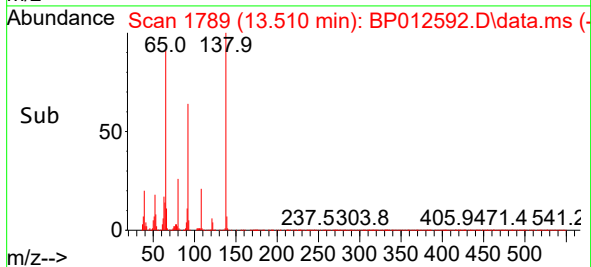

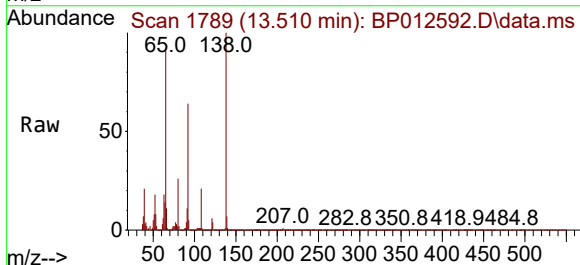




#47
Dimethylphthalate
Concen: 19.505 ng/ul
RT: 13.887 min Scan# 1853
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:163 Resp: 1324778
Ion Ratio Lower Upper
163 100
194 4.2 3.1 4.7
164 10.0 7.8 11.8

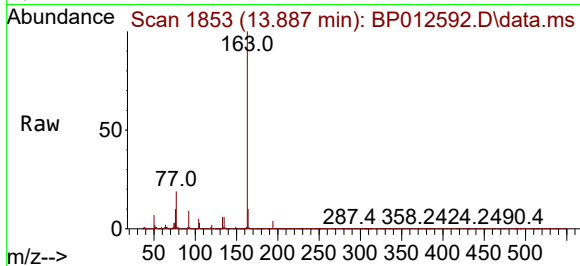

#48
2,6-Dinitrotoluene
Concen: 21.468 ng/ul
RT: 14.010 min Scan# 1874
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:165 Resp: 286427
Ion Ratio Lower Upper
165 100
89 57.0 47.2 70.8
121 20.4 18.6 27.8









#50
Acenaphthylene
Concen: 20.432 ng/ul
RT: 14.140 min Scan# 1896
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:152 Resp: 1655198
Ion Ratio Lower Upper
152 100
151 19.8 15.8 23.8
153 12.8 10.5 15.7



#51
3-Nitroaniline
Concen: 21.860 ng/ul
RT: 14.346 min Scan# 1931
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:138 Resp: 295682
Ion Ratio Lower Upper
138 100
108 10.2 8.3 12.5
92 113.6 91.0 136.6









#52
Acenaphthene
Concen: 19.377 ng/ul
RT: 14.481 min Scan# 1954
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:153 Resp: 1112172
Ion Ratio Lower Upper
153 100
152 47.8 37.6 56.4
154 88.6 70.3 105.5



#53
2,4-Dinitrophenol
Concen: 18.230 ng/ul
RT: 14.557 min Scan# 1967
Delta R.T. -0.006 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:184 Resp: 140422
Ion Ratio Lower Upper
184 100
63 63.5 48.6 72.8
154 62.3 49.8 74.6



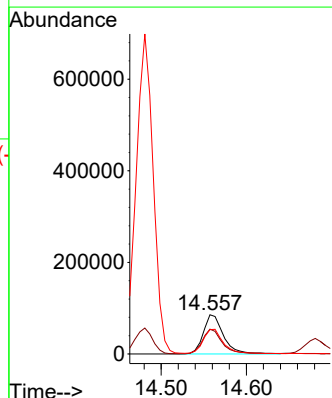





#55
4-Nitrophenol
Concen: 18.499 ng/ul
RT: 14.681 min Scan# 1988
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:109 Resp: 153715
Ion Ratio Lower Upper
109 100
139 135.9 111.2 166.8
65 124.2 107.5 161.3



#56
Dibenzofuran
Concen: 20.364 ng/ul
RT: 14.816 min Scan# 2011
Delta R.T. -0.006 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:168 Resp: 1580189
Ion Ratio Lower Upper
168 100
139 37.7 29.8 44.8









#57
2,4-Dinitrotoluene
Concen: 20.623 ng/ul
RT: 14.804 min Scan# 2009
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:165 Resp: 380886
Ion Ratio Lower Upper
165 100
63 45.3 37.1 55.7
182 2.7 2.2 3.2

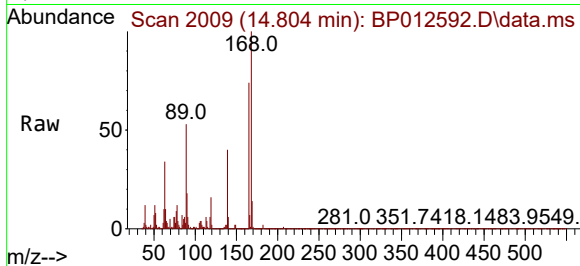

#58
2,3,4,6-Tetrachlorophenol
Concen: 20.343 ng/ul
RT: 15.051 min Scan# 2051
Delta R.T. -0.006 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:232 Resp: 341960
Ion Ratio Lower Upper
232 100
131 43.8 33.3 49.9
130 2.3 1.6 2.4
166 31.8 24.2 36.4


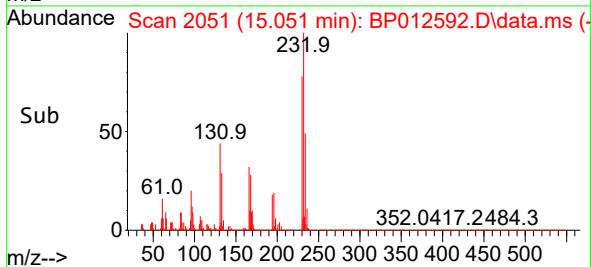

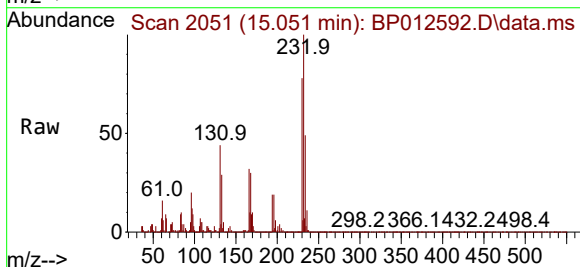




#59
Diethylphthalate
Concen: 19.316 ng/ul
RT: 15.251 min Scan# 2085
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:149 Resp: 1302556
Ion Ratio Lower Upper
149 100
177 22.0 17.2 25.8
150 12.2 9.8 14.6

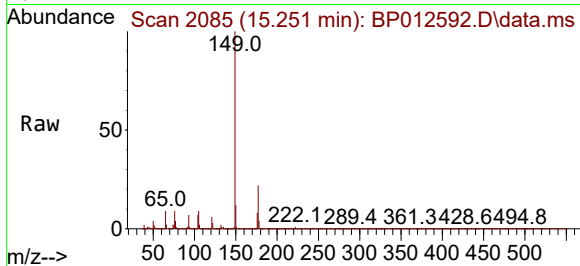

#61
Fluorene
Concen: 19.762 ng/ul
RT: 15.469 min Scan# 2122
Delta R.T. -0.006 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:166 Resp: 1224125
Ion Ratio Lower Upper
166 100
165 98.9 78.6 117.8
167 13.8 10.7 16.1









#62
4-Chlorophenyl-phenylether
Concen: 19.932 ng/ul
RT: 15.469 min Scan# 2122
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:204 Resp: 624569
Ion Ratio Lower Upper
204 100
206 33.4 26.2 39.2
141 58.6 47.7 71.5



#63
4-Nitroaniline
Concen: 24.082 ng/ul
RT: 15.516 min Scan# 2130
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:138 Resp: 272187
Ion Ratio Lower Upper
138 100
92 49.4 41.0 61.4
108 78.4 60.8 91.2







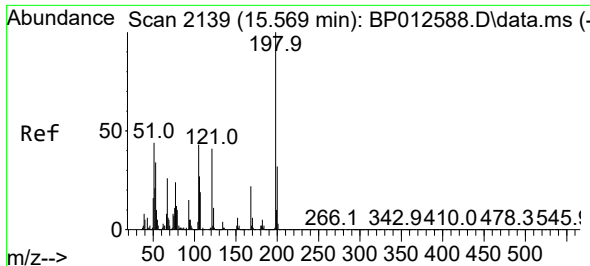

#66
4,6-Dinitro-2-methylphenol
Concen: 19.520 ng/ul
RT: 15.569 min Scan# 2139
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:198 Resp: 215466
Ion Ratio Lower Upper
198 100
182 4.1 4.1 6.1
77 23.9 20.2 30.4

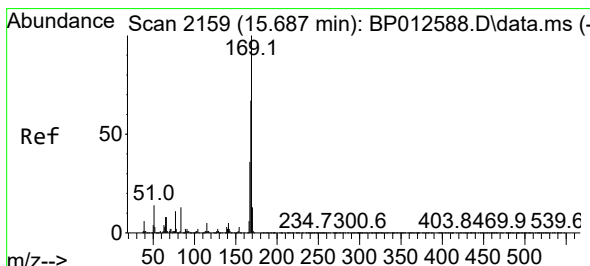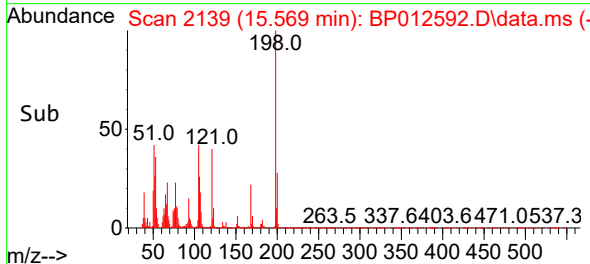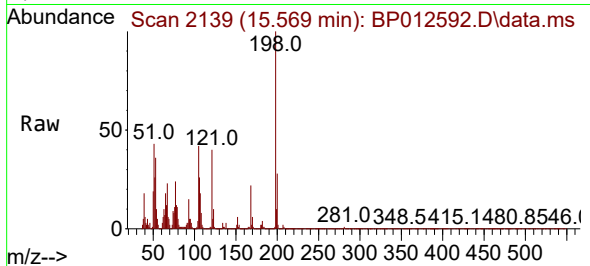

#67
N-Nitrosodiphenylamine
Concen: 20.178 ng/ul
RT: 15.687 min Scan# 2159
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:169 Resp: 1083696
Ion Ratio Lower Upper
169 100
168 65.5 53.4 80.0
167 35.9 29.0 43.4


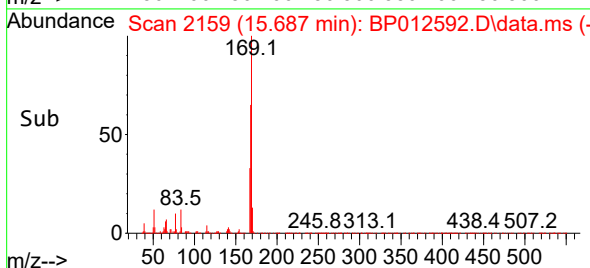
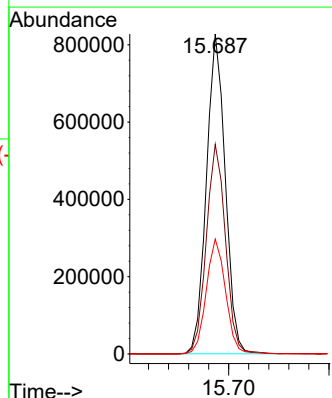
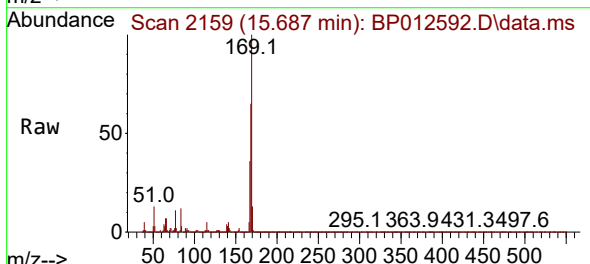




#68
4-Bromophenyl-phenylether
Concen: 20.059 ng/ul
RT: 16.369 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:248 Resp: 409639
Ion Ratio Lower Upper
248 100
250 97.2 78.6 117.8
141 67.2 58.3 87.5

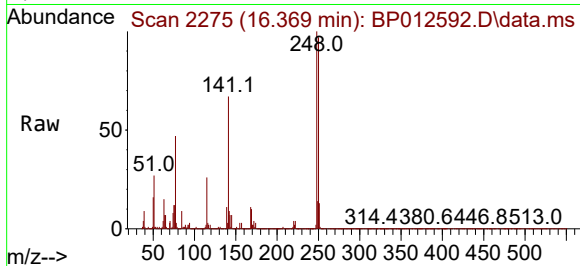

#69
Hexachlorobenzene
Concen: 20.002 ng/ul
RT: 16.475 min Scan# 2293
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:284 Resp: 486267
Ion Ratio Lower Upper
284 100
142 32.0 27.4 41.0
249 29.5 24.5 36.7



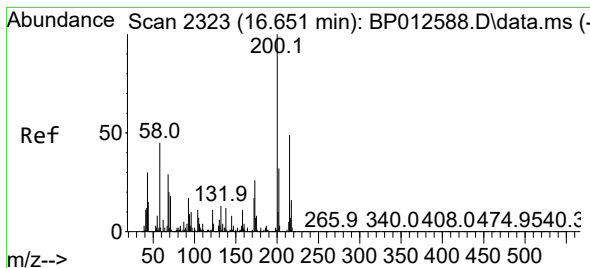

#70

Atrazine

Concen: 19.215 ng/ul

RT: 16.651 min Scan# 2323

Delta R.T. 0.000 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07

Instrument :

BNA_P

ClientSampleId :

SICV616





Tgt Ion:200 Resp: 367575

Ion Ratio Lower Upper

200 100

173 26.6 20.9 31.3

215 48.8 39.1 58.7

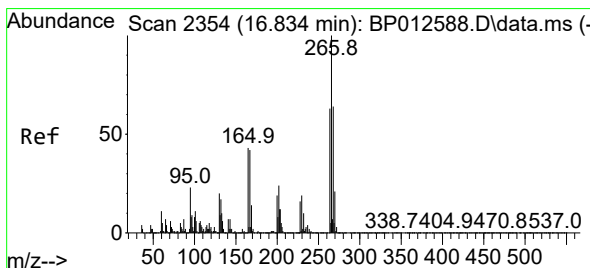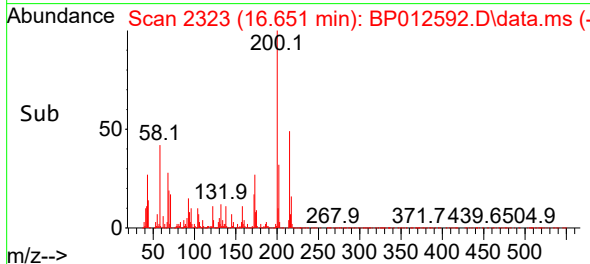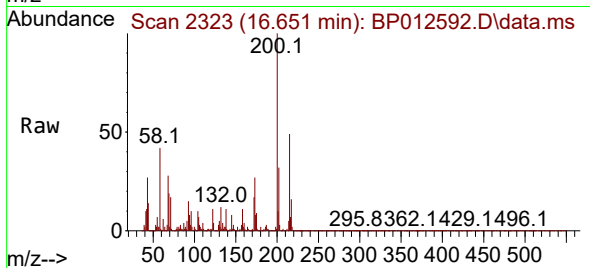

#71

Pentachlorophenol

Concen: 19.122 ng/ul

RT: 16.834 min Scan# 2354

Delta R.T. 0.000 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07




Tgt Ion:266 Resp: 261057


Ion Ratio Lower Upper

266 100

264 61.9 50.2 75.4

268 63.4 51.5 77.3

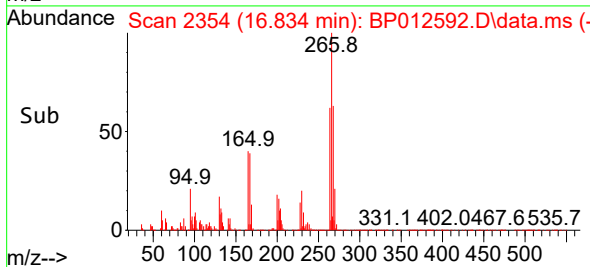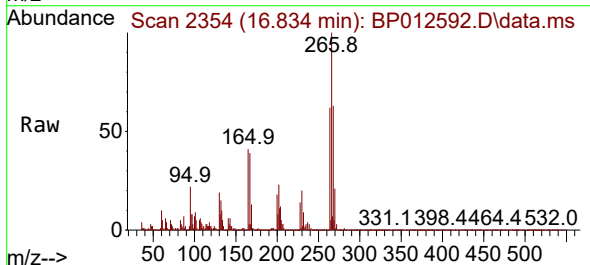



#72

Phenanthrene

Concen: 19.303 ng/ul

RT: 17.222 min Scan# 2420

Delta R.T. 0.000 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07

Instrument :

BNA_P

ClientSampleId :

SICV616





Tgt Ion:178 Resp: 1925150

Ion Ratio Lower Upper

178 100

179 15.5 12.6 18.8

176 18.9 15.5 23.3



#74

Anthracene

Concen: 18.919 ng/ul

RT: 17.316 min Scan# 2436

Delta R.T. 0.000 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07




Tgt Ion:178 Resp: 1931376


Ion Ratio Lower Upper

178 100

179 15.5 12.3 18.5

176 18.9 14.8 22.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.144 ng/uL
RT: 13.210 min Scan# 1738
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:216 Resp: 536988
Ion Ratio Lower Upper
216 100
214 78.1 61.5 92.3
218 49.0 37.9 56.9

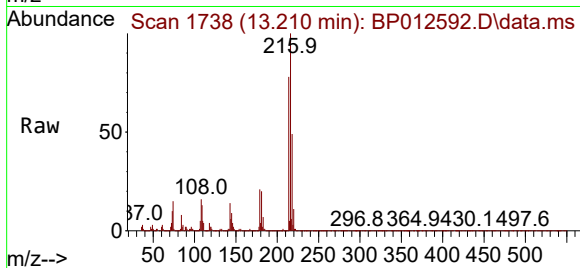

#76
Pentachlorobenzene
Concen: 17.873 ng/uL
RT: 14.734 min Scan# 1997
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:250 Resp: 540287
Ion Ratio Lower Upper
250 100
248 62.7 50.4 75.6
252 63.5 50.9 76.3




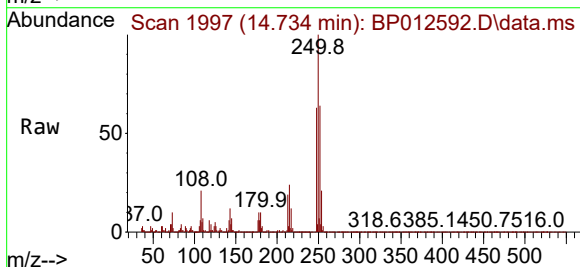




#77
 Carbazole
 Concen: 20.389 ng/ul
 RT: 17.598 min Scan# 2484
 Delta R.T. 0.000 min
 Lab File: BP012592.D
 Acq: 09 Nov 2022 17:07




Instrument :
 BNA_P
 ClientSampleId :
 SICV616


Tgt Ion:167 Resp: 1736382
 Ion Ratio Lower Upper
 167 100
 166 21.6 17.1 25.7
 139 12.7 10.2 15.4

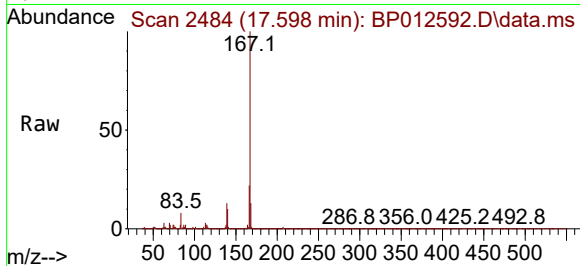

#78
 Di-n-butylphthalate
 Concen: 18.899 ng/ul
 RT: 18.139 min Scan# 2576
 Delta R.T. 0.000 min
 Lab File: BP012592.D
 Acq: 09 Nov 2022 17:07

Tgt Ion:149 Resp: 2163633
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.4 11.0
 104 5.1 3.9 5.9









#80
Fluoranthene
Concen: 20.442 ng/ul
RT: 19.198 min Scan# 2756
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:202 Resp: 2127178
Ion Ratio Lower Upper
202 100
101 10.9 9.4 14.0
100 8.1 7.0 10.4

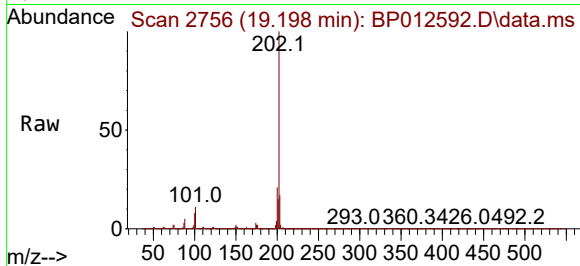

#82
Pyrene
Concen: 20.355 ng/ul
RT: 19.551 min Scan# 2816
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:202 Resp: 2159284
Ion Ratio Lower Upper
202 100
101 12.4 11.3 16.9
100 10.1 8.9 13.3









#83
Butylbenzylphthalate
Concen: 19.981 ng/ul
RT: 20.428 min Scan# 2965
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:149 Resp: 851411
Ion Ratio Lower Upper
149 100
91 69.4 56.6 85.0
206 21.2 15.8 23.6

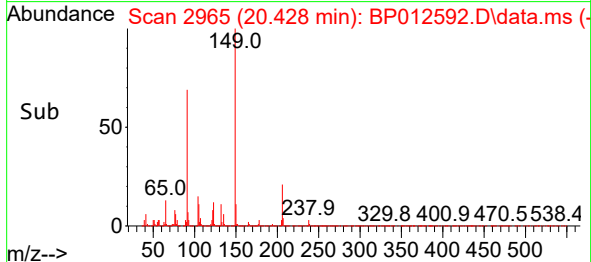

#84
3,3'-Dichlorobenzidine
Concen: 21.955 ng/ul
RT: 21.204 min Scan# 3097
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:252 Resp: 648710
Ion Ratio Lower Upper
252 100
254 64.7 52.0 78.0
126 9.9 9.0 13.4


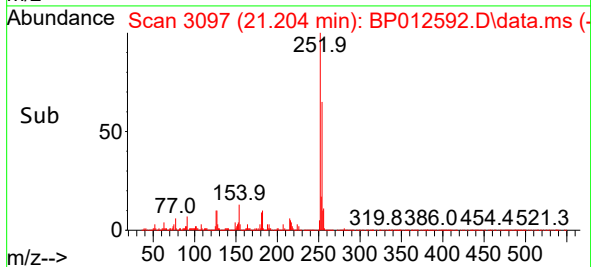

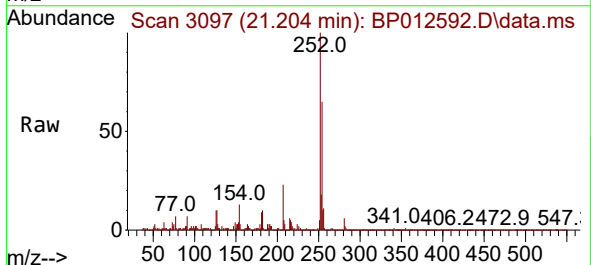




#85
Benzo(a)anthracene
Concen: 19.024 ng/ul
RT: 21.263 min Scan# 3107
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:228 Resp: 1813511
Ion Ratio Lower Upper
228 100
229 19.5 15.7 23.5
226 27.2 21.5 32.3



#86
Bis(2-ethylhexyl)phthalate
Concen: 19.564 ng/ul
RT: 21.186 min Scan# 3094
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:149 Resp: 1154841
Ion Ratio Lower Upper
149 100
167 27.4 21.6 32.4
279 4.7 3.8 5.6









#87
Chrysene
Concen: 19.179 ng/ul
RT: 21.316 min Scan# 3116
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:228 Resp: 1716616
Ion Ratio Lower Upper
228 100
226 30.4 24.1 36.1
229 19.8 15.8 23.8



#89
Di-n-octyl phthalate
Concen: 17.147 ng/ul
RT: 22.098 min Scan# 3249
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:149 Resp: 1695957



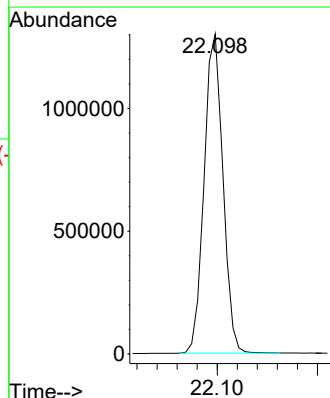





#90
Benzo(b)fluoranthene
Concen: 17.941 ng/ul
RT: 22.927 min Scan# 3390
Delta R.T. 0.000 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07




Instrument :
BNA_P
ClientSampleId :
SICV616


Tgt Ion:252 Resp: 1647254
Ion Ratio Lower Upper
252 100
253 22.2 17.9 26.9
125 9.6 8.2 12.4



#91
Benzo(k)fluoranthene
Concen: 18.498 ng/ul
RT: 22.974 min Scan# 3398
Delta R.T. -0.006 min
Lab File: BP012592.D
Acq: 09 Nov 2022 17:07

Tgt Ion:252 Resp: 1618698
Ion Ratio Lower Upper
252 100
253 22.3 17.9 26.9
125 9.3 7.9 11.9





#93

Benzo(a)pyrene

Concen: 19.208 ng/ul

RT: 23.545 min Scan# 3496

Delta R.T. -0.006 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07

Instrument :

BNA_P

ClientSampleId :

SICV616





Tgt Ion:252 Resp: 1447655

Ion Ratio Lower Upper

252 100

253 21.7 17.8 26.6

125 10.2 8.9 13.3

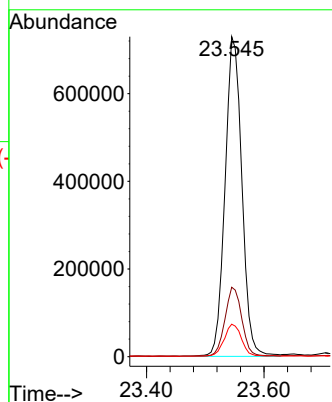

#94

Indeno(1,2,3-cd)pyrene

Concen: 22.889 ng/ul

RT: 26.115 min Scan# 3932

Delta R.T. -0.006 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07




Tgt Ion:276 Resp: 1981084


Ion Ratio Lower Upper

276 100

138 21.6 19.1 28.7

277 24.9 19.8 29.6





#95

Dibenzo(a,h)anthracene

Concen: 22.256 ng/ul

RT: 26.127 min Scan# 3935

Delta R.T. -0.006 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07

Instrument :

BNA_P

ClientSampleId :

SICV616





Tgt Ion:278 Resp: 1747364

Ion Ratio Lower Upper

278 100

139 14.6 12.8 19.2

279 23.8 19.4 29.2

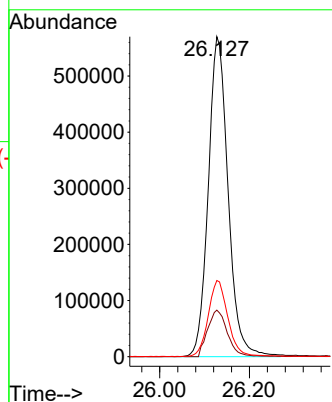

#96

Benzo(g,h,i)perylene

Concen: 22.255 ng/ul

RT: 26.874 min Scan# 4061

Delta R.T. -0.006 min

Lab File: BP012592.D

Acq: 09 Nov 2022 17:07

Tgt Ion:276 Resp: 1727509

Ion Ratio Lower Upper

276 100

138 19.8 17.0 25.6

277 23.7 19.4 29.0

