
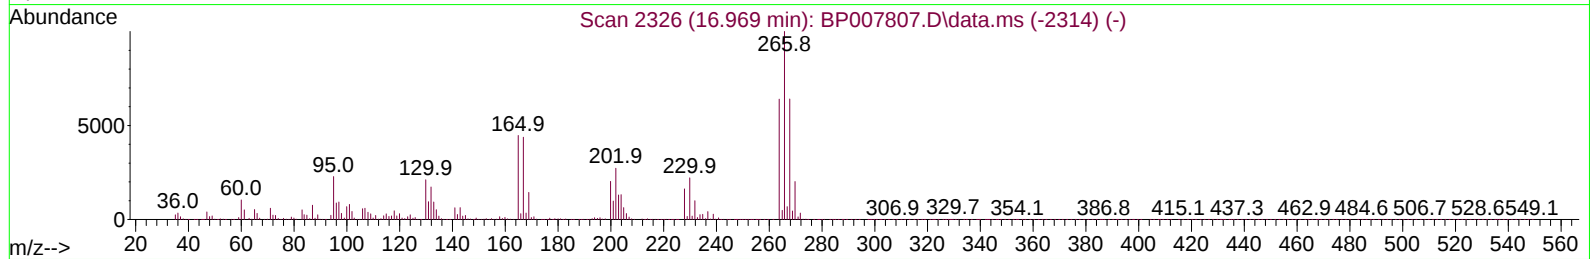
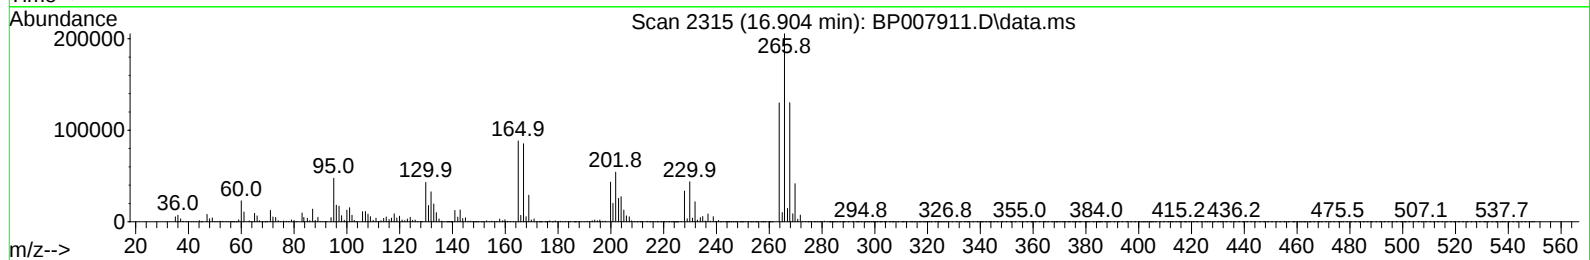


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111021\
 Data File : BP007911.D
 Acq On : 10 Nov 2021 09:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 13:10:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 10:45:24 2021
 Response via : Initial Calibration

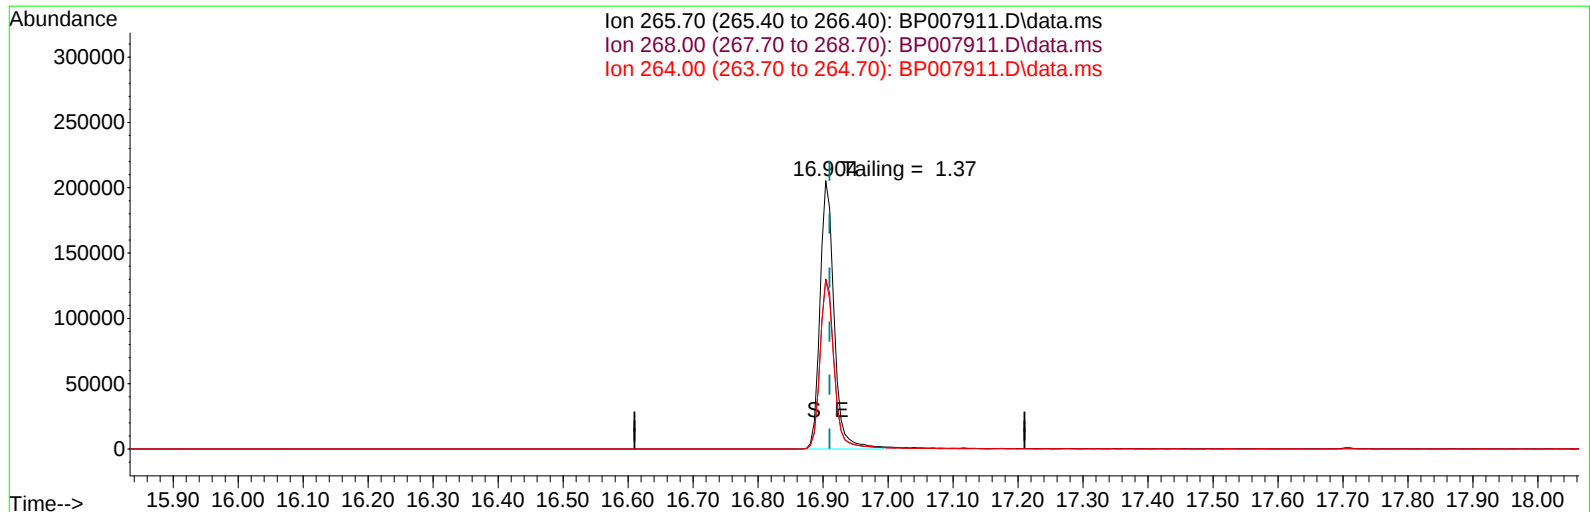

TIC: BP007911.D\data.ms

(70) Pentachlorophenol (C)




16.904min (-0.006) 2332106.01 ng

response 314993

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	63.30
264.00	60.90	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111021\
 Data File : BP007911.D
 Acq On : 10 Nov 2021 09:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 13:10:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 10:45:24 2021
 Response via : Initial Calibration

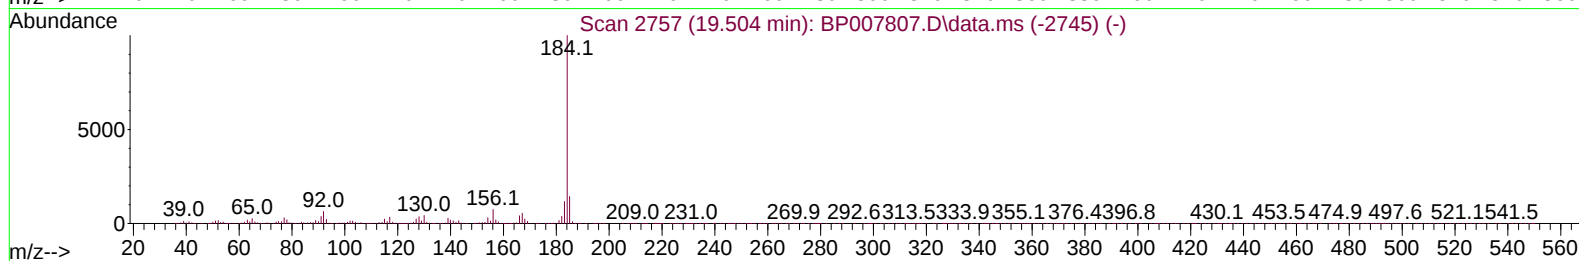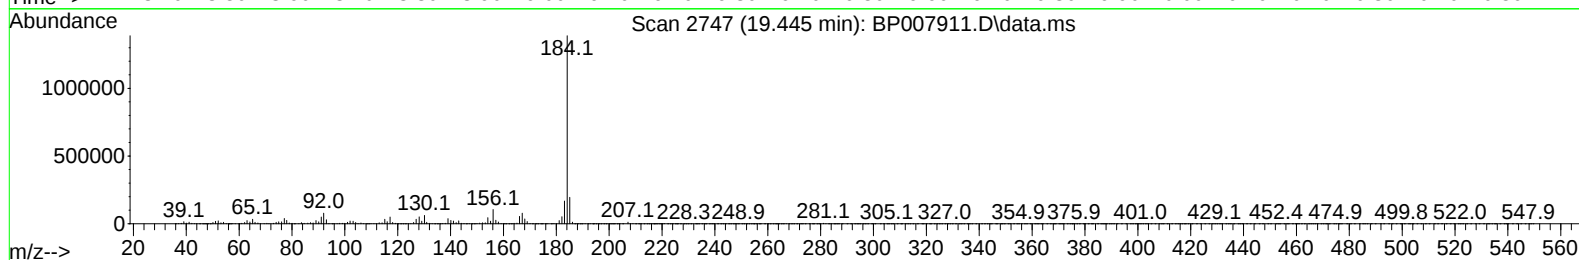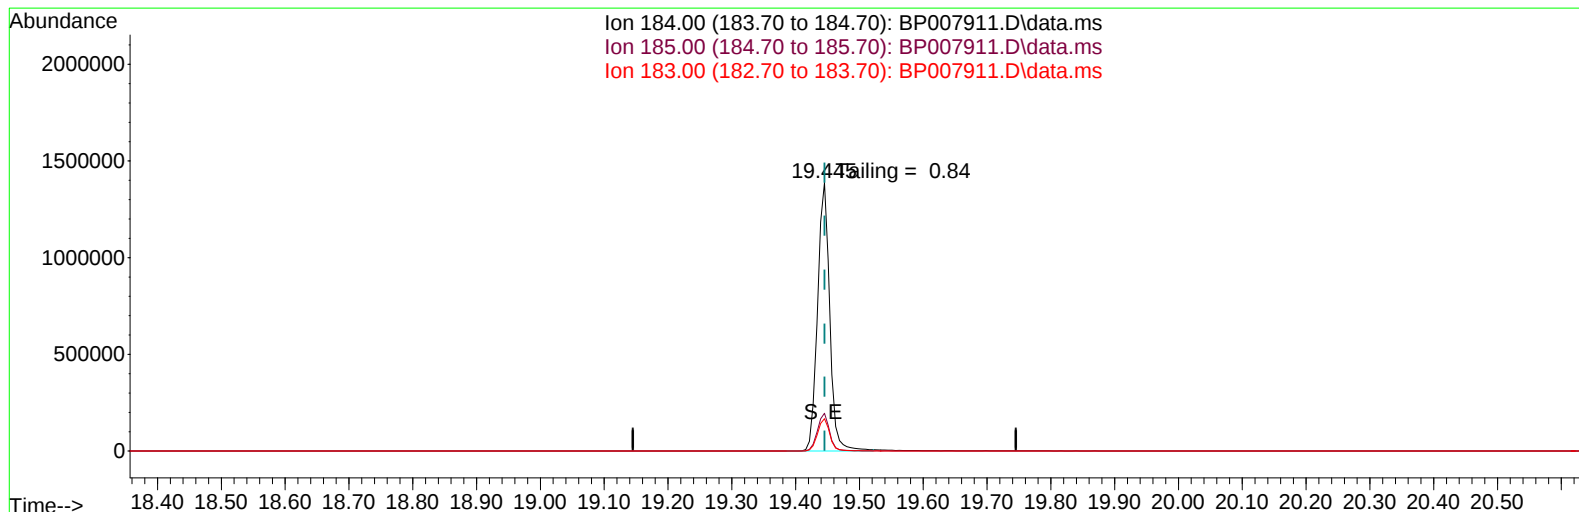

TIC: BP007911.D\data.ms

(77) Benzidine**19.445min (-0.000) 1296903.25 ng****response 1863087**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.08
183.00	11.40	12.09
0.00	0.00	0.00