

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111021\
Data File : BP007922.D
Acq On : 10 Nov 2021 16:31
Operator : CG/JU
Sample : PB140662BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140662BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007922.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.446	360	367	378	rBV	2551042	3691609	30.18%	8.133%
2	7.040	629	638	658	rBV	2309631	3814562	31.18%	8.404%
3	7.858	769	777	785	rBV	489396	777762	6.36%	1.713%
4	9.016	966	974	988	rBV	1326130	2218814	18.14%	4.888%
5	10.657	1242	1253	1266	rBV	600240	1029847	8.42%	2.269%
6	13.122	1663	1672	1689	rBV	3786783	5907120	48.29%	13.013%
7	14.492	1898	1905	1919	rBV	987951	1585899	12.96%	3.494%
8	15.987	2149	2159	2186	rBV	3556346	5710202	46.68%	12.580%
9	17.251	2367	2374	2386	rBV	1489427	2218107	18.13%	4.887%
10	19.816	2804	2810	2821	rBV	9717125	12232246	100.00%	26.948%
11	21.345	3065	3070	3079	rBV	2303315	3054442	24.97%	6.729%
12	23.757	3473	3480	3490	rVB2	1503207	3151683	25.77%	6.943%




Sum of corrected areas: 45392293

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111021\
Data File : BP007922.D
Acq On : 10 Nov 2021 16:31
Operator : CG/JU
Sample : PB140662BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140662BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

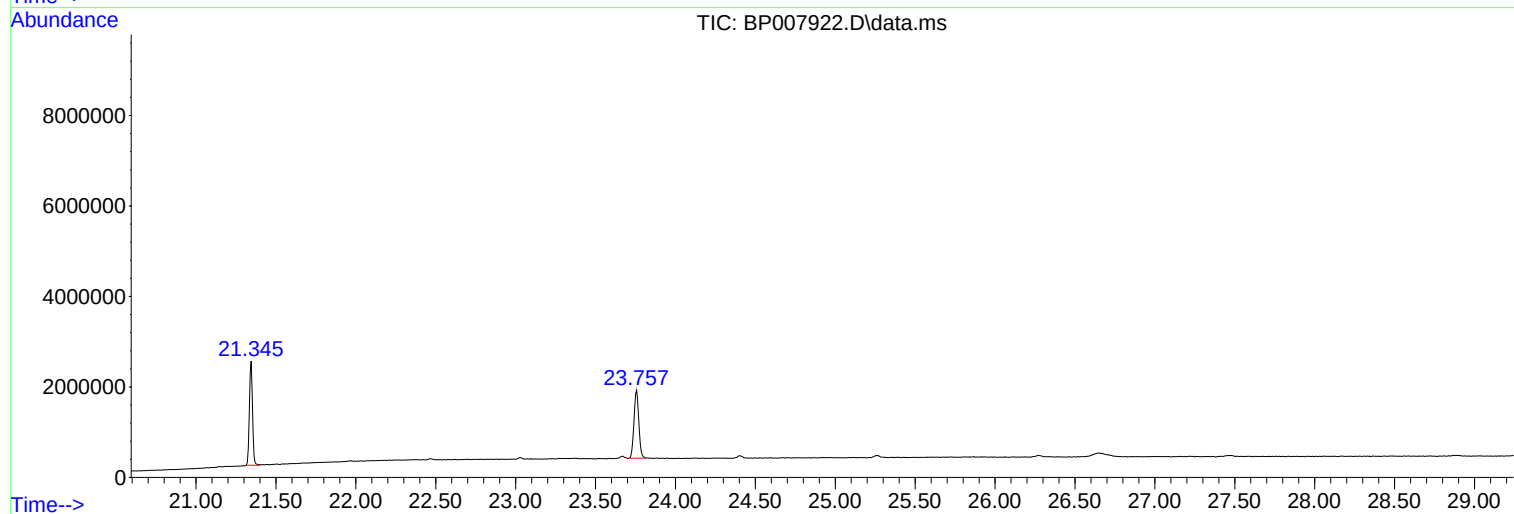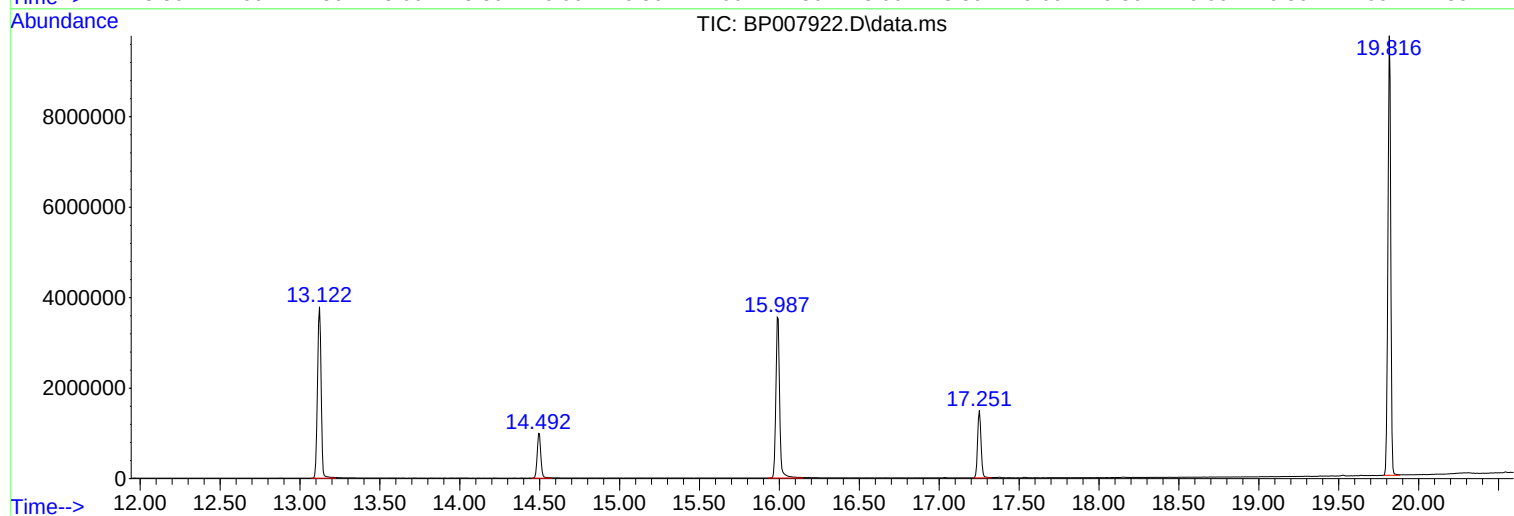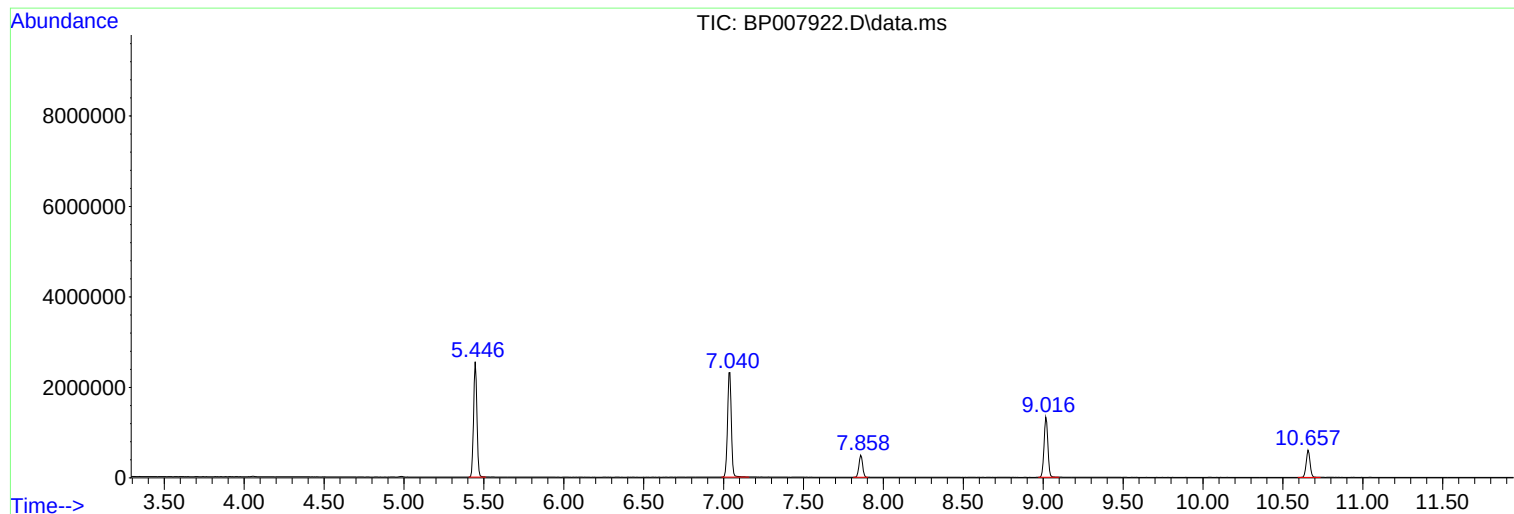

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111021\
Data File : BP007922.D
Acq On : 10 Nov 2021 16:31
Operator : CG/JU
Sample : PB140662BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140662BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111021\
Data File : BP007922.D
Acq On : 10 Nov 2021 16:31
Operator : CG/JU
Sample : PB140662BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140662BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------