
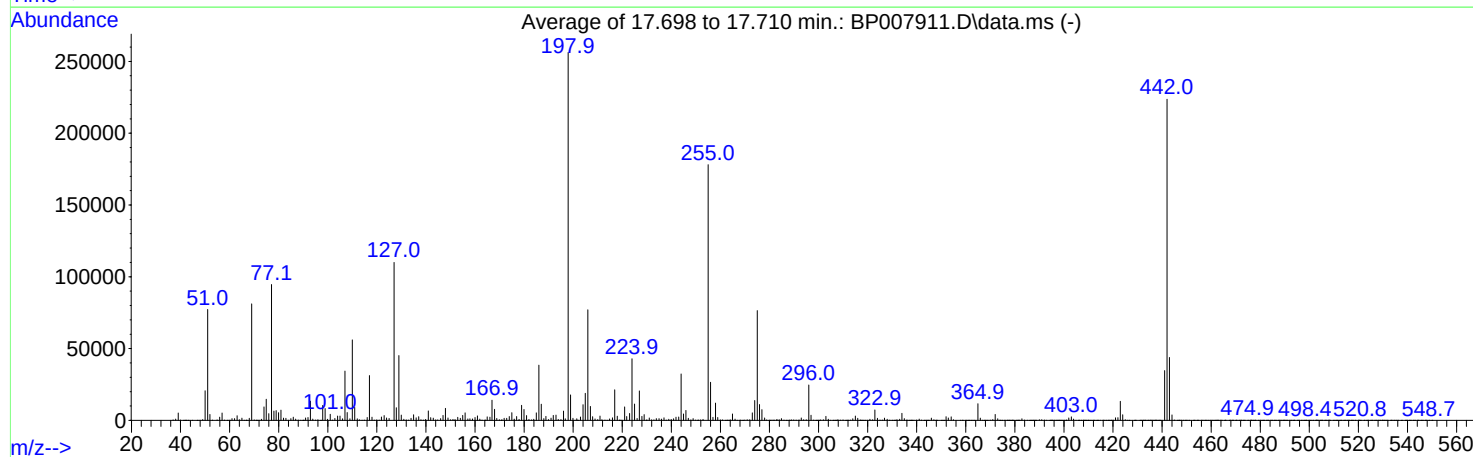


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111021\
 Data File : BP007911.D
 Acq On : 10 Nov 2021 09:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 11 13:53:53 2021

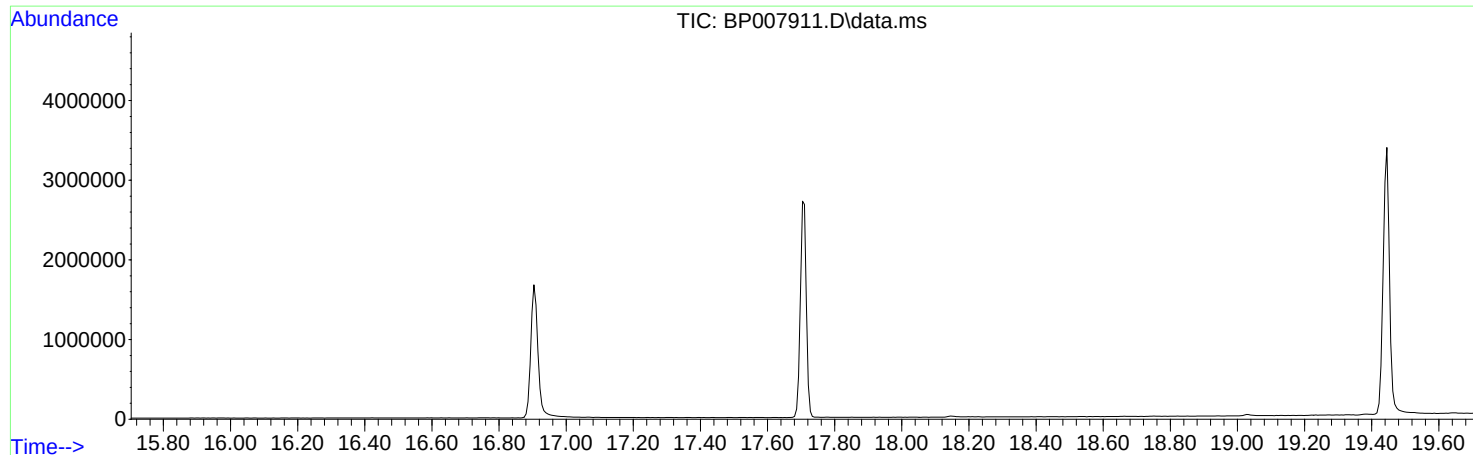




AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	77190	PASS
68	69	0.00	2	1.9	1514	PASS
69	198	0.00	100	31.7	81152	PASS
70	69	0.00	2	0.5	389	PASS
127	198	10	80	42.9	110034	PASS
197	198	0.00	2	0.4	1077	PASS
198	198	100	100	100.0	256202	PASS
199	198	5	9	6.9	17696	PASS
275	198	10	60	29.9	76483	PASS
365	198	1	100	4.5	11653	PASS
441	198	0.01	100	13.5	34692	PASS
442	442	100	100	100.0	223725	PASS
443	442	15	24	19.6	43789	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111021\
 Data File : BP007911.D
 Acq On : 10 Nov 2021 09:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 10 13:10:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 10:45:24 2021
 Response via : Initial Calibration

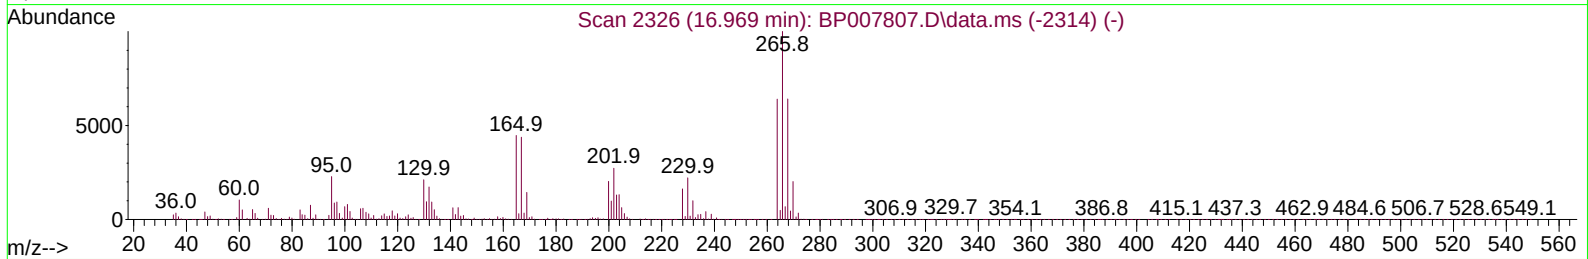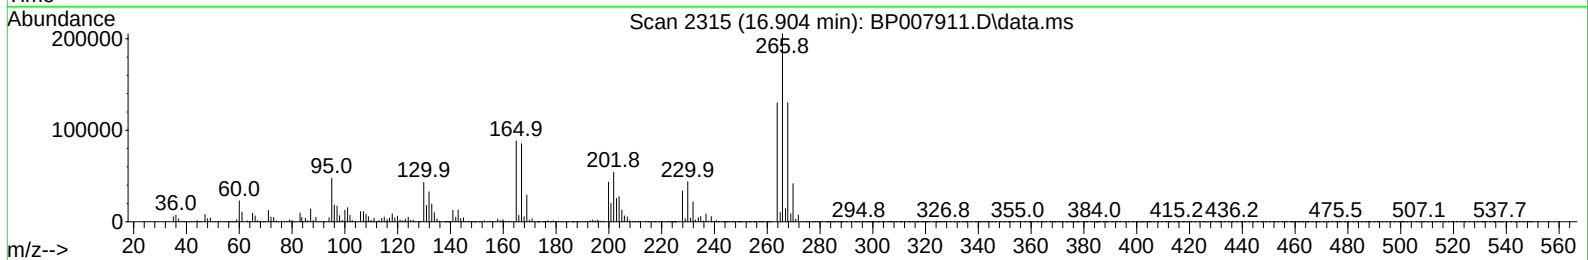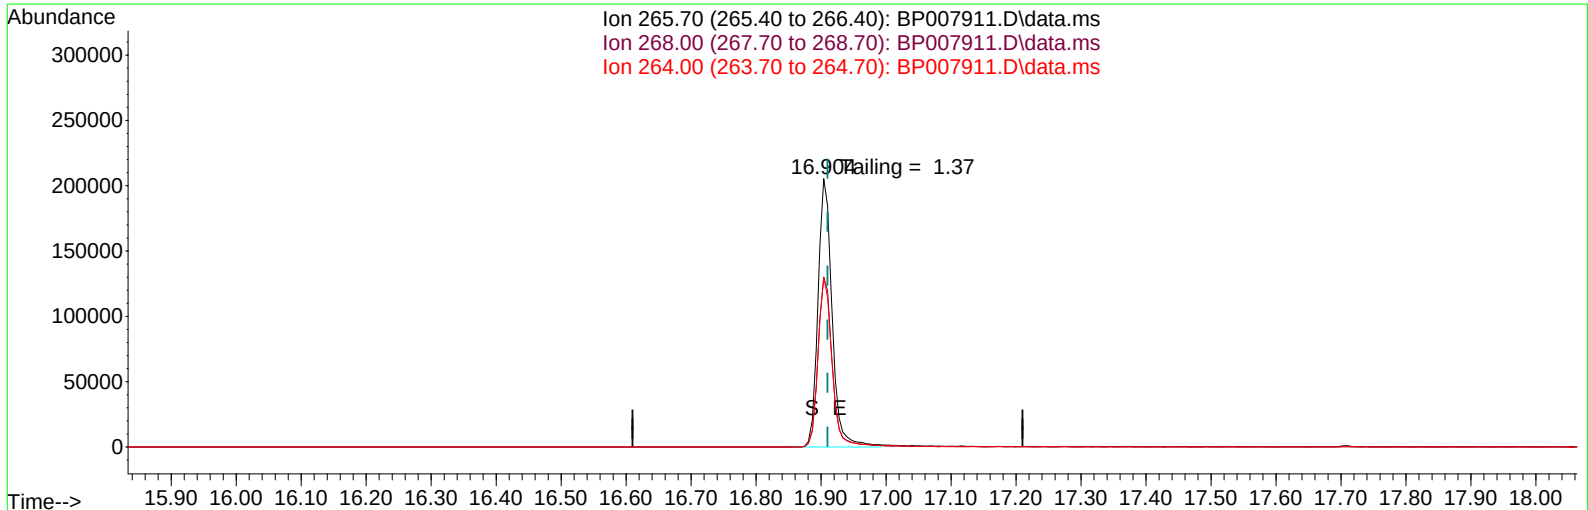

TIC: BP007911.D\data.ms

(70) Pentachlorophenol (C)

16.904min (-0.006) 2332106.01 ng




response 314993

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	63.30
264.00	60.90	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111021\
Data File : BP007911.D
Acq On : 10 Nov 2021 09:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 10 13:10:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 10:45:24 2021
Response via : Initial Calibration

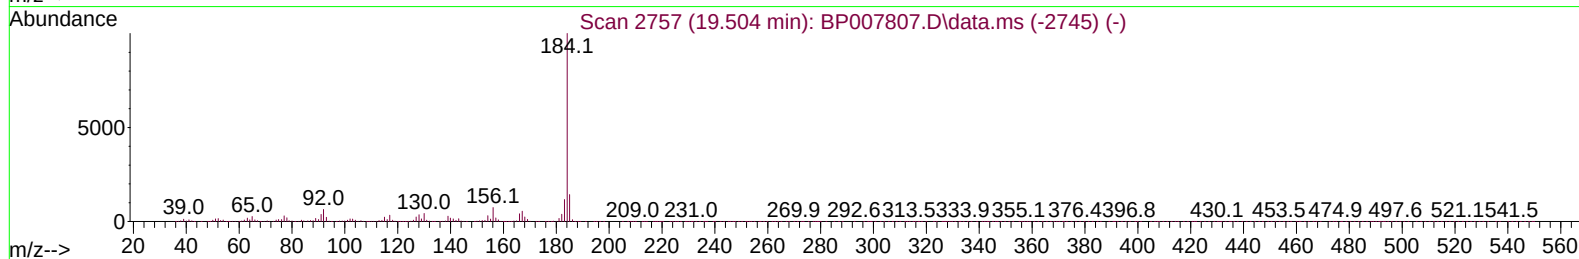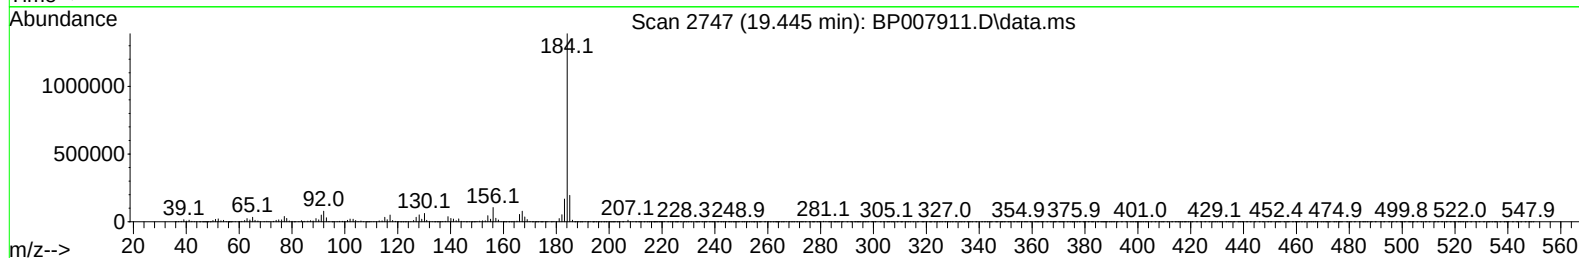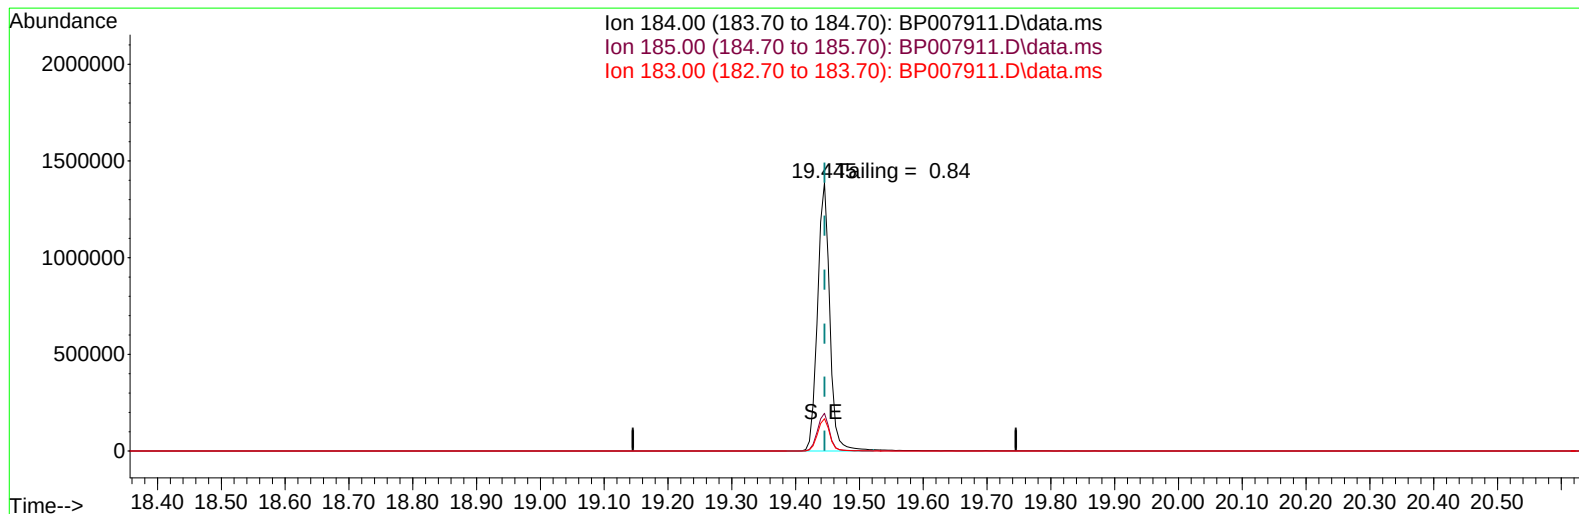

TIC: BP007911.D\data.ms

(77) Benzidine

19.445min (-0.000) 1296903.25 ng

response 1863087

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.08
183.00	11.40	12.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/10/2021	BNA_P	<u>BP007911.D</u>
Compound Name	Response	Retention Time
DDT	1033796	20.65
DDD	24910	20.22
DDE	2338	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27248	1061044	2.57

Instrument :
BNA_P
ClientSampleId :
DFTPP