
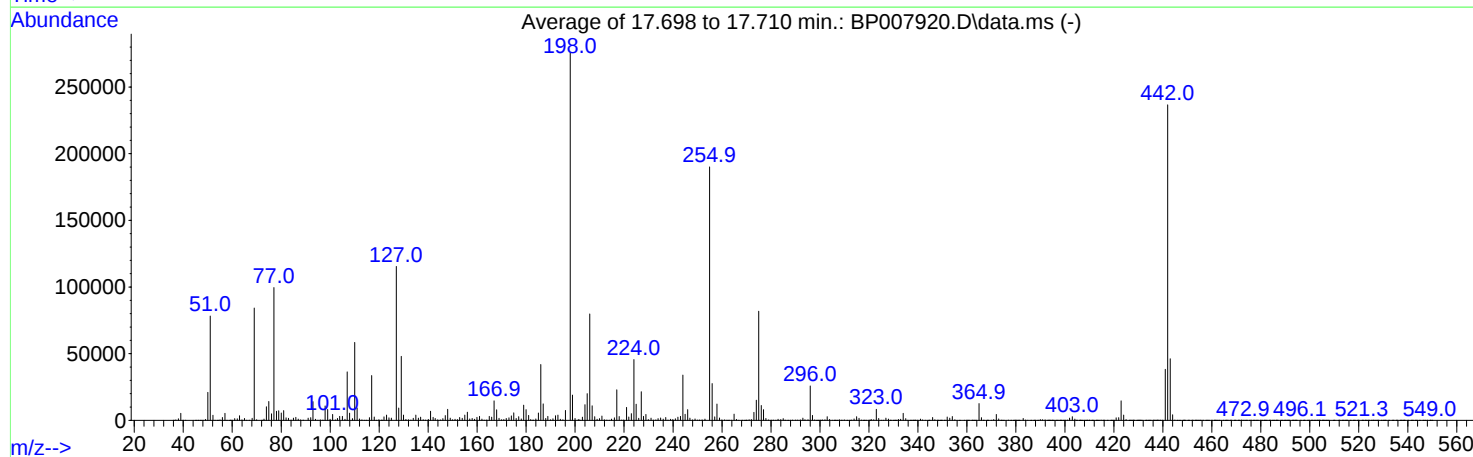


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111021\
 Data File : BP007920.D
 Acq On : 10 Nov 2021 15:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 11 13:53:53 2021

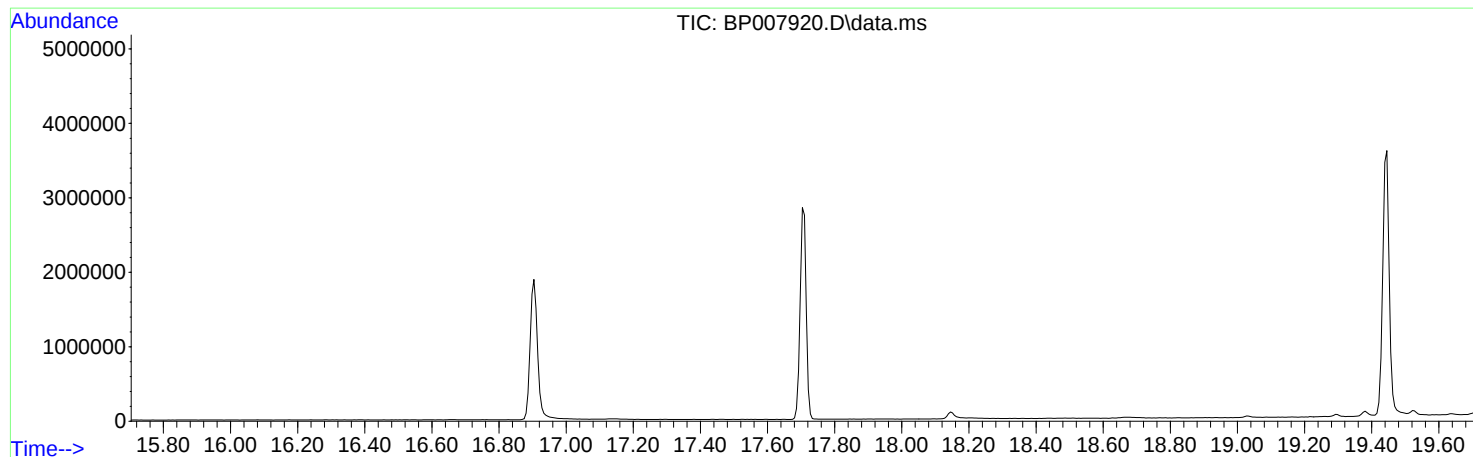




AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	78221	PASS
68	69	0.00	2	1.9	1597	PASS
69	198	0.00	100	30.5	84248	PASS
70	69	0.00	2	0.5	440	PASS
127	198	10	80	41.8	115456	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	275883	PASS
199	198	5	9	6.9	18938	PASS
275	198	10	60	29.7	81813	PASS
365	198	1	100	4.6	12659	PASS
441	198	0.01	100	13.9	38301	PASS
442	442	100	100	100.0	236669	PASS
443	442	15	24	19.5	46234	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111021\
 Data File : BP007920.D
 Acq On : 10 Nov 2021 15:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 10 17:19:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 10:45:24 2021
 Response via : Initial Calibration

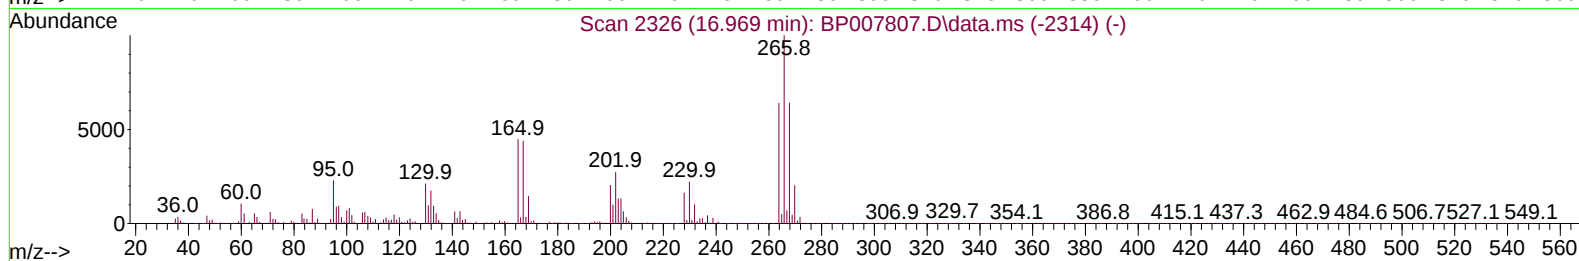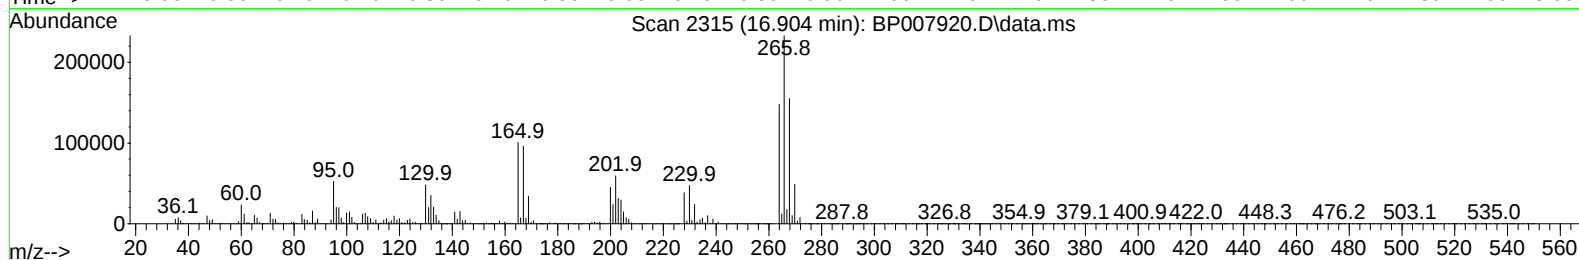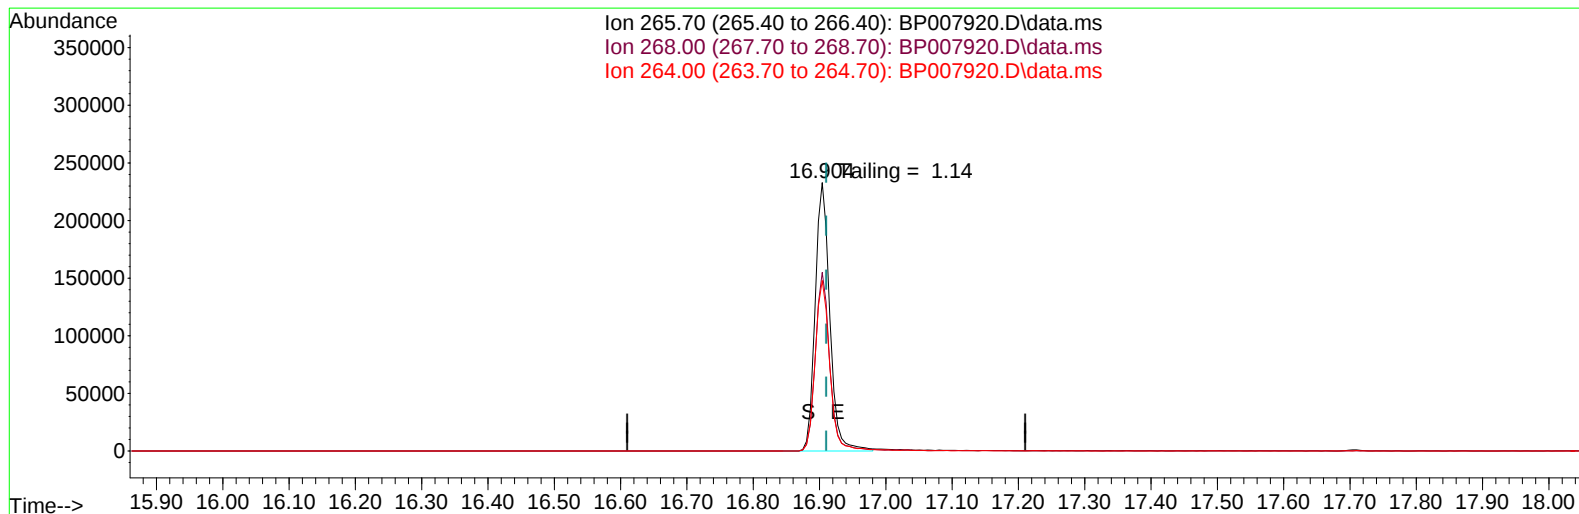

TIC: BP007920.D\data.ms

(70) Pentachlorophenol (C)

16.904min (-0.006) 206108.65 ng




response 361903

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	66.53
264.00	60.90	63.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111021\
Data File : BP007920.D
Acq On : 10 Nov 2021 15:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 10 17:19:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 10:45:24 2021
Response via : Initial Calibration

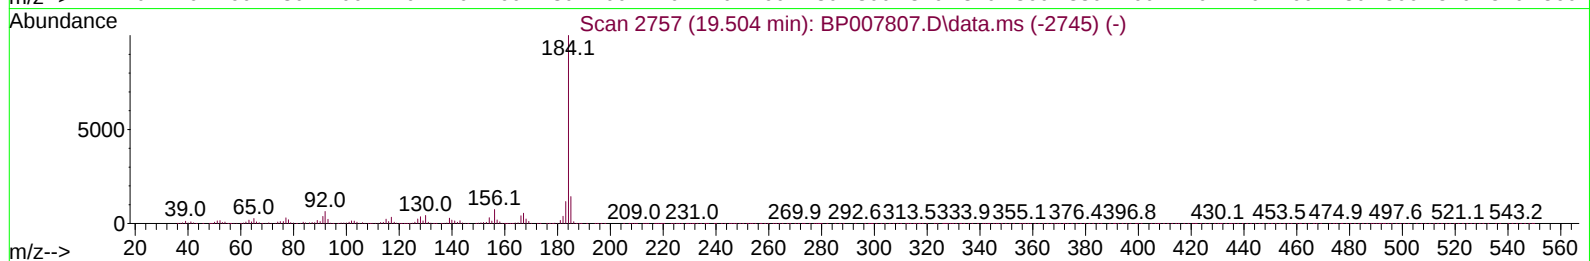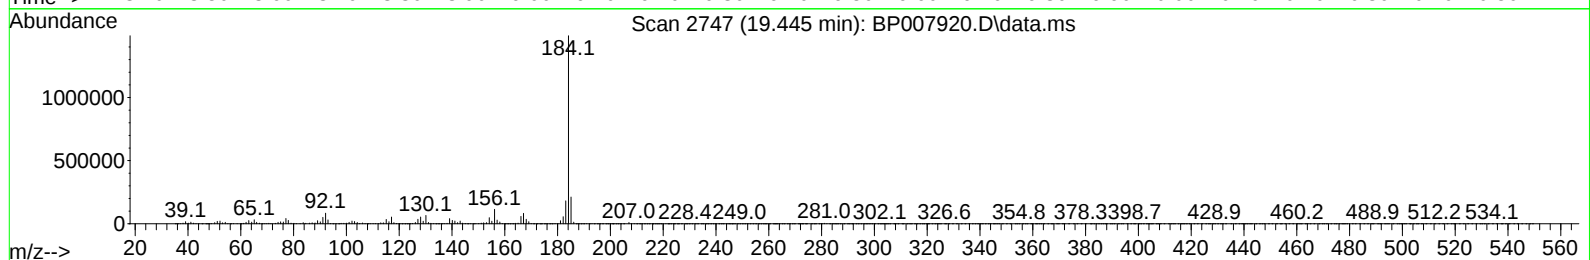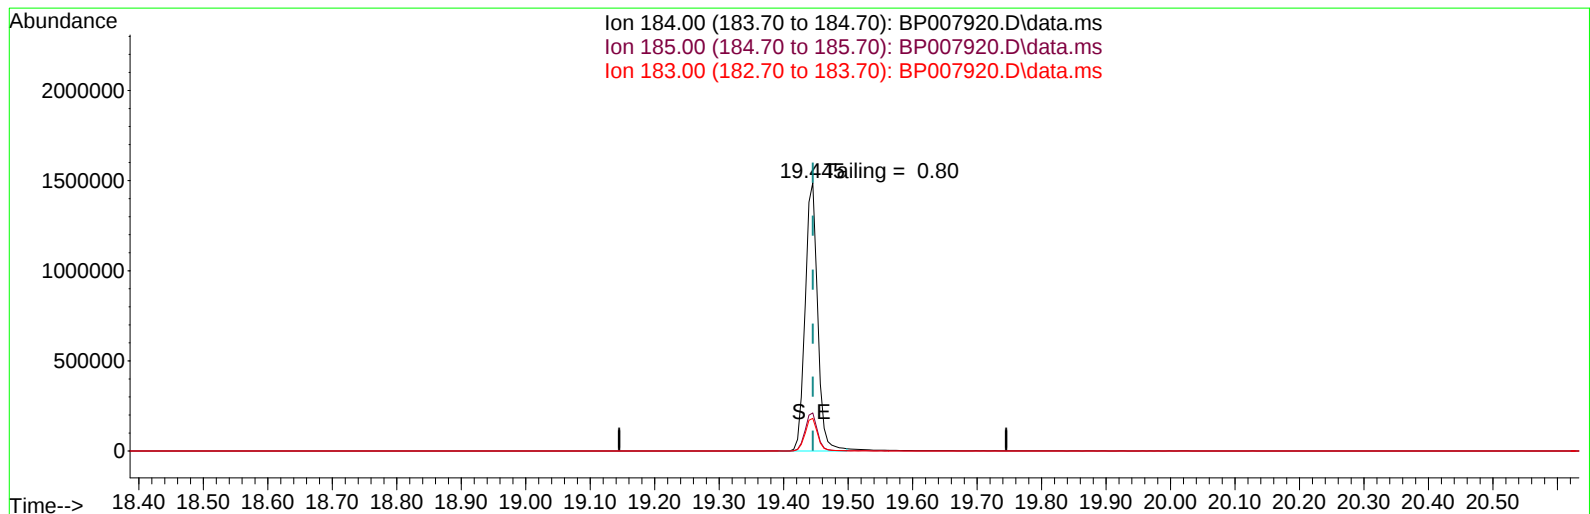

TIC: BP007920.D\data.ms

(77) Benzidine

19.445min (-0.000) 56799.72 ng

response 2035619

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.20
183.00	11.40	12.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/10/2021	BNA_P	<u>BP007920.D</u>
Compound Name	Response	Retention Time
DDT	1154856	20.65
DDD	19748	20.22
DDE	2541	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22289	1177145	1.89