

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
 Data File : BP012605.D
 Acq On : 10 Nov 2022 18:24
 Operator : CG/JU
 Sample : N5493-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA5

Quant Time: Nov 10 21:36:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 09 23:28:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	245823	20.000	ng/u1	0.00
20) Naphthalene-d8	10.557	136	1143141	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.416	164	777114	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.181	188	1705628	20.000	ng/u1	0.00
79) Chrysene-d12	21.280	240	1816447	20.000	ng/u1	0.00
88) Perylene-d12	23.651	264	1881351	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	23960	3.973	ng/uL	0.00
4) Pyridine-d5	3.652	84	130164	7.637	ng/u1	0.01
7) Phenol-d5	6.952	99	108756	5.248	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.099	67	370331	29.868	ng/u1	0.00
11) 2-Chlorophenol-d4	7.299	132	338294	21.214	ng/u1	0.00
15) 4-Methylphenol-d8	8.487	113	217861	13.290	ng/u1	0.00
21) Nitrobenzene-d5	8.928	128	240419	28.424	ng/u1	0.00
24) 2-Nitrophenol-d4	9.652	143	238263	25.647	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	385118	23.010	ng/u1	0.00
31) 4-Chloroaniline-d4	10.710	131	572039	24.265	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	1597580	29.825	ng/u1	0.00
49) Acenaphthylene-d8	14.104	160	1720817	28.398	ng/u1	0.00
54) 4-Nitrophenol-d4	14.698	143	29955	3.552	ng/u1	0.03
60) Fluorene-d10	15.416	176	1432708	31.545	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	235363	24.949	ng/u1	0.00
73) Anthracene-d10	17.275	188	2517167	33.984	ng/u1	0.00
81) Pyrene-d10	19.522	212	2936104	28.844	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.498	264	3090230	33.320	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.252	88	8901	1.382 ng/uL	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012605.D
Acq On : 10 Nov 2022 18:24
Operator : CG/JU
Sample : N5493-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA5

Quant Time: Nov 10 21:36:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 09 23:28:28 2022
Response via : Initial Calibration

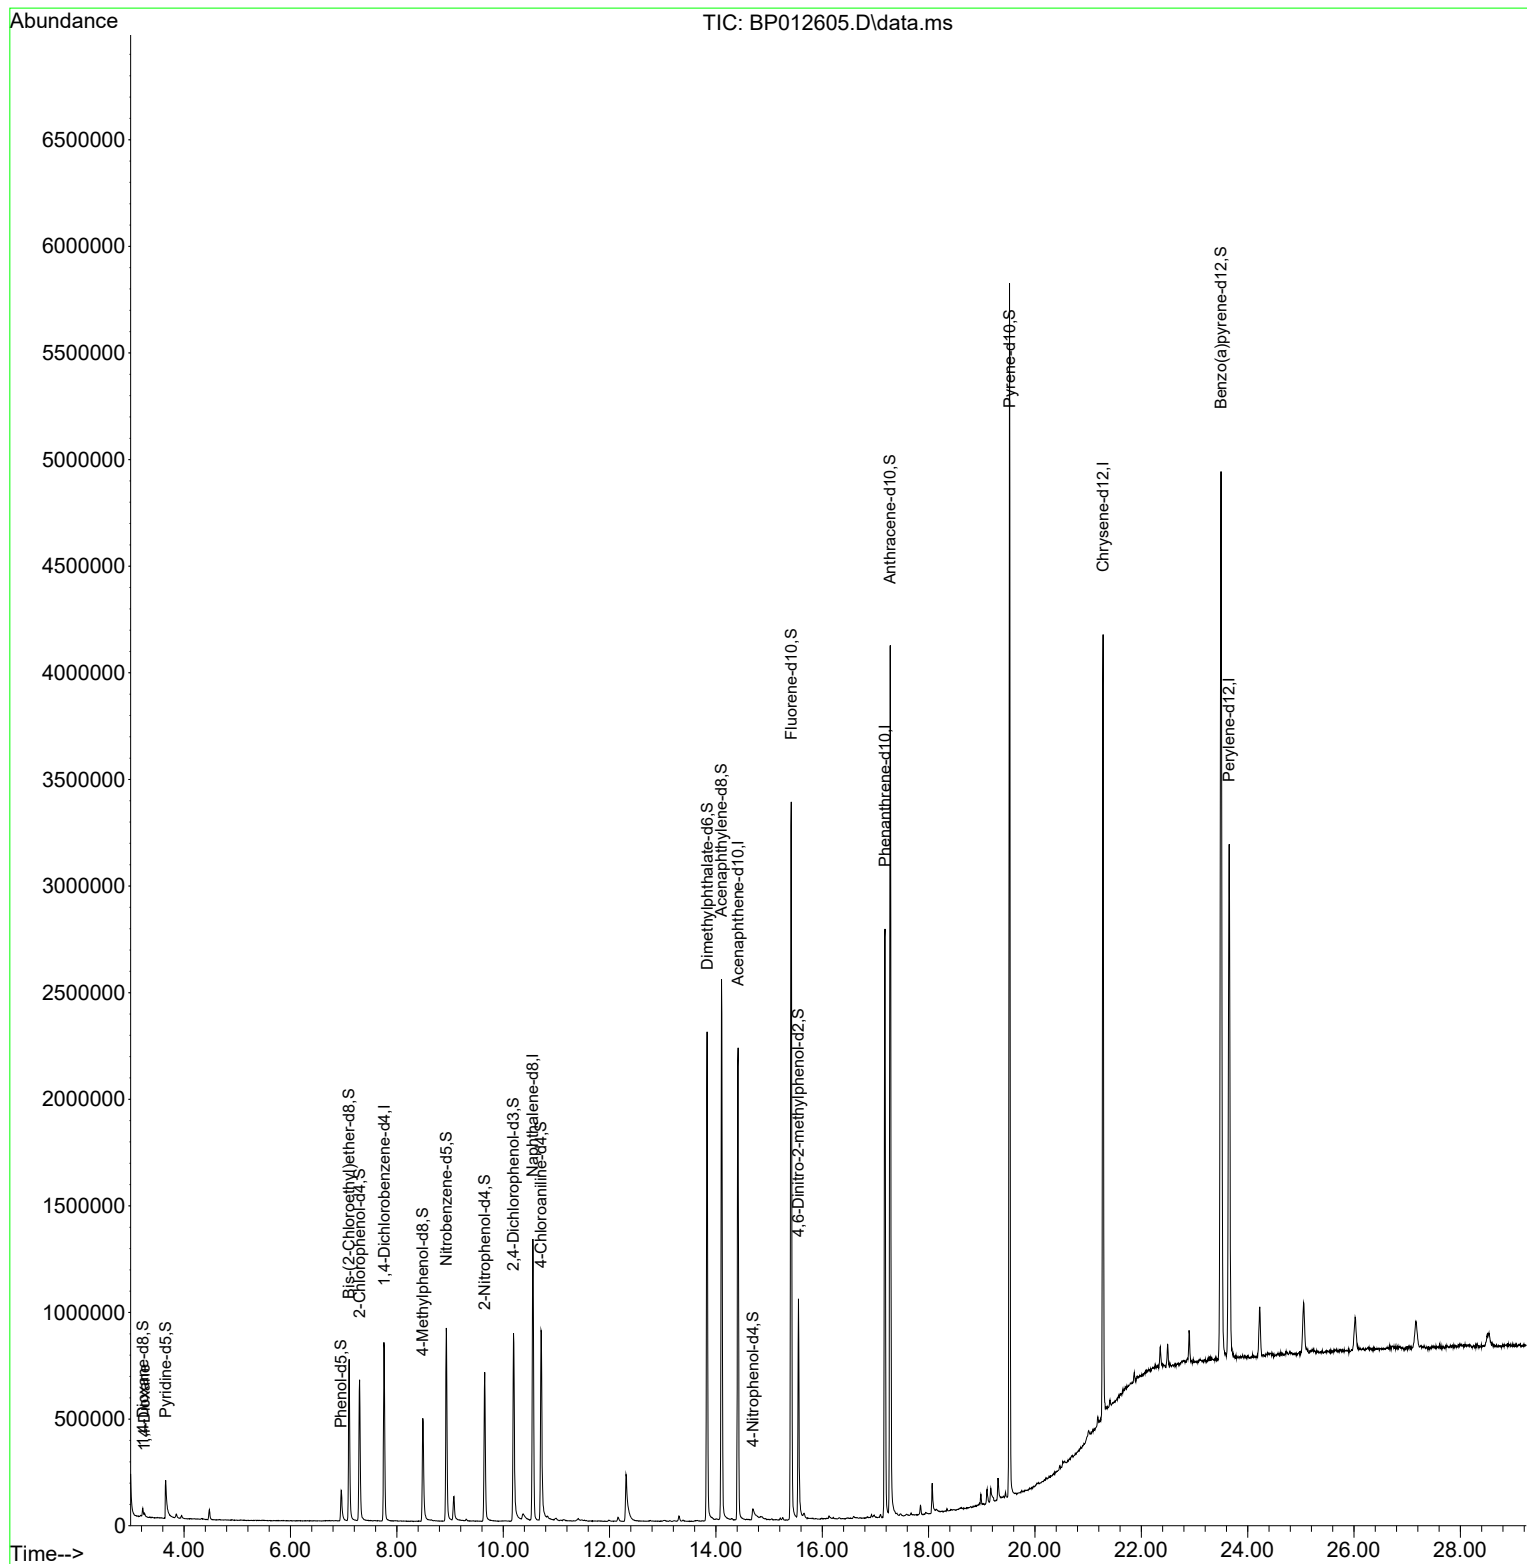

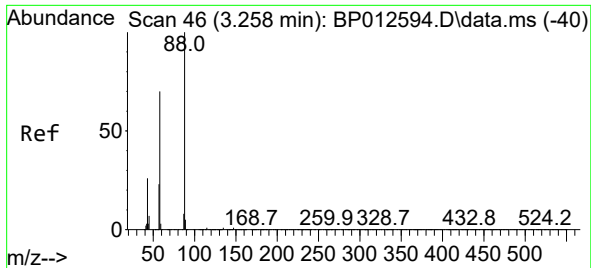

#2
 1,4-Dioxane
 Concen: 1.382 ng/uL
 RT: 3.252 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: BP012605.D
 Acq: 10 Nov 2022 18:24

Instrument :
 BNA_P
 ClientSampleId :
 H0AA5

Tgt Ion: 88	Resp:	8901
Ion	Ratio	Lower Upper
88	100	
43	24.9	18.9 28.3
58	62.5	57.8 86.8

