

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
 Data File : BP012601.D
 Acq On : 10 Nov 2022 16:06
 Operator : CG/JU
 Sample : N5493-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AC6

Quant Time: Nov 10 21:35:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 09 23:28:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.764	152	237821	20.000	ng/u1	0.00
20) Naphthalene-d8	10.563	136	1114155	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.416	164	738326	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.181	188	1646624	20.000	ng/u1	0.00
79) Chrysene-d12	21.280	240	1788427	20.000	ng/u1	0.00
88) Perylene-d12	23.657	264	1860337	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	23884	4.093	ng/uL	0.00
4) Pyridine-d5	3.652	84	143775	8.719	ng/u1	0.01
7) Phenol-d5	6.952	99	123240	6.147	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.105	67	401787	33.495	ng/u1	0.00
11) 2-Chlorophenol-d4	7.299	132	375728	24.354	ng/u1	0.00
15) 4-Methylphenol-d8	8.493	113	249474	15.731	ng/u1	0.00
21) Nitrobenzene-d5	8.934	128	268001	32.509	ng/u1	0.00
24) 2-Nitrophenol-d4	9.652	143	268732	29.679	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.199	165	440866	27.027	ng/u1	0.00
31) 4-Chloroaniline-d4	10.716	131	620788	27.018	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	1742952	34.249	ng/u1	0.00
49) Acenaphthylene-d8	14.110	160	1920359	33.356	ng/u1	0.00
54) 4-Nitrophenol-d4	14.693	143	31239	3.899	ng/u1	0.02
60) Fluorene-d10	15.416	176	1520471	35.236	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	251736	27.641	ng/u1	0.00
73) Anthracene-d10	17.281	188	2508250	35.077	ng/u1	0.00
81) Pyrene-d10	19.522	212	3009512	30.029	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.498	264	3212088	35.025	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.258	88	10574	1.696	ng/uL	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012601.D
Acq On : 10 Nov 2022 16:06
Operator : CG/JU
Sample : N5493-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AC6


Quant Time: Nov 10 21:35:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 09 23:28:28 2022
Response via : Initial Calibration

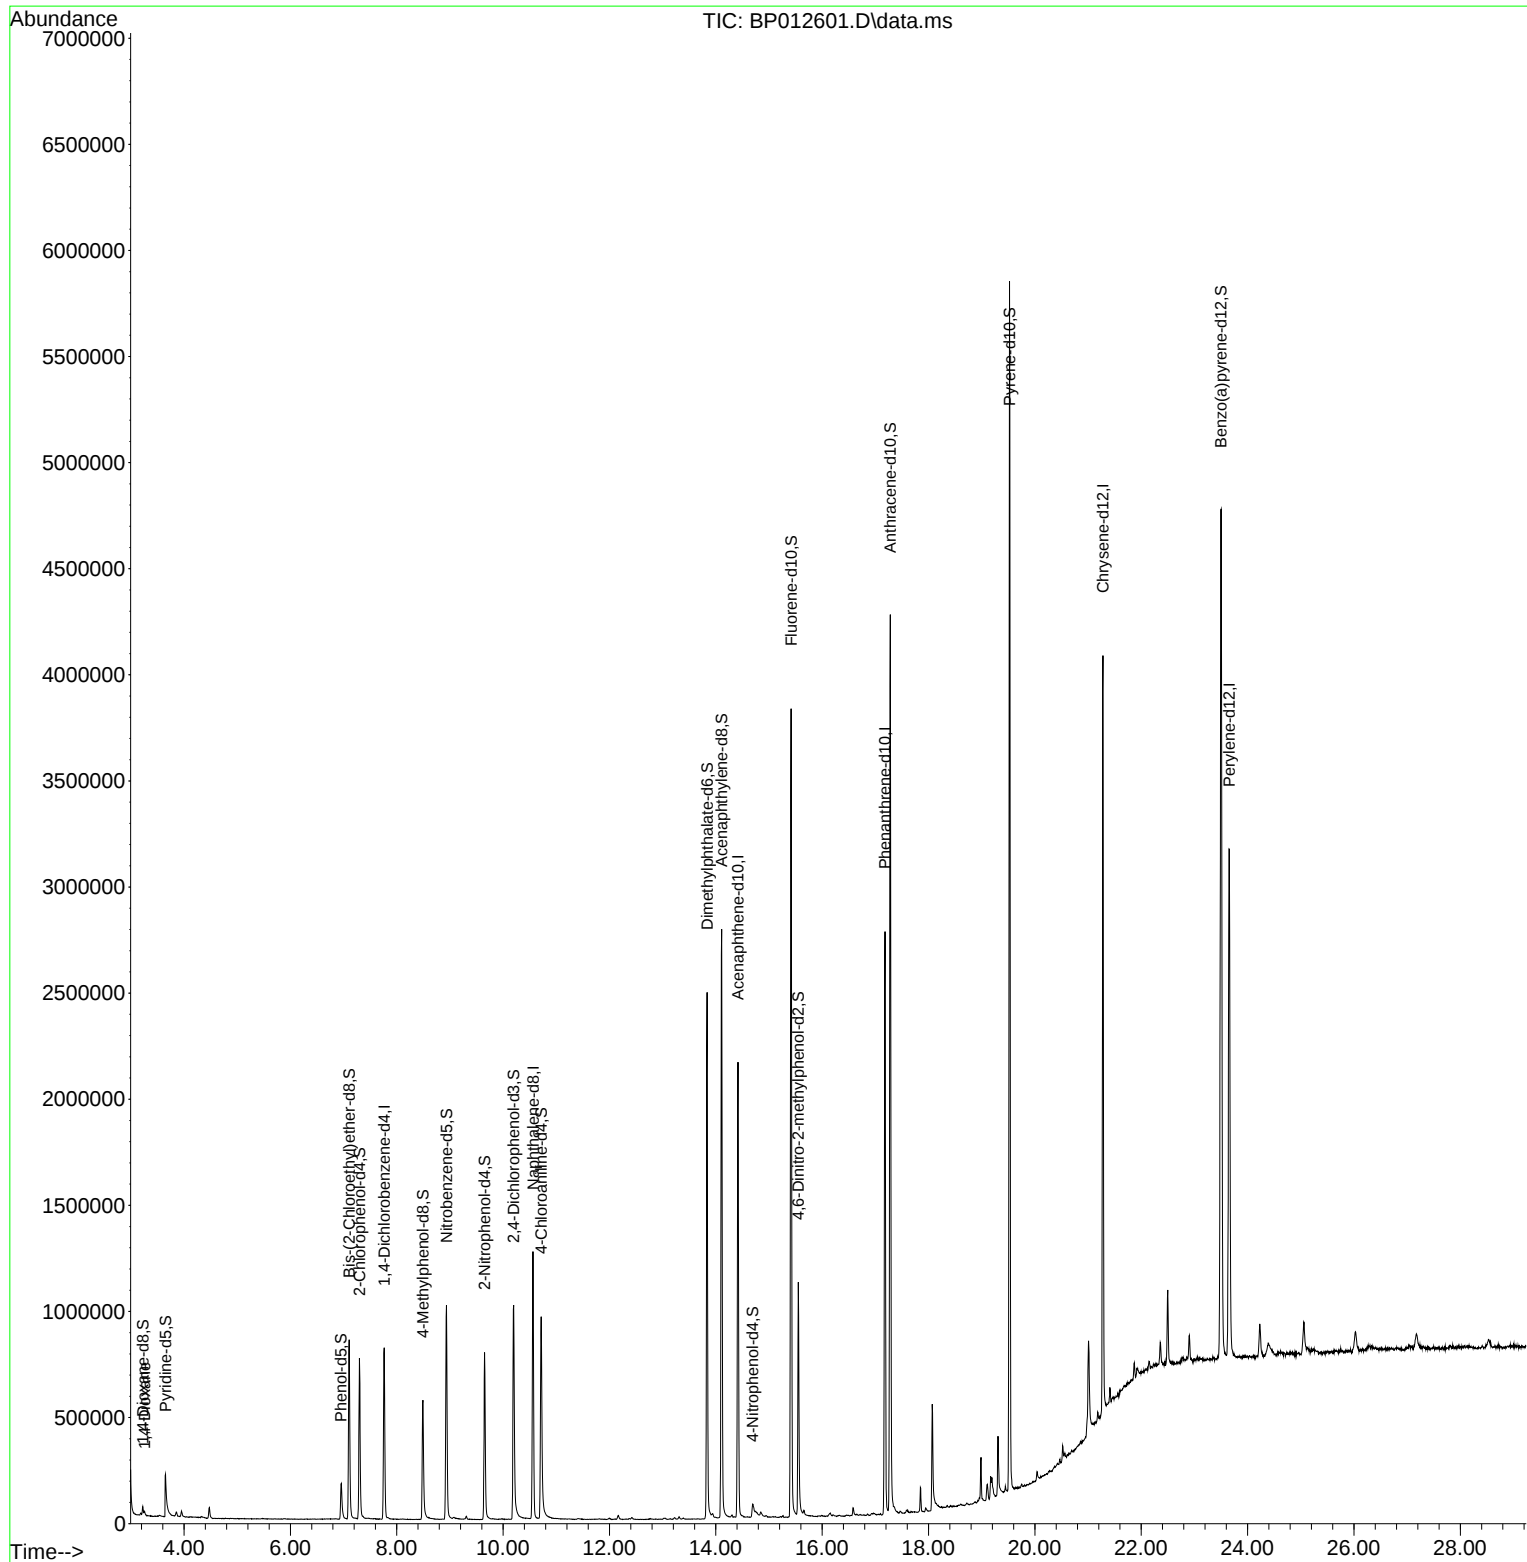

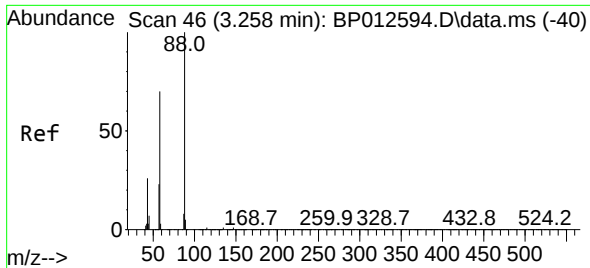

#2
 1,4-Dioxane
 Concen: 1.696 ng/uL
 RT: 3.258 min Scan# 40
 Delta R.T. -0.000 min
 Lab File: BP012601.D
 Acq: 10 Nov 2022 16:06

Instrument :
 BNA_P
 ClientSampleId :
 H0AC6

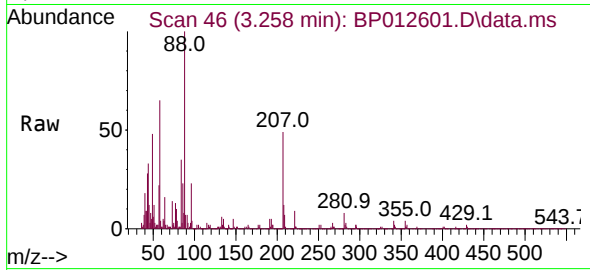

Tgt Ion: 88 Resp: 10574

Ion	Ratio	Lower	Upper
88	100		
43	27.8	18.9	28.3
58	65.0	57.8	86.8

