

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
 Data File : BP012595.D
 Acq On : 10 Nov 2022 12:40
 Operator : CG/JU
 Sample : PB148940BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK940

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012595.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	36	40	51	rVB	56137	87161	1.25%	0.158%
2	3.646	110	112	136	rBV	264823	565461	8.13%	1.027%
3	3.952	161	164	168	rVB3	6188	8776	0.13%	0.016%
4	6.952	667	674	693	rBV	819688	1487583	21.38%	2.701%
5	7.105	693	700	722	rVV	727647	1277663	18.36%	2.320%
6	7.299	726	733	750	rBV	888843	1512494	21.74%	2.746%
7	7.763	806	812	825	rBV	337477	575906	8.28%	1.046%
8	8.487	925	935	953	rBV	1058243	1915746	27.53%	3.478%
9	8.934	1003	1011	1024	rBV	851587	1523296	21.89%	2.766%
10	9.652	1125	1133	1150	rBV	715561	1270338	18.26%	2.306%
11	10.199	1216	1226	1245	rBV	953881	1916685	27.55%	3.480%
12	10.557	1280	1287	1303	rVB	544932	947158	13.61%	1.720%
13	10.722	1308	1315	1340	rVV	331198	780245	11.21%	1.417%
14	12.175	1553	1562	1570	rBV3	14729	38208	0.55%	0.069%
15	13.051	1707	1711	1716	rVB3	5616	9582	0.14%	0.017%
16	13.834	1837	1844	1857	rBV	2198920	3151031	45.29%	5.721%
17	14.110	1883	1891	1910	rBV	2409382	3771194	54.20%	6.847%
18	14.416	1936	1943	1951	rBV	914581	1363060	19.59%	2.475%
19	14.475	1951	1953	1960	rVB6	9799	15056	0.22%	0.027%
20	14.675	1980	1987	2010	rBV	486502	1415007	20.34%	2.569%
21	15.245	2081	2084	2089	rVB5	5410	7213	0.10%	0.013%
22	15.416	2103	2113	2129	rBV	3169913	4875006	70.07%	8.851%
23	15.551	2130	2136	2149	rVV	946952	1455971	20.93%	2.643%
24	15.657	2151	2154	2158	rVB2	12821	18453	0.27%	0.034%
25	15.916	2194	2198	2204	rVB9	6557	11367	0.16%	0.021%
26	16.469	2289	2292	2297	rBV7	4896	7515	0.11%	0.014%
27	16.857	2352	2358	2363	rBV10	6596	14349	0.21%	0.026%
28	17.181	2406	2413	2423	rBV	1119467	1723543	24.77%	3.129%
29	17.281	2423	2430	2447	rVV	3659248	5579709	80.20%	10.131%
30	18.081	2561	2566	2571	rBV6	22866	48788	0.70%	0.089%
31	19.098	2735	2739	2744	rBV2	53060	72468	1.04%	0.132%
32	19.169	2747	2751	2754	rBV	46381	64214	0.92%	0.117%
33	19.522	2805	2811	2824	rBV	4772905	6671281	95.89%	12.112%
34	21.280	3105	3110	3121	rBV	1450730	2103789	30.24%	3.820%
35	23.498	3480	3487	3502	rBV2	3381127	6957556	100.00%	12.632%
36	23.651	3508	3513	3526	rVB2	887205	1834954	26.37%	3.332%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012595.D
Acq On : 10 Nov 2022 12:40
Operator : CG/JU
Sample : PB148940BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Title : SVOA CALIBRATION




Sum of corrected areas: 55077826

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012595.D
Acq On : 10 Nov 2022 12:40
Operator : CG/JU
Sample : PB148940BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

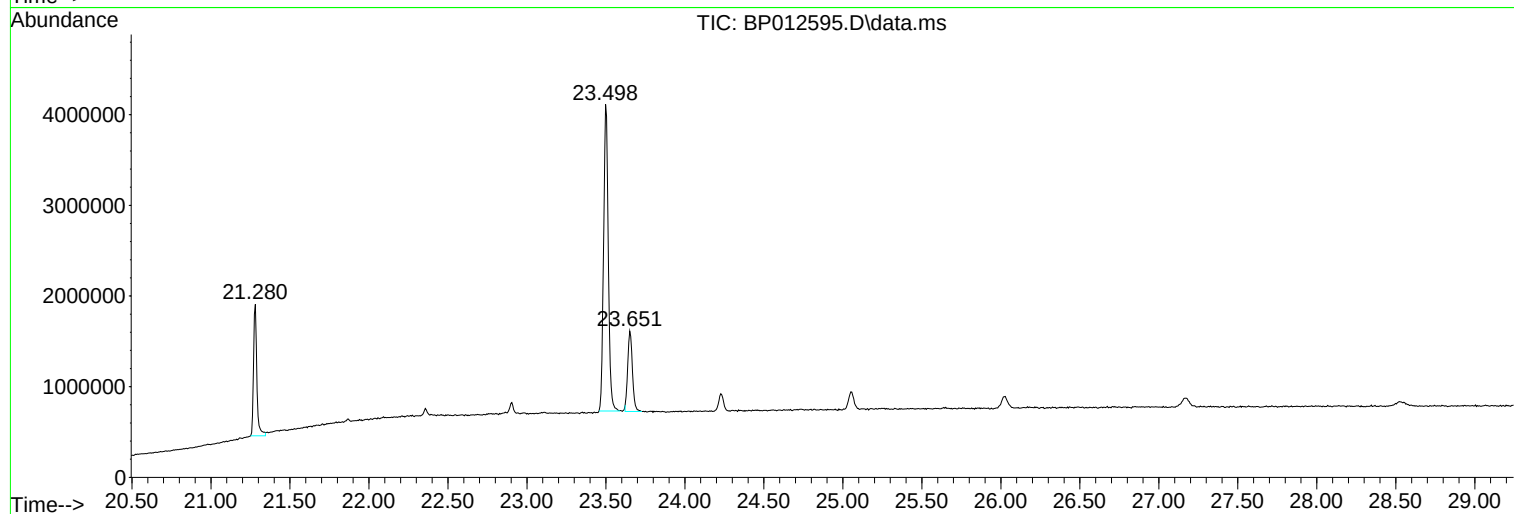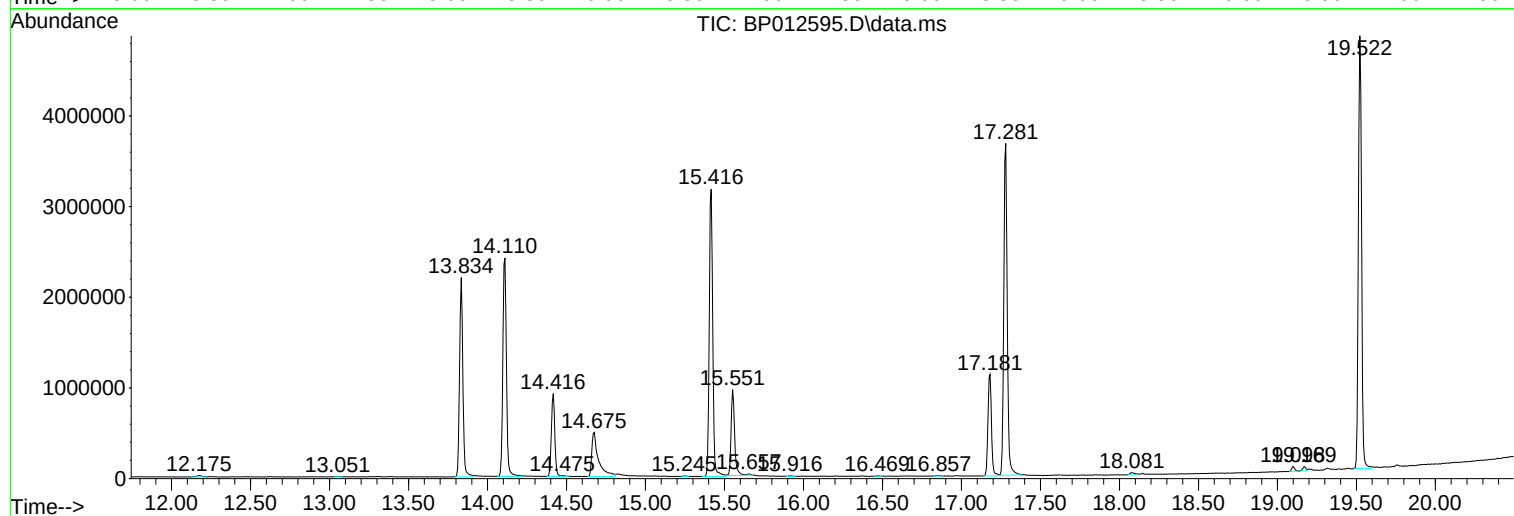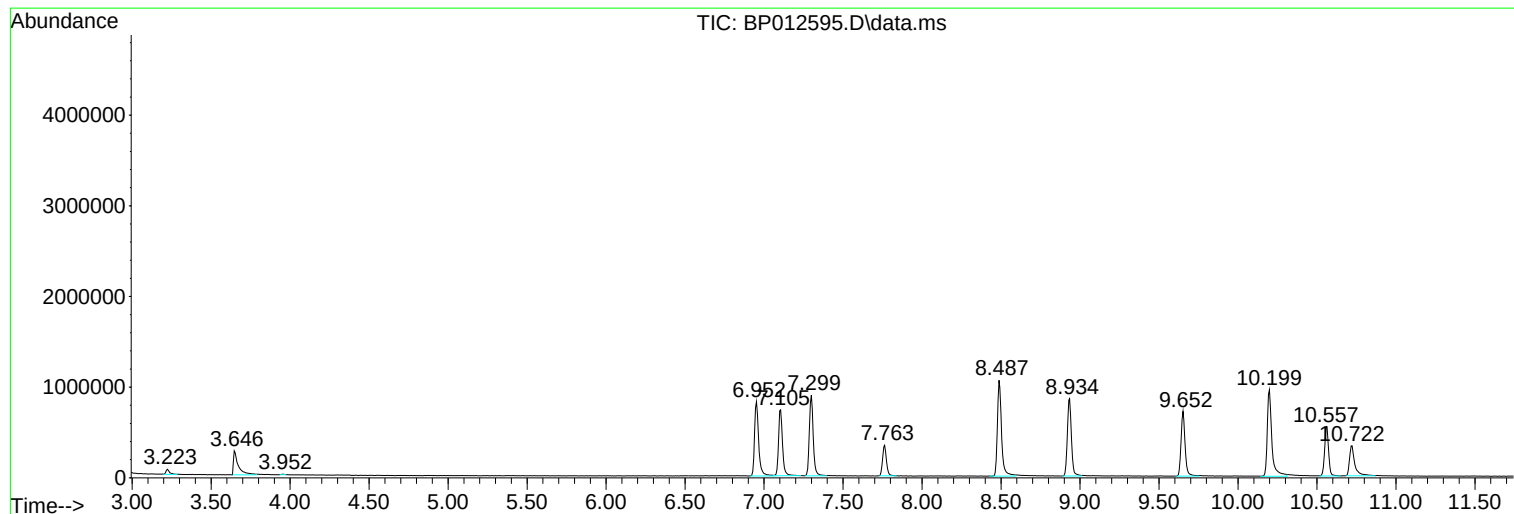

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012595.D
Acq On : 10 Nov 2022 12:40
Operator : CG/JU
Sample : PB148940BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012595.D
Acq On : 10 Nov 2022 12:40
Operator : CG/JU
Sample : PB148940BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc