

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
 Data File : BP012596.D
 Acq On : 10 Nov 2022 13:14
 Operator : CG/JU
 Sample : PB148942BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK942

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012596.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	36	40	51	rVB	61329	100990	1.47%	0.156%
2	3.646	109	112	135	rBV	274244	571018	8.30%	0.882%
3	3.952	160	164	170	rVB	10870	16401	0.24%	0.025%
4	5.369	401	405	411	rVB9	4569	8311	0.12%	0.013%
5	6.952	667	674	694	rBV	897257	1607811	23.37%	2.483%
6	7.105	694	700	722	rVB	805742	1365836	19.86%	2.109%
7	7.299	726	733	748	rBV	942256	1613512	23.46%	2.491%
8	7.763	803	812	826	rBV	680782	1152337	16.75%	1.779%
9	8.240	888	893	898	rBV8	4150	7620	0.11%	0.012%
10	8.487	928	935	962	rBV	1136430	2078154	30.21%	3.209%
11	8.934	1002	1011	1035	rBV	940211	1661625	24.16%	2.566%
12	9.510	1104	1109	1116	rVB3	4443	9643	0.14%	0.015%
13	9.652	1126	1133	1148	rBV	765765	1346714	19.58%	2.079%
14	9.763	1148	1152	1156	rVB7	6658	10803	0.16%	0.017%
15	10.199	1217	1226	1256	rBV	1033800	2075139	30.17%	3.204%
16	10.416	1262	1263	1270	rVB7	5383	8355	0.12%	0.013%
17	10.557	1280	1287	1301	rBV	1061921	1829188	26.59%	2.824%
18	10.716	1307	1314	1338	rBV	471956	1041682	15.14%	1.608%
19	12.169	1554	1561	1568	rBV2	16239	33093	0.48%	0.051%
20	12.246	1572	1574	1579	rVB6	5199	6927	0.10%	0.011%
21	12.375	1591	1596	1602	rVB9	3631	9442	0.14%	0.015%
22	12.457	1605	1610	1615	rBV4	7500	14030	0.20%	0.022%
23	12.610	1633	1636	1640	rBV6	5010	8108	0.12%	0.013%
24	12.869	1674	1680	1689	rVB6	3166	8657	0.13%	0.013%
25	13.046	1705	1710	1718	rVB3	14979	29243	0.43%	0.045%
26	13.263	1740	1747	1750	rBV	7307	12544	0.18%	0.019%
27	13.304	1750	1754	1759	rVV5	8973	15846	0.23%	0.024%
28	13.387	1762	1768	1773	rBV4	5545	11415	0.17%	0.018%
29	13.834	1837	1844	1857	rBV	2220823	3262343	47.43%	5.037%
30	14.110	1884	1891	1910	rBV	2570647	3915147	56.92%	6.045%
31	14.416	1935	1943	1951	rBV	1705668	2590437	37.66%	4.000%
32	14.475	1951	1953	1960	rVB	18986	28800	0.42%	0.044%
33	14.669	1980	1986	2009	rBV	503827	1450311	21.09%	2.239%
34	14.981	2037	2039	2043	rVB5	6404	7217	0.10%	0.011%
35	15.057	2048	2052	2060	rVB10	8227	15246	0.22%	0.024%
36	15.251	2080	2085	2090	rVB	12300	18383	0.27%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
 Data File : BP012596.D
 Acq On : 10 Nov 2022 13:14
 Operator : CG/JU
 Sample : PB148942BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK942

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Title : SVOA CALIBRATION

37	15.416	2106	2113	2121	rBV	3257285	4981706	72.43%	7.692%
38	15.551	2130	2136	2149	rBV	994262	1514722	22.02%	2.339%
39	15.657	2151	2154	2157	rVV3	19735	31334	0.46%	0.048%
40	15.687	2157	2159	2163	rVV3	15385	19111	0.28%	0.030%
41	15.757	2167	2171	2178	rVB2	9003	16496	0.24%	0.025%
42	15.916	2194	2198	2206	rBV7	12696	21709	0.32%	0.034%
43	16.369	2271	2275	2283	rVB9	9397	15643	0.23%	0.024%
44	16.475	2289	2293	2297	rBV6	11430	16484	0.24%	0.025%
45	16.663	2321	2325	2329	rBV7	7112	11103	0.16%	0.017%
46	16.851	2351	2357	2362	rBV9	10128	21710	0.32%	0.034%
47	17.181	2406	2413	2423	rBV	2154334	3237602	47.07%	4.999%
48	17.281	2423	2430	2453	rVB	3744706	5790014	84.18%	8.940%
49	18.081	2561	2566	2573	rBV9	19665	47475	0.69%	0.073%
50	18.145	2573	2577	2581	rVB	18357	26149	0.38%	0.040%
51	19.098	2735	2739	2744	rBV2	50643	66089	0.96%	0.102%
52	19.169	2747	2751	2754	rBV	50174	72671	1.06%	0.112%
53	19.310	2773	2775	2781	rBV7	15370	28735	0.42%	0.044%
54	19.522	2805	2811	2823	rBV	4836225	6803971	98.92%	10.506%
55	19.751	2847	2850	2856	rBV	50820	67086	0.98%	0.104%
56	21.275	3105	3109	3121	rBV	2608776	3713489	53.99%	5.734%
57	23.498	3481	3487	3503	rVB2	3361562	6878385	100.00%	10.621%
58	23.651	3507	3513	3526	rVB2	1705323	3438202	49.99%	5.309%




Sum of corrected areas: 64762214

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012596.D
Acq On : 10 Nov 2022 13:14
Operator : CG/JU
Sample : PB148942BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK942

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

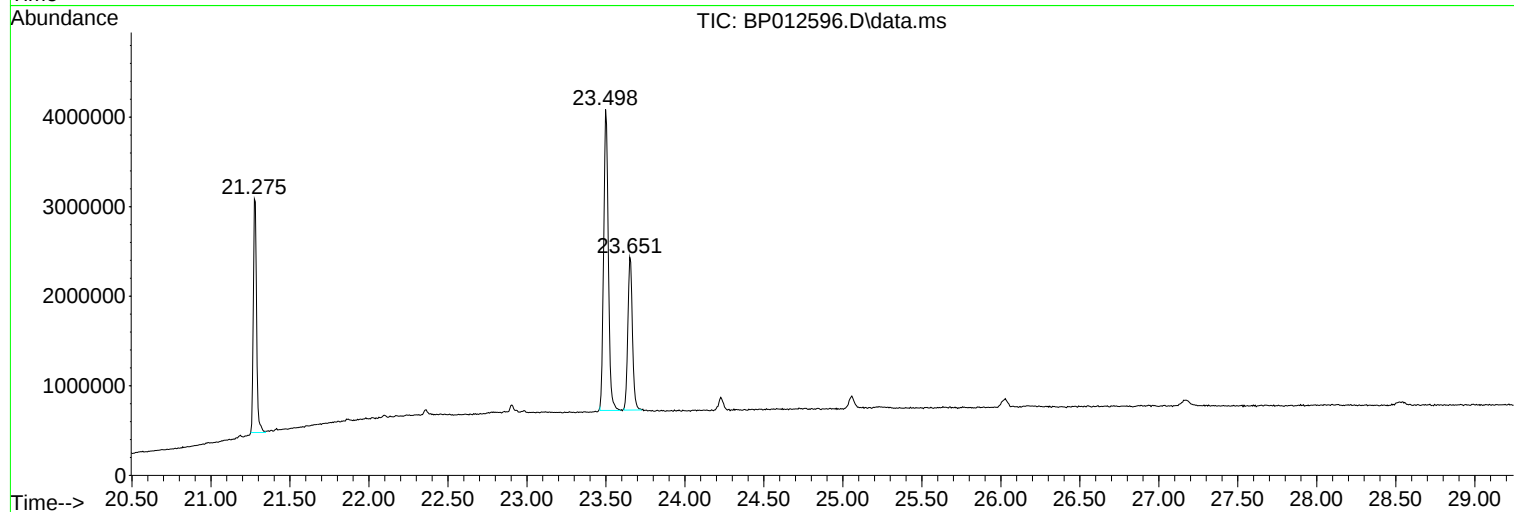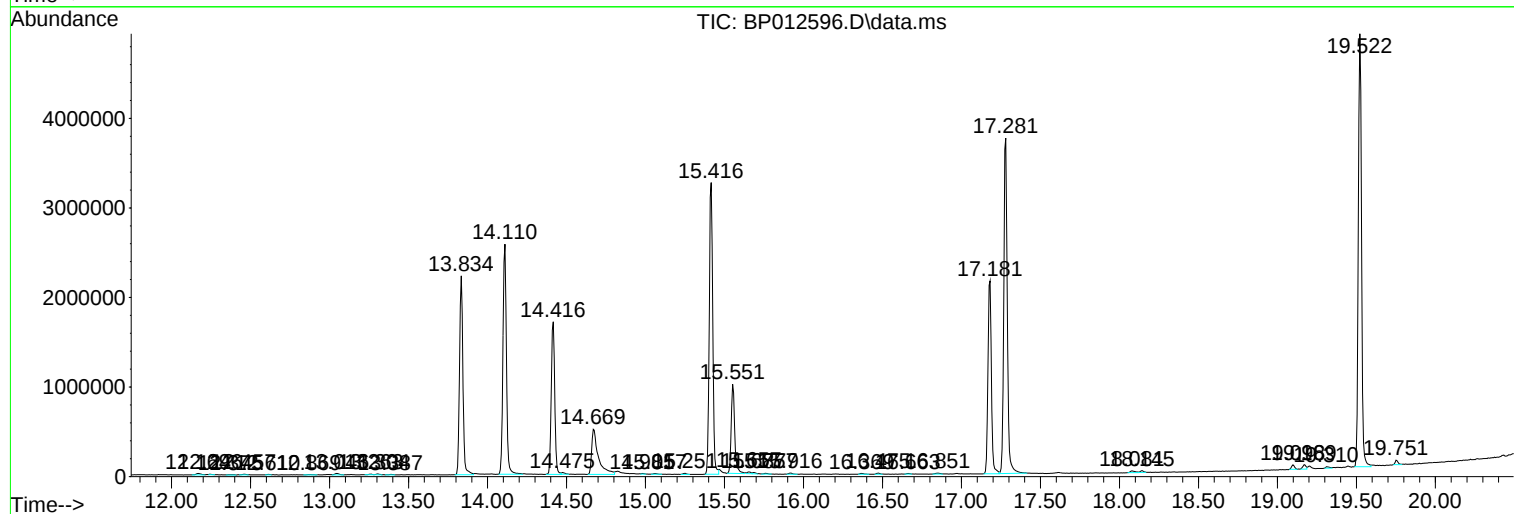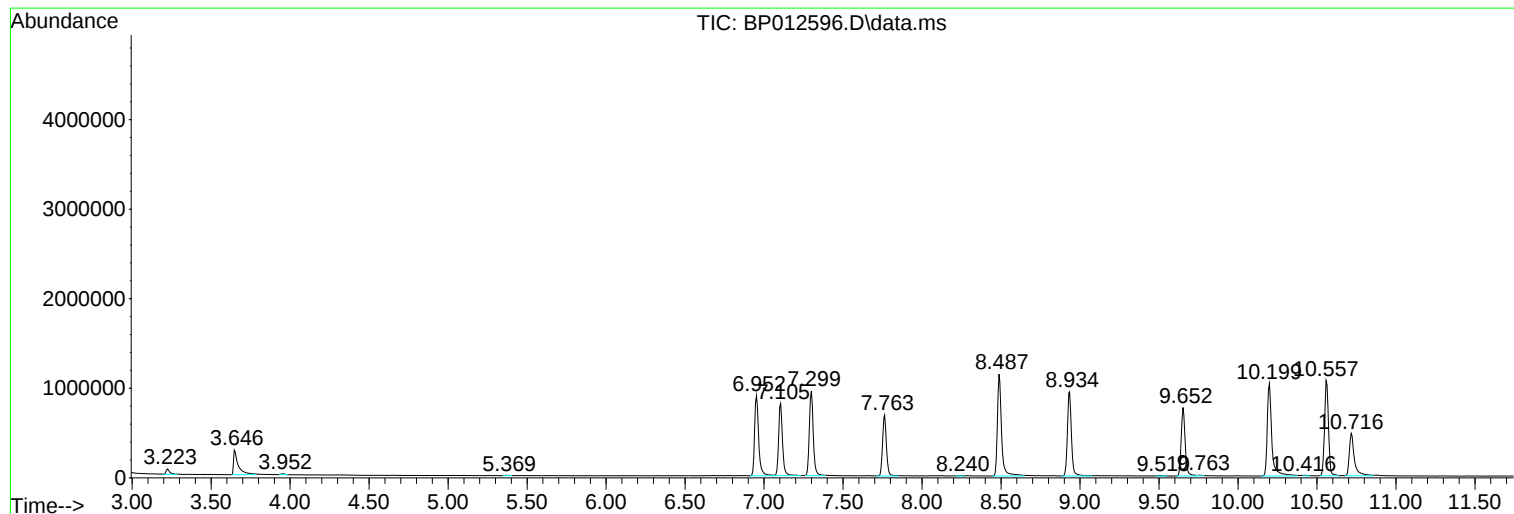

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012596.D
Acq On : 10 Nov 2022 13:14
Operator : CG/JU
Sample : PB148942BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK942

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012596.D
Acq On : 10 Nov 2022 13:14
Operator : CG/JU
Sample : PB148942BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK942

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc