

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
 Data File : BP012597.D
 Acq On : 10 Nov 2022 13:48
 Operator : CG/JU
 Sample : N5493-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012597.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	37	40	45	rBV	36378	51926	0.64%	0.073%
2	3.652	111	113	135	rBV	190434	409224	5.04%	0.578%
3	3.858	144	148	153	rVB2	17893	27053	0.33%	0.038%
4	3.952	159	164	171	rVB2	16564	28816	0.35%	0.041%
5	4.181	199	203	209	rBV3	14530	21745	0.27%	0.031%
6	4.475	248	253	259	rBV2	38115	60871	0.75%	0.086%
7	4.905	320	326	331	rBV5	9521	18246	0.22%	0.026%
8	6.957	669	675	687	rBV	165229	332027	4.09%	0.469%
9	7.105	693	700	712	rBV	785993	1331571	16.39%	1.881%
10	7.299	726	733	751	rBV	693402	1179242	14.52%	1.666%
11	7.763	804	812	823	rBV	894434	1519133	18.70%	2.146%
12	8.493	929	936	959	rBV	521083	987215	12.15%	1.395%
13	8.934	1002	1011	1030	rBV	948823	1659443	20.43%	2.345%
14	9.310	1069	1075	1079	rVB2	10526	17526	0.22%	0.025%
15	9.651	1122	1133	1149	rBV	713078	1266616	15.59%	1.790%
16	10.198	1218	1226	1248	rBV	949010	1857947	22.87%	2.625%
17	10.369	1248	1255	1275	rVB4	35336	160296	1.97%	0.226%
18	10.557	1280	1287	1300	rVB	1398391	2453820	30.21%	3.467%
19	10.716	1306	1314	1336	rBV	861174	1742555	21.45%	2.462%
20	11.992	1526	1531	1538	rBV5	8901	18050	0.22%	0.026%
21	12.163	1554	1560	1567	rBV4	17959	34225	0.42%	0.048%
22	12.769	1657	1663	1667	rBV8	5180	9766	0.12%	0.014%
23	13.016	1700	1705	1717	rVB5	10898	25902	0.32%	0.037%
24	13.310	1749	1755	1760	rVB4	10685	20222	0.25%	0.029%
25	13.387	1763	1768	1772	rBV6	6637	12112	0.15%	0.017%
26	13.834	1834	1844	1867	rBV	2286255	3383747	41.66%	4.781%
27	14.110	1880	1891	1916	rBV	2622673	4085109	50.29%	5.772%
28	14.416	1936	1943	1955	rBV	2371556	3506831	43.17%	4.955%
29	14.698	1985	1991	2007	rBV2	50813	194140	2.39%	0.274%
30	15.051	2044	2051	2055	rBV2	10473	16523	0.20%	0.023%
31	15.210	2073	2078	2082	rBV	24439	35158	0.43%	0.050%
32	15.257	2082	2086	2092	rVB2	21430	35259	0.43%	0.050%
33	15.416	2106	2113	2131	rBV	3454823	5272250	64.91%	7.449%
34	15.551	2131	2136	2149	rVV	968125	1475738	18.17%	2.085%
35	15.657	2151	2154	2160	rVB3	21154	36370	0.45%	0.051%
36	15.822	2179	2182	2186	rVB5	9748	14304	0.18%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
 Data File : BP012597.D
 Acq On : 10 Nov 2022 13:48
 Operator : CG/JU
 Sample : N5493-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Title : SVOA CALIBRATION

37	15.881	2188	2192	2197	rVB8	5555	9160	0.11%	0.013%
38	15.986	2207	2210	2215	rBV7	5287	9734	0.12%	0.014%
39	16.045	2217	2220	2223	rVV4	8916	11000	0.14%	0.016%
40	16.086	2224	2227	2231	rVV4	13112	19757	0.24%	0.028%
41	16.128	2231	2234	2243	rVV5	18631	41603	0.51%	0.059%
42	16.198	2243	2246	2249	rVB5	6397	9923	0.12%	0.014%
43	16.316	2257	2266	2272	rBV3	16170	38962	0.48%	0.055%
44	16.586	2308	2312	2319	rBV7	14647	27690	0.34%	0.039%
45	16.928	2366	2370	2373	rBV	17794	19929	0.25%	0.028%
46	16.975	2373	2378	2384	rVB3	14188	27769	0.34%	0.039%
47	17.092	2394	2398	2402	rVB2	35017	45839	0.56%	0.065%
48	17.180	2406	2413	2423	rBV	2960150	4349810	53.55%	6.146%
49	17.280	2423	2430	2442	rVV	4070601	5952169	73.28%	8.410%
50	17.469	2459	2462	2469	rVB5	14610	23890	0.29%	0.034%
51	17.675	2493	2497	2502	rBV5	12777	23203	0.29%	0.033%
52	17.851	2522	2527	2531	rBV	58268	71129	0.88%	0.100%
53	17.945	2541	2543	2548	rBV6	10970	17355	0.21%	0.025%
54	18.069	2559	2564	2574	rBV	205447	354814	4.37%	0.501%
55	19.098	2735	2739	2743	rBV3	61483	98684	1.21%	0.139%
56	19.169	2748	2751	2762	rVB2	59841	135700	1.67%	0.192%
57	19.304	2771	2774	2783	rBV3	109415	178919	2.20%	0.253%
58	19.522	2805	2811	2827	rBV	5420111	7437990	91.57%	10.509%
59	19.751	2847	2850	2855	rBV	47505	57101	0.70%	0.081%
60	21.280	3105	3110	3120	rBV	3984224	5197799	63.99%	7.344%
61	23.504	3480	3488	3503	rVB2	3904415	8122386	100.00%	11.476%
62	23.657	3507	3514	3525	rVB2	2506128	5192383	63.93%	7.336%




Sum of corrected areas: 70775676

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012597.D
Acq On : 10 Nov 2022 13:48
Operator : CG/JU
Sample : N5493-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

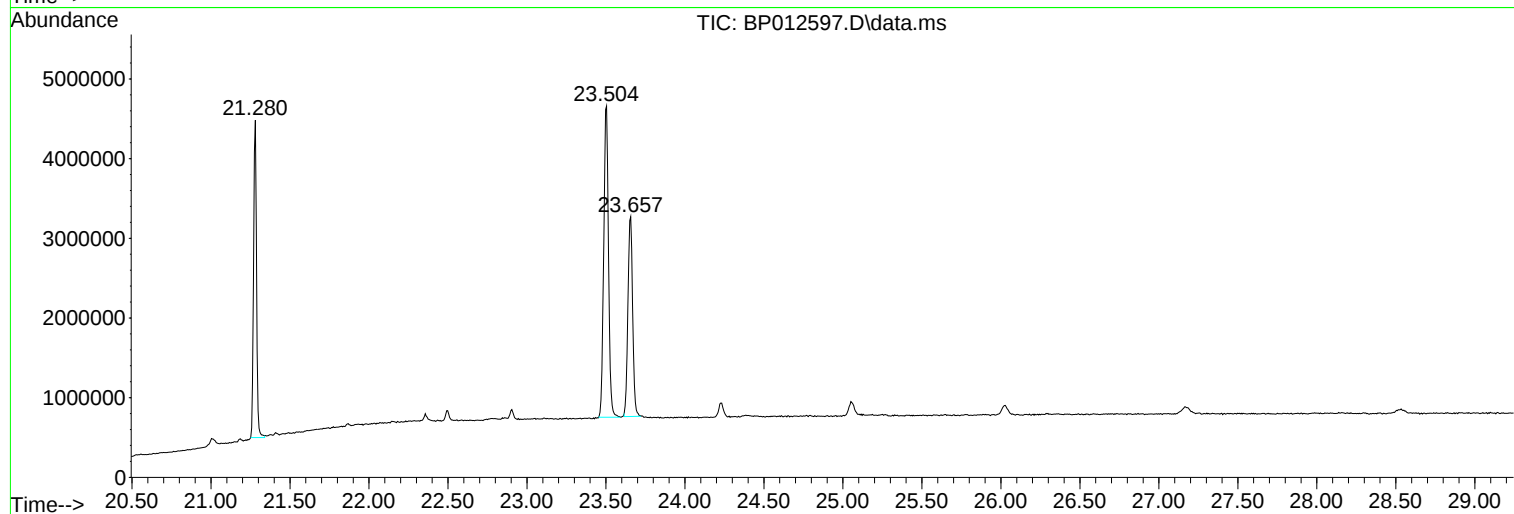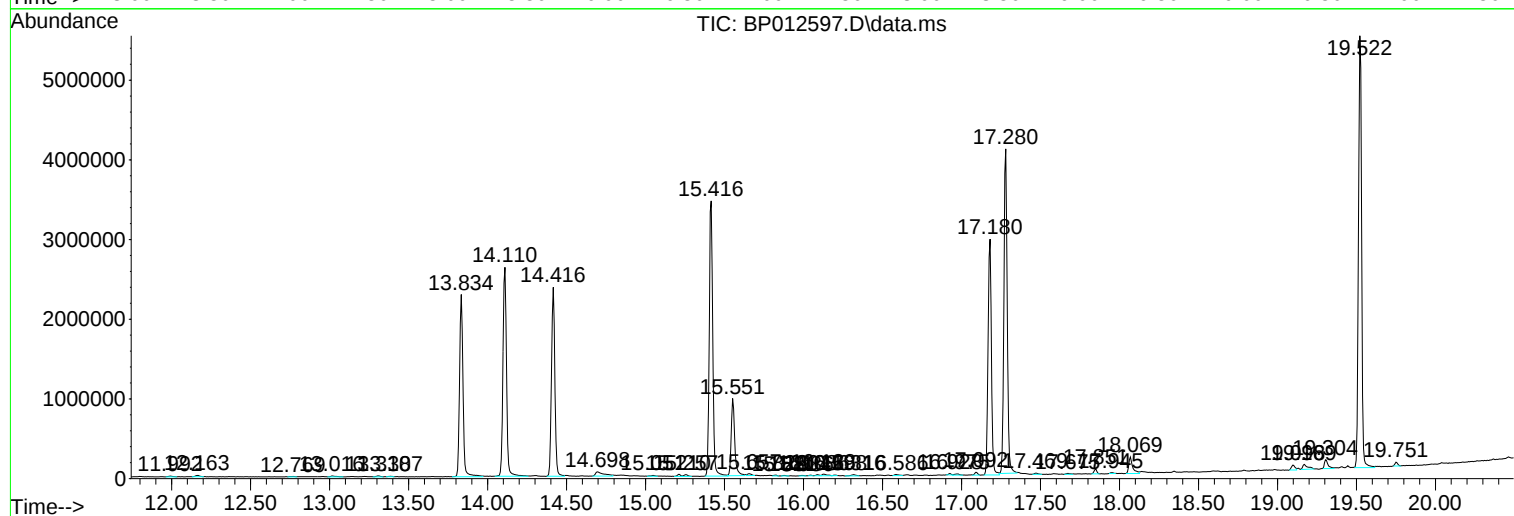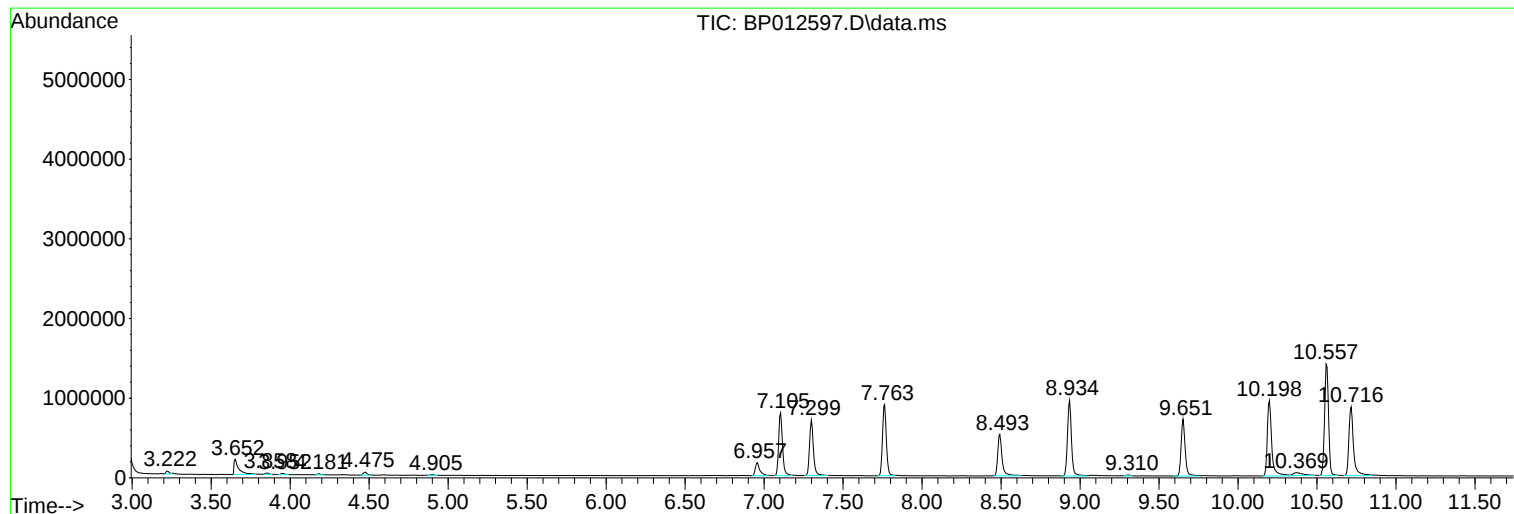

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012597.D
Acq On : 10 Nov 2022 13:48
Operator : CG/JU
Sample : N5493-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012597.D
Acq On : 10 Nov 2022 13:48
Operator : CG/JU
Sample : N5493-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc