

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
 Data File : BP012598.D
 Acq On : 10 Nov 2022 14:23
 Operator : CG/JU
 Sample : N5541-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012598.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	36	40	52	rVB	42628	71034	0.98%	0.109%
2	3.652	110	113	129	rBV	161067	349065	4.80%	0.535%
3	3.852	143	147	154	rVB	21856	38610	0.53%	0.059%
4	3.952	159	164	177	rVB	43904	79886	1.10%	0.122%
5	4.893	320	324	333	rVB3	11764	21454	0.30%	0.033%
6	6.958	668	675	692	rBV	165930	334097	4.60%	0.512%
7	7.105	693	700	713	rBV	743879	1275236	17.55%	1.955%
8	7.299	726	733	752	rBV	688443	1200382	16.52%	1.840%
9	7.763	803	812	823	rBV	869239	1469597	20.23%	2.253%
10	8.493	929	936	952	rBV	516370	979537	13.48%	1.502%
11	8.934	1004	1011	1028	rBV	884578	1554768	21.40%	2.384%
12	9.299	1069	1073	1085	rVB9	3907	7939	0.11%	0.012%
13	9.652	1125	1133	1145	rBV	689341	1204808	16.58%	1.847%
14	10.199	1218	1226	1254	rBV	864633	1750003	24.09%	2.683%
15	10.563	1280	1288	1300	rBV	1330764	2341254	32.23%	3.590%
16	10.716	1307	1314	1347	rBV	839080	1764800	24.29%	2.706%
17	12.175	1554	1562	1569	rBV4	14332	36435	0.50%	0.056%
18	13.310	1749	1755	1760	rBV5	12281	18503	0.25%	0.028%
19	13.387	1763	1768	1773	rBV8	4239	7539	0.10%	0.012%
20	13.746	1824	1829	1835	rBV10	3779	9106	0.13%	0.014%
21	13.834	1835	1844	1859	rBV	2065850	3030404	41.71%	4.646%
22	14.110	1882	1891	1908	rBV	2410811	3748142	51.59%	5.747%
23	14.416	1936	1943	1958	rBV	2233193	3367495	46.35%	5.163%
24	14.704	1985	1992	2012	rBV2	47675	208097	2.86%	0.319%
25	14.875	2018	2021	2027	rVB8	13370	20623	0.28%	0.032%
26	15.416	2106	2113	2130	rBV	3148046	4881960	67.20%	7.485%
27	15.551	2130	2136	2150	rVV	795991	1286187	17.70%	1.972%
28	15.657	2151	2154	2161	rVB3	20319	36631	0.50%	0.056%
29	16.628	2312	2319	2321	rBV7	3303	7785	0.11%	0.012%
30	17.181	2406	2413	2423	rBV	2854494	4177191	57.50%	6.404%
31	17.281	2423	2430	2446	rVV2	3428364	5535997	76.20%	8.488%
32	17.392	2446	2449	2456	rVB4	28278	49773	0.69%	0.076%
33	17.945	2540	2543	2546	rBV5	4338	7288	0.10%	0.011%
34	18.069	2560	2564	2575	rBV2	73431	145138	2.00%	0.223%
35	19.098	2735	2739	2744	rBV	51349	74486	1.03%	0.114%
36	19.169	2747	2751	2755	rBV	45150	69760	0.96%	0.107%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012598.D
Acq On : 10 Nov 2022 14:23
Operator : CG/JU
Sample : N5541-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Title : SVOA CALIBRATION

37	19.310	2771	2775	2781	rBV3	60384	101918	1.40%	0.156%
38	19.522	2805	2811	2826	rBV	4816386	6645887	91.48%	10.189%
39	21.280	3105	3110	3120	rBV	3768446	4982325	68.58%	7.639%
40	23.498	3480	3487	3499	rBV2	3364586	7264725	100.00%	11.138%
41	23.657	3507	3514	3527	rVB2	2414296	5068559	69.77%	7.771%




Sum of corrected areas: 65224424

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012598.D
Acq On : 10 Nov 2022 14:23
Operator : CG/JU
Sample : N5541-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

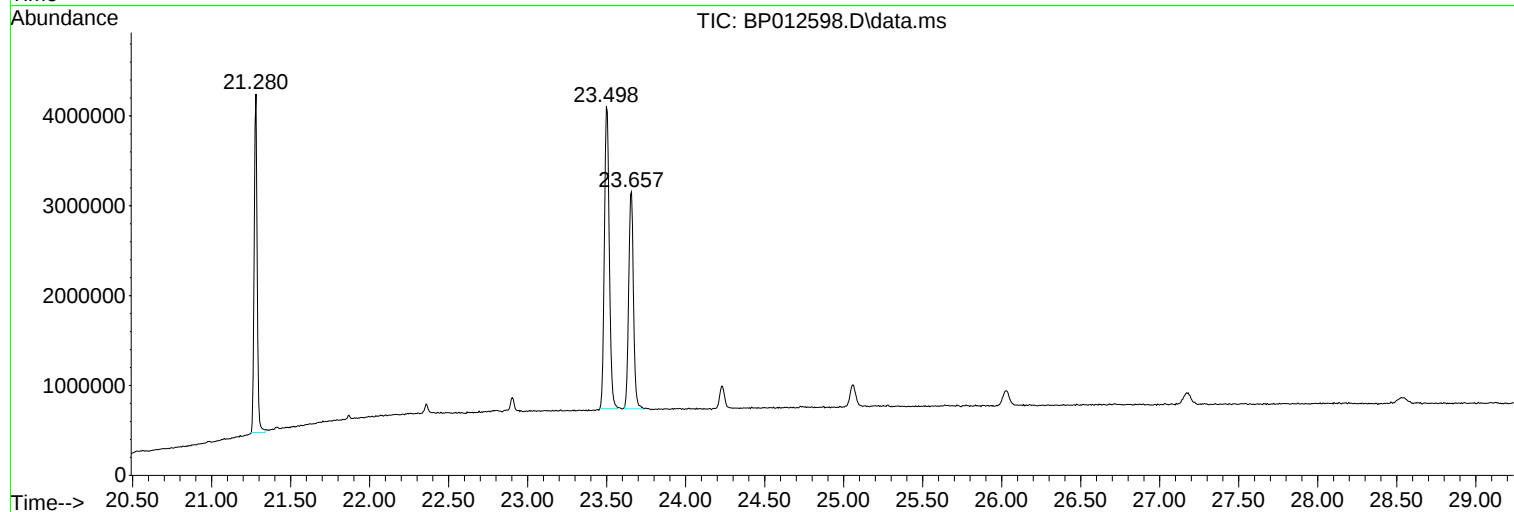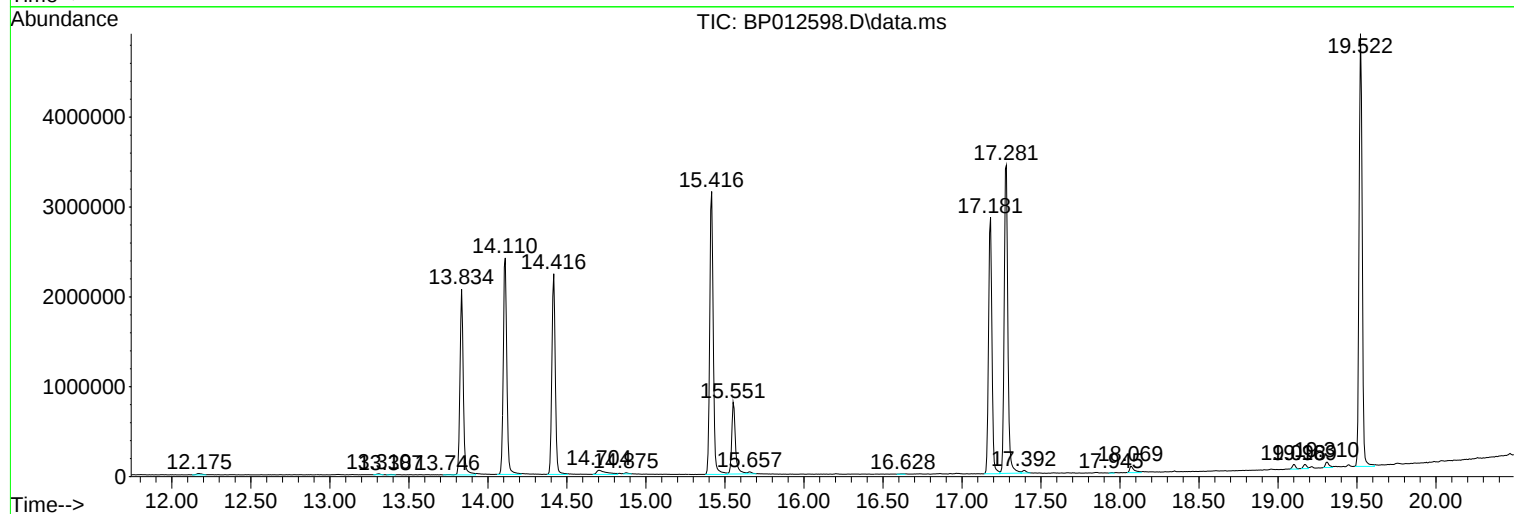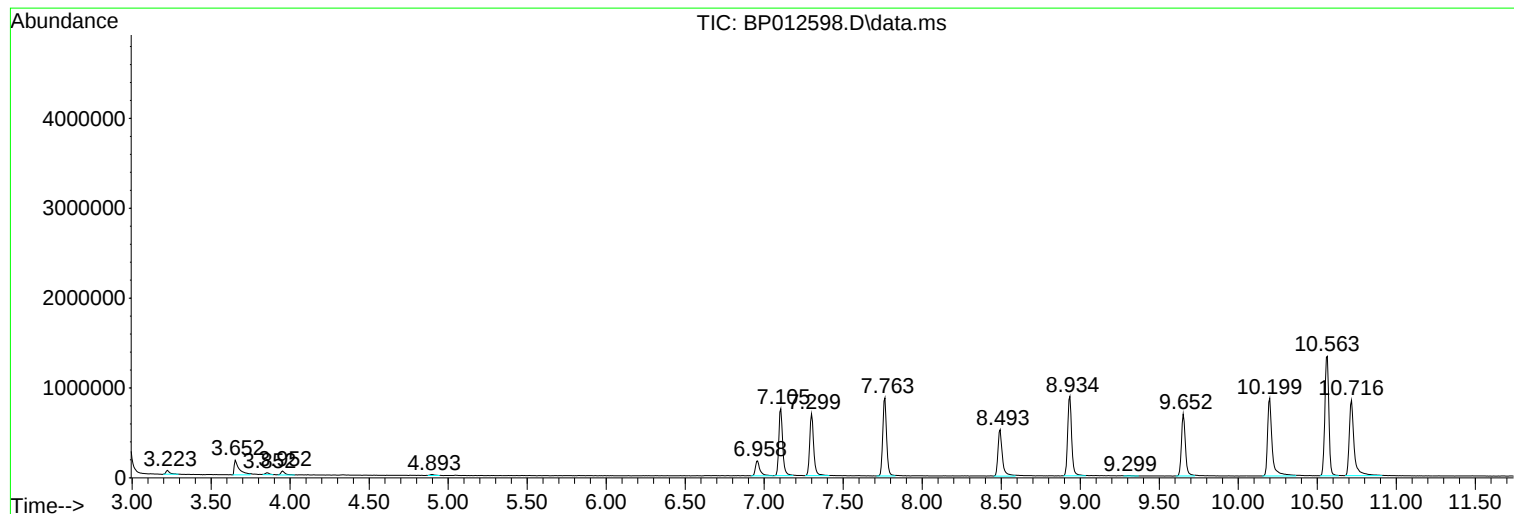

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012598.D
Acq On : 10 Nov 2022 14:23
Operator : CG/JU
Sample : N5541-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012598.D
Acq On : 10 Nov 2022 14:23
Operator : CG/JU
Sample : N5541-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
