

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
 Data File : BP012599.D
 Acq On : 10 Nov 2022 14:57
 Operator : CG/JU
 Sample : N5493-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	55	rVB2	39431	80040	1.02%	0.121%
2	3.652	110	113	130	rBV	137366	291267	3.70%	0.441%
3	3.852	143	147	153	rVB2	18804	29541	0.38%	0.045%
4	3.952	160	164	171	rVB3	14309	22581	0.29%	0.034%
5	4.475	248	253	259	rBV	20257	36747	0.47%	0.056%
6	4.893	317	324	331	rBV6	9335	19608	0.25%	0.030%
7	6.958	667	675	692	rBV	134685	278010	3.53%	0.421%
8	7.105	693	700	718	rVB	696327	1204661	15.30%	1.825%
9	7.299	727	733	749	rBV	604702	1038767	13.20%	1.574%
10	7.763	804	812	823	rBV	822183	1394997	17.72%	2.113%
11	8.493	928	936	954	rBV	447694	850105	10.80%	1.288%
12	8.934	1004	1011	1030	rBV	852434	1495171	19.00%	2.265%
13	9.304	1068	1074	1081	rVB2	12212	24221	0.31%	0.037%
14	9.652	1126	1133	1150	rBV	645656	1126370	14.31%	1.706%
15	10.199	1219	1226	1243	rBV	800684	1602300	20.36%	2.427%
16	10.557	1280	1287	1303	rVB	1289321	2240340	28.46%	3.394%
17	10.716	1307	1314	1339	rBV	778035	1598790	20.31%	2.422%
18	11.998	1523	1532	1540	rBV	4244	11501	0.15%	0.017%
19	12.163	1554	1560	1566	rBV2	15107	27312	0.35%	0.041%
20	13.016	1700	1705	1709	rBV7	5996	11932	0.15%	0.018%
21	13.228	1734	1741	1744	rBV9	4012	7979	0.10%	0.012%
22	13.310	1750	1755	1760	rVB3	10353	15845	0.20%	0.024%
23	13.834	1836	1844	1868	rBV	2176417	3228279	41.01%	4.891%
24	14.110	1882	1891	1918	rBV	2376273	3753553	47.69%	5.686%
25	14.304	1920	1924	1928	rVB7	6302	10520	0.13%	0.016%
26	14.416	1936	1943	1966	rBV	2199129	3222688	40.94%	4.882%
27	14.704	1985	1992	2003	rBV4	49218	170517	2.17%	0.258%
28	15.051	2047	2051	2055	rVB2	7964	10813	0.14%	0.016%
29	15.210	2074	2078	2082	rBV	11981	16286	0.21%	0.025%
30	15.257	2082	2086	2090	rVB3	15605	23355	0.30%	0.035%
31	15.416	2106	2113	2129	rBV	3302529	5017748	63.75%	7.602%
32	15.551	2130	2136	2150	rVV	1010787	1524267	19.36%	2.309%
33	15.657	2150	2154	2160	rVB4	22016	41106	0.52%	0.062%
34	15.822	2179	2182	2187	rVB6	7814	11353	0.14%	0.017%
35	16.092	2224	2228	2230	rBV4	8249	10803	0.14%	0.016%
36	16.145	2231	2237	2244	rVV6	18960	49870	0.63%	0.076%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
 Data File : BP012599.D
 Acq On : 10 Nov 2022 14:57
 Operator : CG/JU
 Sample : N5493-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Title : SVOA CALIBRATION

37	16.322	2259	2267	2271	rBV5	11688	26327	0.33%	0.040%
38	16.475	2286	2293	2296	rBV9	7615	18193	0.23%	0.028%
39	16.586	2308	2312	2318	rBV8	12014	20332	0.26%	0.031%
40	16.928	2367	2370	2373	rBV2	14796	16247	0.21%	0.025%
41	17.092	2394	2398	2404	rVB5	15375	20653	0.26%	0.031%
42	17.181	2406	2413	2423	rBV	2690510	3979710	50.56%	6.029%
43	17.281	2423	2430	2449	rVB	3935758	6112970	77.66%	9.261%
44	17.469	2460	2462	2468	rVB6	9822	13503	0.17%	0.020%
45	17.669	2493	2496	2500	rBV6	7902	13289	0.17%	0.020%
46	17.845	2523	2526	2532	rVB	28808	36809	0.47%	0.056%
47	18.069	2559	2564	2573	rBV	181340	299070	3.80%	0.453%
48	19.098	2735	2739	2747	rBV2	59320	101486	1.29%	0.154%
49	19.169	2747	2751	2763	rVV2	62785	156111	1.98%	0.237%
50	19.304	2770	2774	2781	rBV2	103799	177014	2.25%	0.268%
51	19.522	2805	2811	2824	rBV	5519258	7321277	93.01%	11.091%
52	21.280	3105	3110	3120	rBV	3607781	4702443	59.74%	7.124%
53	23.498	3480	3487	3502	rVB2	3791214	7871336	100.00%	11.925%
54	23.651	3507	3513	3523	rVB2	2251985	4622679	58.73%	7.003%




Sum of corrected areas: 66008692

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012599.D
Acq On : 10 Nov 2022 14:57
Operator : CG/JU
Sample : N5493-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

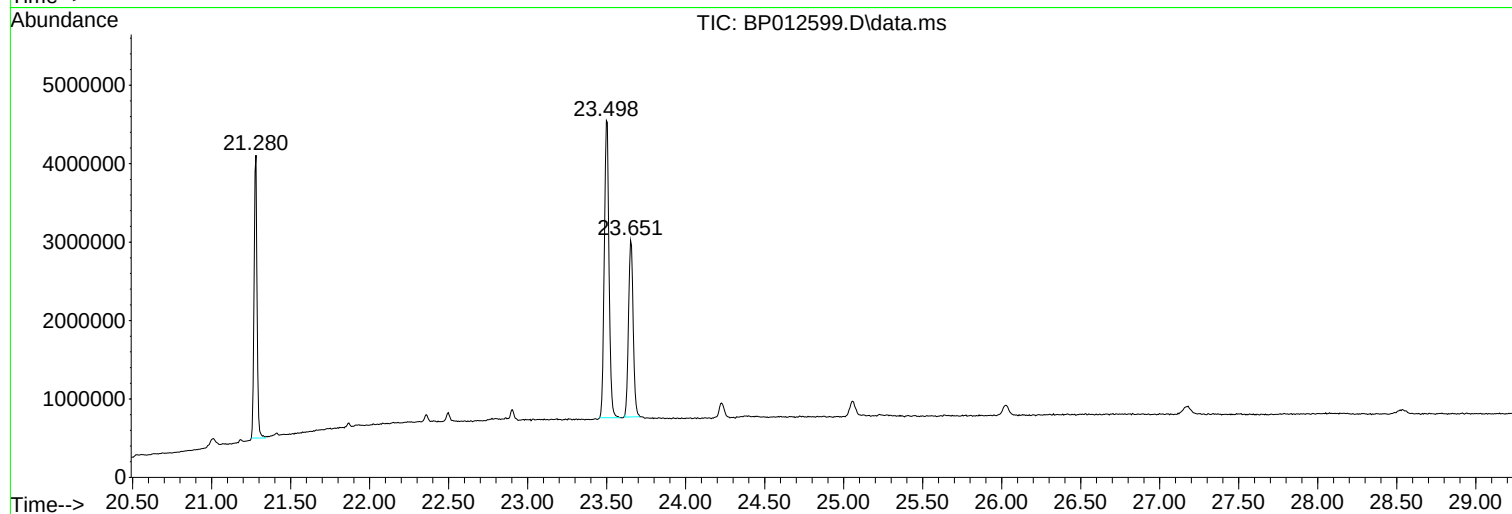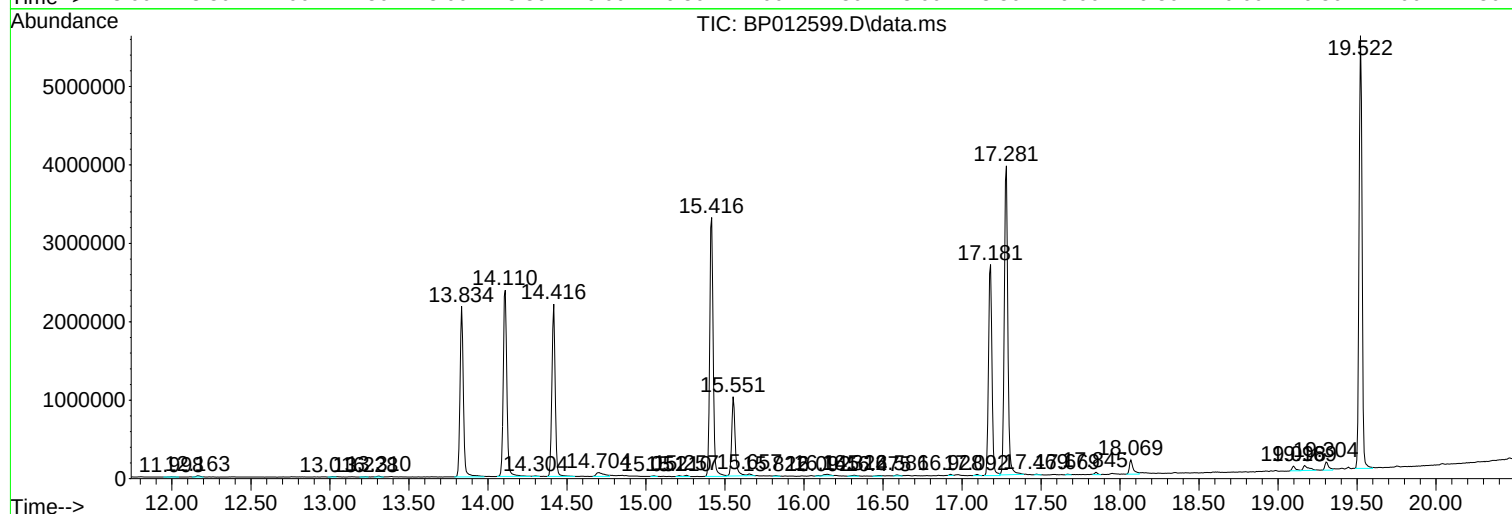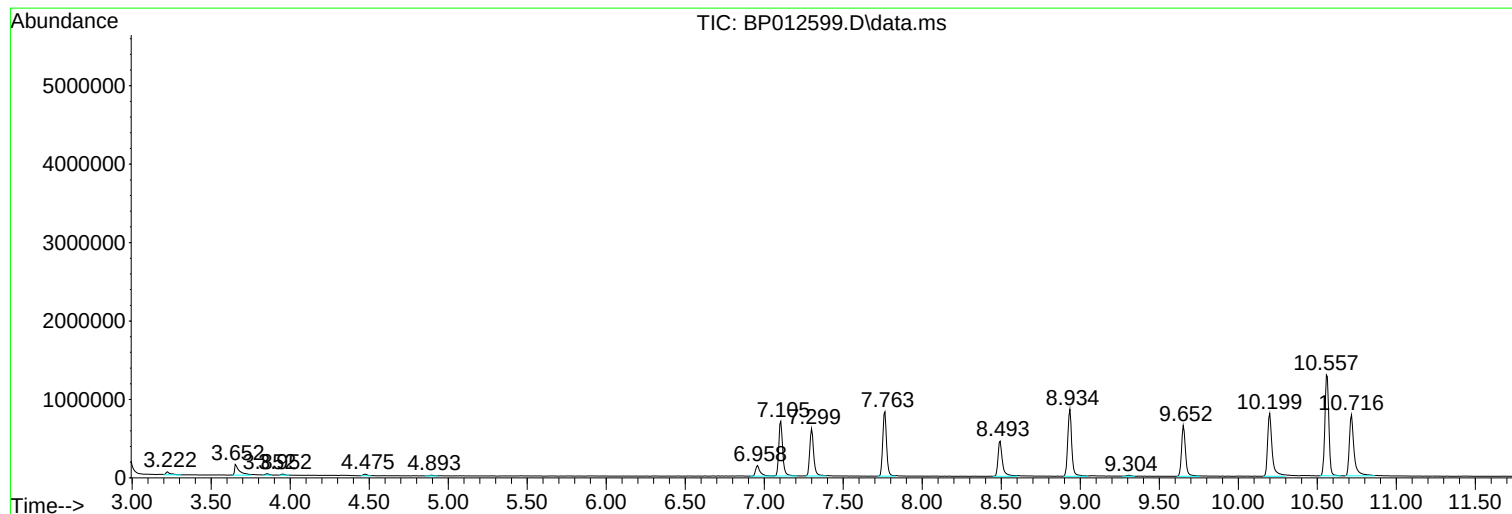

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012599.D
Acq On : 10 Nov 2022 14:57
Operator : CG/JU
Sample : N5493-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012599.D
Acq On : 10 Nov 2022 14:57
Operator : CG/JU
Sample : N5493-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc