

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
 Data File : BP012603.D
 Acq On : 10 Nov 2022 17:15
 Operator : CG/JU
 Sample : N5541-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012603.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	36	40	49	rVB	41973	67110	0.93%	0.106%
2	3.652	111	113	130	rBV	161528	347371	4.81%	0.549%
3	3.852	143	147	152	rVB	17751	27760	0.38%	0.044%
4	3.952	160	164	171	rVB	32090	48663	0.67%	0.077%
5	4.893	321	324	332	rVB	11923	22571	0.31%	0.036%
6	5.046	347	350	356	rVB3	6754	10361	0.14%	0.016%
7	6.952	668	674	693	rBV	161461	328986	4.55%	0.520%
8	7.105	693	700	717	rBV	769995	1342482	18.58%	2.121%
9	7.299	726	733	750	rBV	709326	1208749	16.73%	1.909%
10	7.763	803	812	822	rBV	695330	1181186	16.35%	1.866%
11	8.487	928	935	953	rBV	507031	979315	13.55%	1.547%
12	8.934	1003	1011	1026	rBV	927050	1631451	22.58%	2.577%
13	9.304	1070	1074	1078	rVB4	5905	9213	0.13%	0.015%
14	9.652	1124	1133	1160	rBV	705586	1285568	17.79%	2.031%
15	10.199	1216	1226	1245	rBV	888995	1786990	24.73%	2.823%
16	10.557	1279	1287	1299	rBV	1108777	1913363	26.48%	3.023%
17	10.716	1306	1314	1341	rBV	773995	1667912	23.09%	2.635%
18	12.169	1555	1561	1566	rBV2	15086	30111	0.42%	0.048%
19	13.051	1702	1711	1717	rVB2	4824	12834	0.18%	0.020%
20	13.228	1733	1741	1743	rBV8	4353	8527	0.12%	0.013%
21	13.263	1743	1747	1751	rVV5	5244	10794	0.15%	0.017%
22	13.304	1751	1754	1761	rVV9	6648	13755	0.19%	0.022%
23	13.387	1764	1768	1775	rVB8	5491	11079	0.15%	0.018%
24	13.745	1825	1829	1835	rBV9	4106	7756	0.11%	0.012%
25	13.834	1837	1844	1857	rBV	2255665	3281841	45.42%	5.184%
26	14.110	1883	1891	1908	rBV	2542054	4016407	55.59%	6.345%
27	14.416	1936	1943	1960	rBV	1869871	2791882	38.64%	4.410%
28	14.698	1985	1991	2003	rBV3	49182	166721	2.31%	0.263%
29	14.869	2016	2020	2033	rVB3	16154	39774	0.55%	0.063%
30	15.416	2106	2113	2122	rBV	3323301	5165841	71.50%	8.161%
31	15.551	2130	2136	2151	rBV	851507	1317870	18.24%	2.082%
32	15.657	2151	2154	2165	rVB3	23250	41238	0.57%	0.065%
33	16.592	2308	2313	2316	rBV7	7787	13917	0.19%	0.022%
34	16.969	2373	2377	2382	rVB5	6042	9929	0.14%	0.016%
35	17.181	2406	2413	2423	rBV	2352976	3478055	48.14%	5.494%
36	17.281	2423	2430	2445	rVV	3713774	5809319	80.41%	9.177%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
 Data File : BP012603.D
 Acq On : 10 Nov 2022 17:15
 Operator : CG/JU
 Sample : N5541-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KX8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Title : SVOA CALIBRATION

37	17.392	2446	2449	2458	rVB5	28609	53023	0.73%	0.084%
38	17.845	2522	2526	2531	rBV2	27561	38175	0.53%	0.060%
39	18.069	2559	2564	2575	rBV	151766	263933	3.65%	0.417%
40	18.980	2717	2719	2724	rVB6	27960	33280	0.46%	0.053%
41	19.098	2735	2739	2745	rBV2	55528	80169	1.11%	0.127%
42	19.169	2747	2751	2766	rVV3	60675	170510	2.36%	0.269%
43	19.304	2770	2774	2784	rBV	122609	219327	3.04%	0.346%
44	19.522	2805	2811	2827	rBV	5176185	6957408	96.30%	10.991%
45	21.280	3105	3110	3120	rBV	3179030	4190027	57.99%	6.619%
46	23.498	3480	3487	3501	rBV2	3506287	7224969	100.00%	11.413%
47	23.651	3507	3513	3524	rVB2	1912051	3985390	55.16%	6.296%




Sum of corrected areas: 63302912

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012603.D
Acq On : 10 Nov 2022 17:15
Operator : CG/JU
Sample : N5541-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

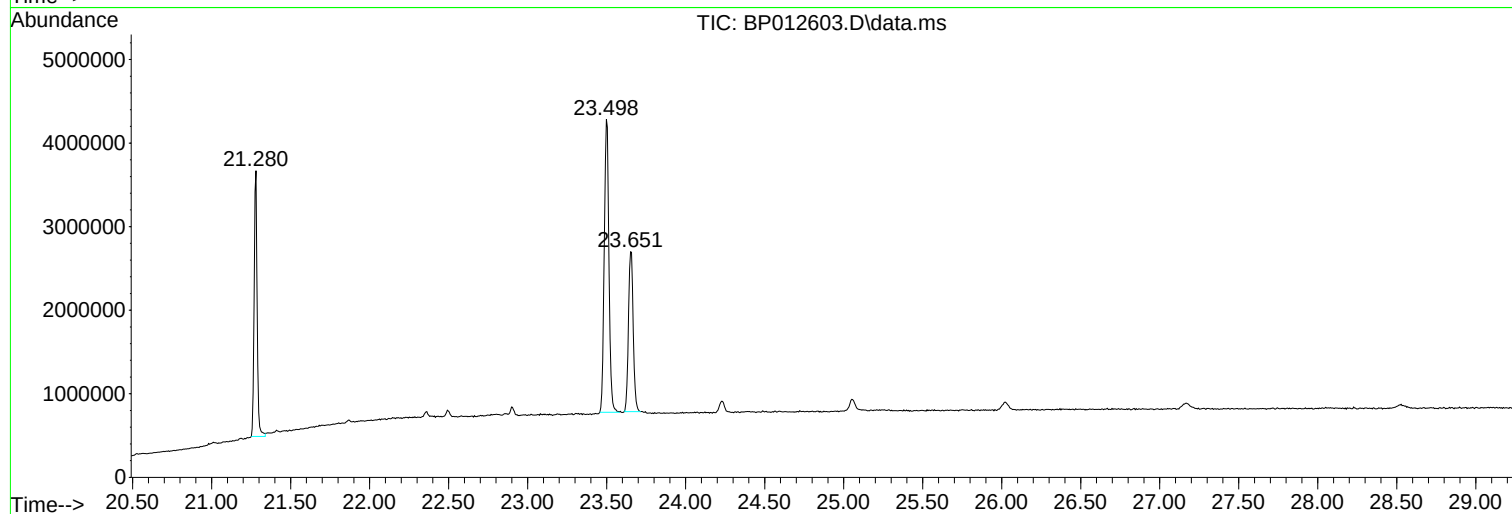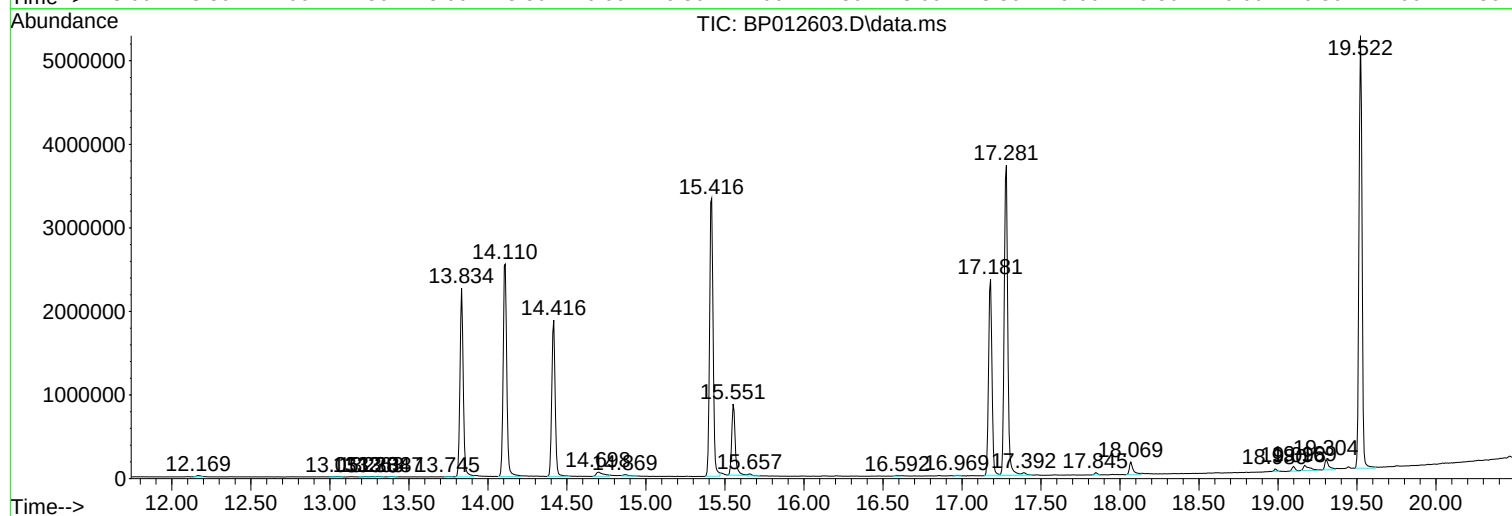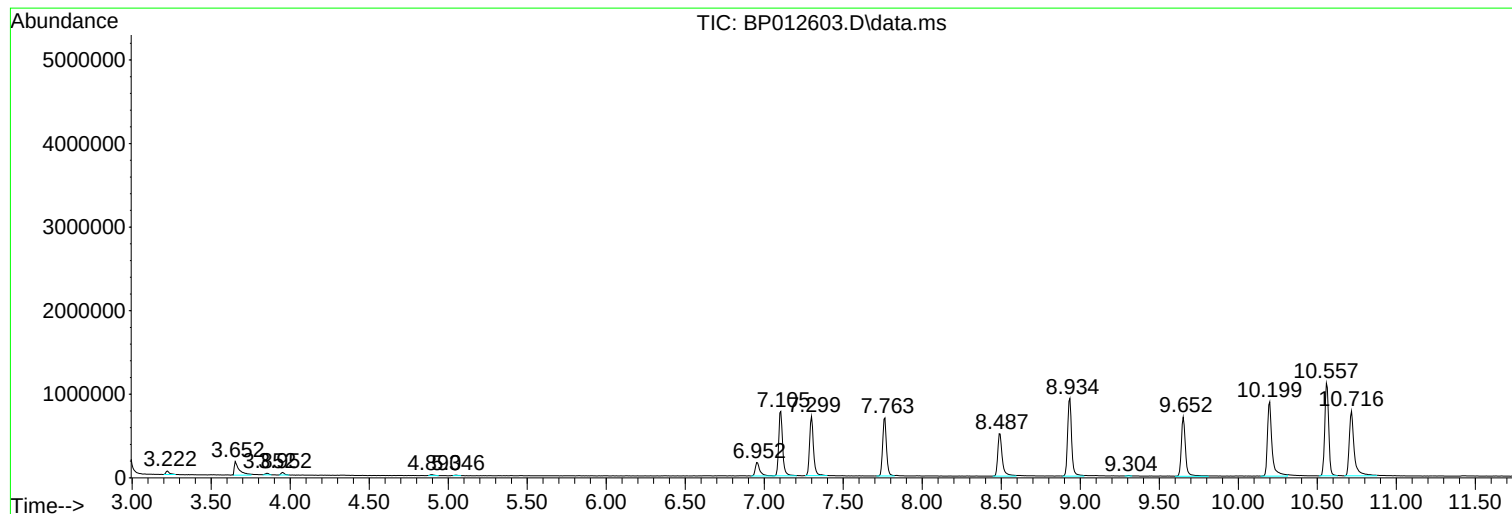

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012603.D
Acq On : 10 Nov 2022 17:15
Operator : CG/JU
Sample : N5541-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111022\
Data File : BP012603.D
Acq On : 10 Nov 2022 17:15
Operator : CG/JU
Sample : N5541-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc