
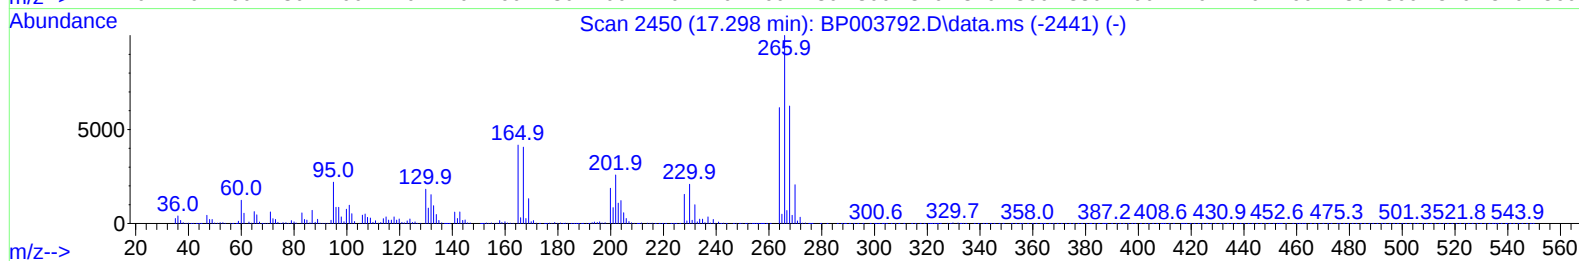
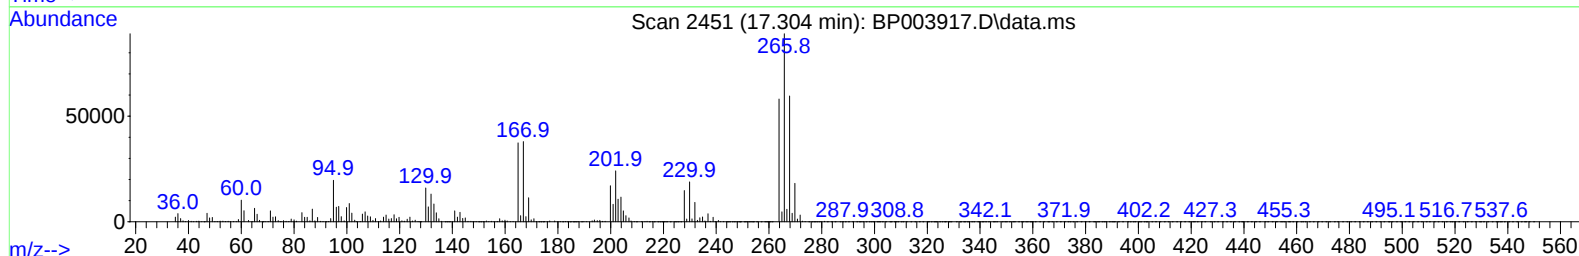


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111120\
Data File : BP003917.D
Acq On : 11 Nov 2020 12:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 05:11:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 13:41:24 2020
Response via : Initial Calibration

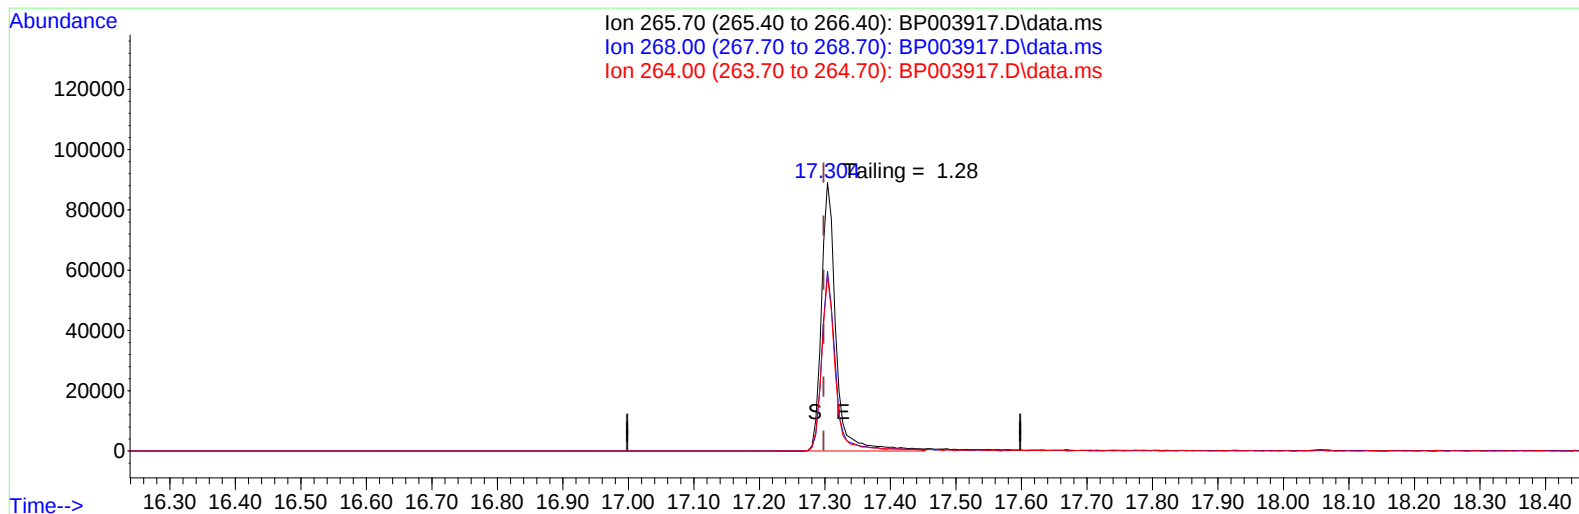

TIC: BP003917.D\data.ms

(70) Pentachlorophenol (C)




17.304min (+ 0.006) 37092.98 ng

response 137634

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	66.92
264.00	63.30	65.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111120\
Data File : BP003917.D
Acq On : 11 Nov 2020 12:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 05:11:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 13:41:24 2020
Response via : Initial Calibration

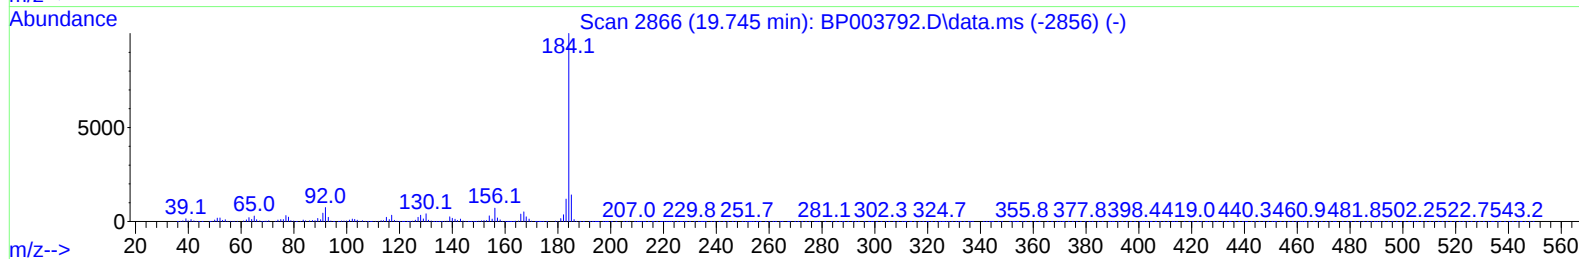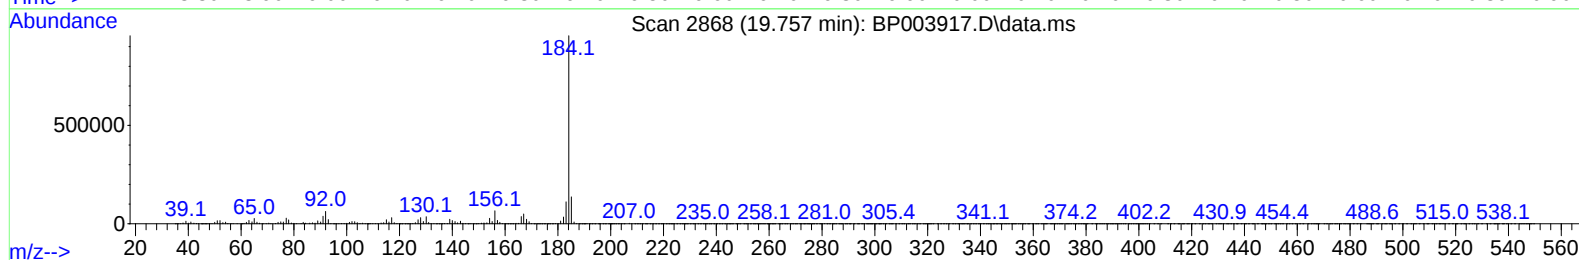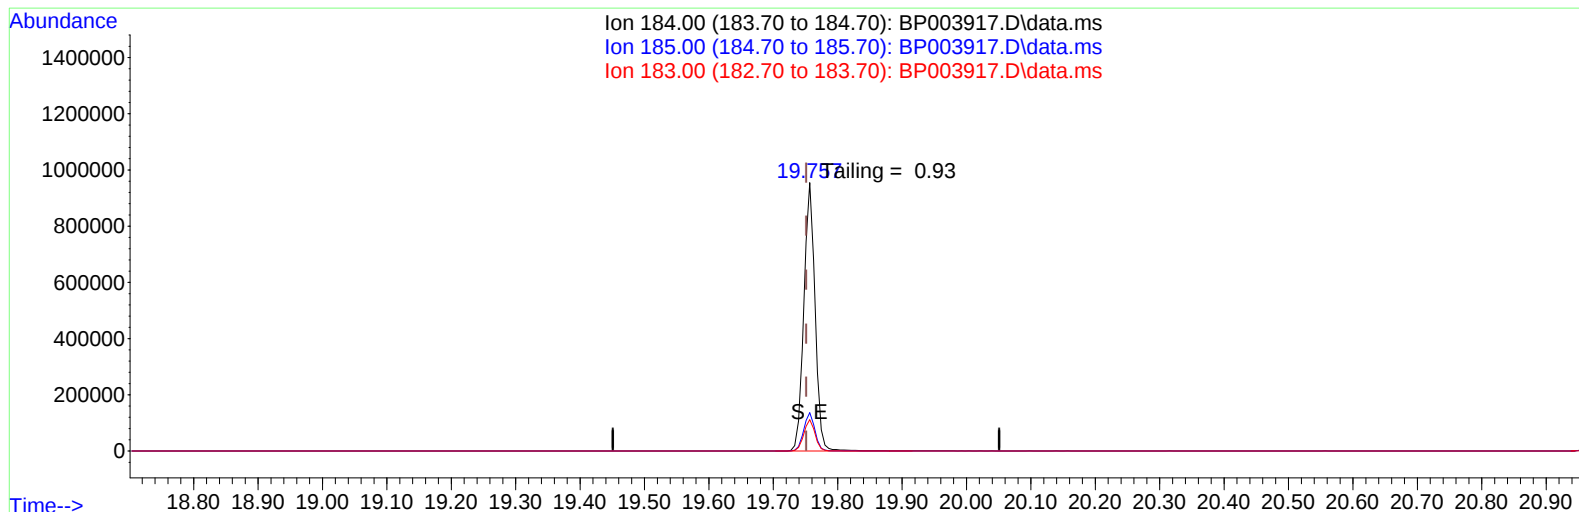

TIC: BP003917.D\data.ms

(77) Benzidine

19.757min (+ 0.006) 17088.24 ng

response 1164067

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.31
183.00	12.00	11.67
0.00	0.00	0.00