

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111120\
 Data File : BP003930.D
 Acq On : 11 Nov 2020 20:30
 Operator : CG/JU
 Sample : L4701-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TRANSFORMER-1-(1-4)

Manual Integrations
 APPROVED

mohammad
 11/12/2020 11:38:54 AM

Quant Time: Nov 12 00:25:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 13:41:24 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.281	152	152384	20.00	ng	0.00
21) Naphthalene-d8	11.110	136	562343	20.00	ng	# 0.00
39) Acenaphthene-d10	14.898	164	353602	20.00	ng	0.00
64) Phenanthrene-d10	17.634	188	755734	20.00	ng	# 0.00
76) Chrysene-d12	21.663	240	727483	20.00	ng	0.00
86) Perylene-d12	24.139	264	619132	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.805	112	789260	86.44	ng	0.00
7) Phenol-d6	7.446	99	1025708	78.26	ng	0.00
23) Nitrobenzene-d5	9.440	82	695033	60.53	ng	0.00
42) 2,4,6-Tribromophenol	16.381	330	366534	82.88	ng	0.00
45) 2-Fluorobiphenyl	13.522	172	1505689	59.53	ng	0.00
79) Terphenyl-d14	20.133	244	1878882	49.90	ng	0.00
Target Compounds						
32) Benzoic acid	10.387	122	28848m	12.88	ng	Qvalue
50) Dimethylphthalate	14.322	163	157289	5.69	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111120\
Data File : BP003930.D
Acq On : 11 Nov 2020 20:30
Operator : CG/JU
Sample : L4701-01
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
TRANSFORMER-1-(1-4)

Manual Integrations
APPROVED


mohammad
11/12/2020 11:38:54 AM

Quant Time: Nov 12 00:25:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 13:41:24 2020
Response via : Initial Calibration



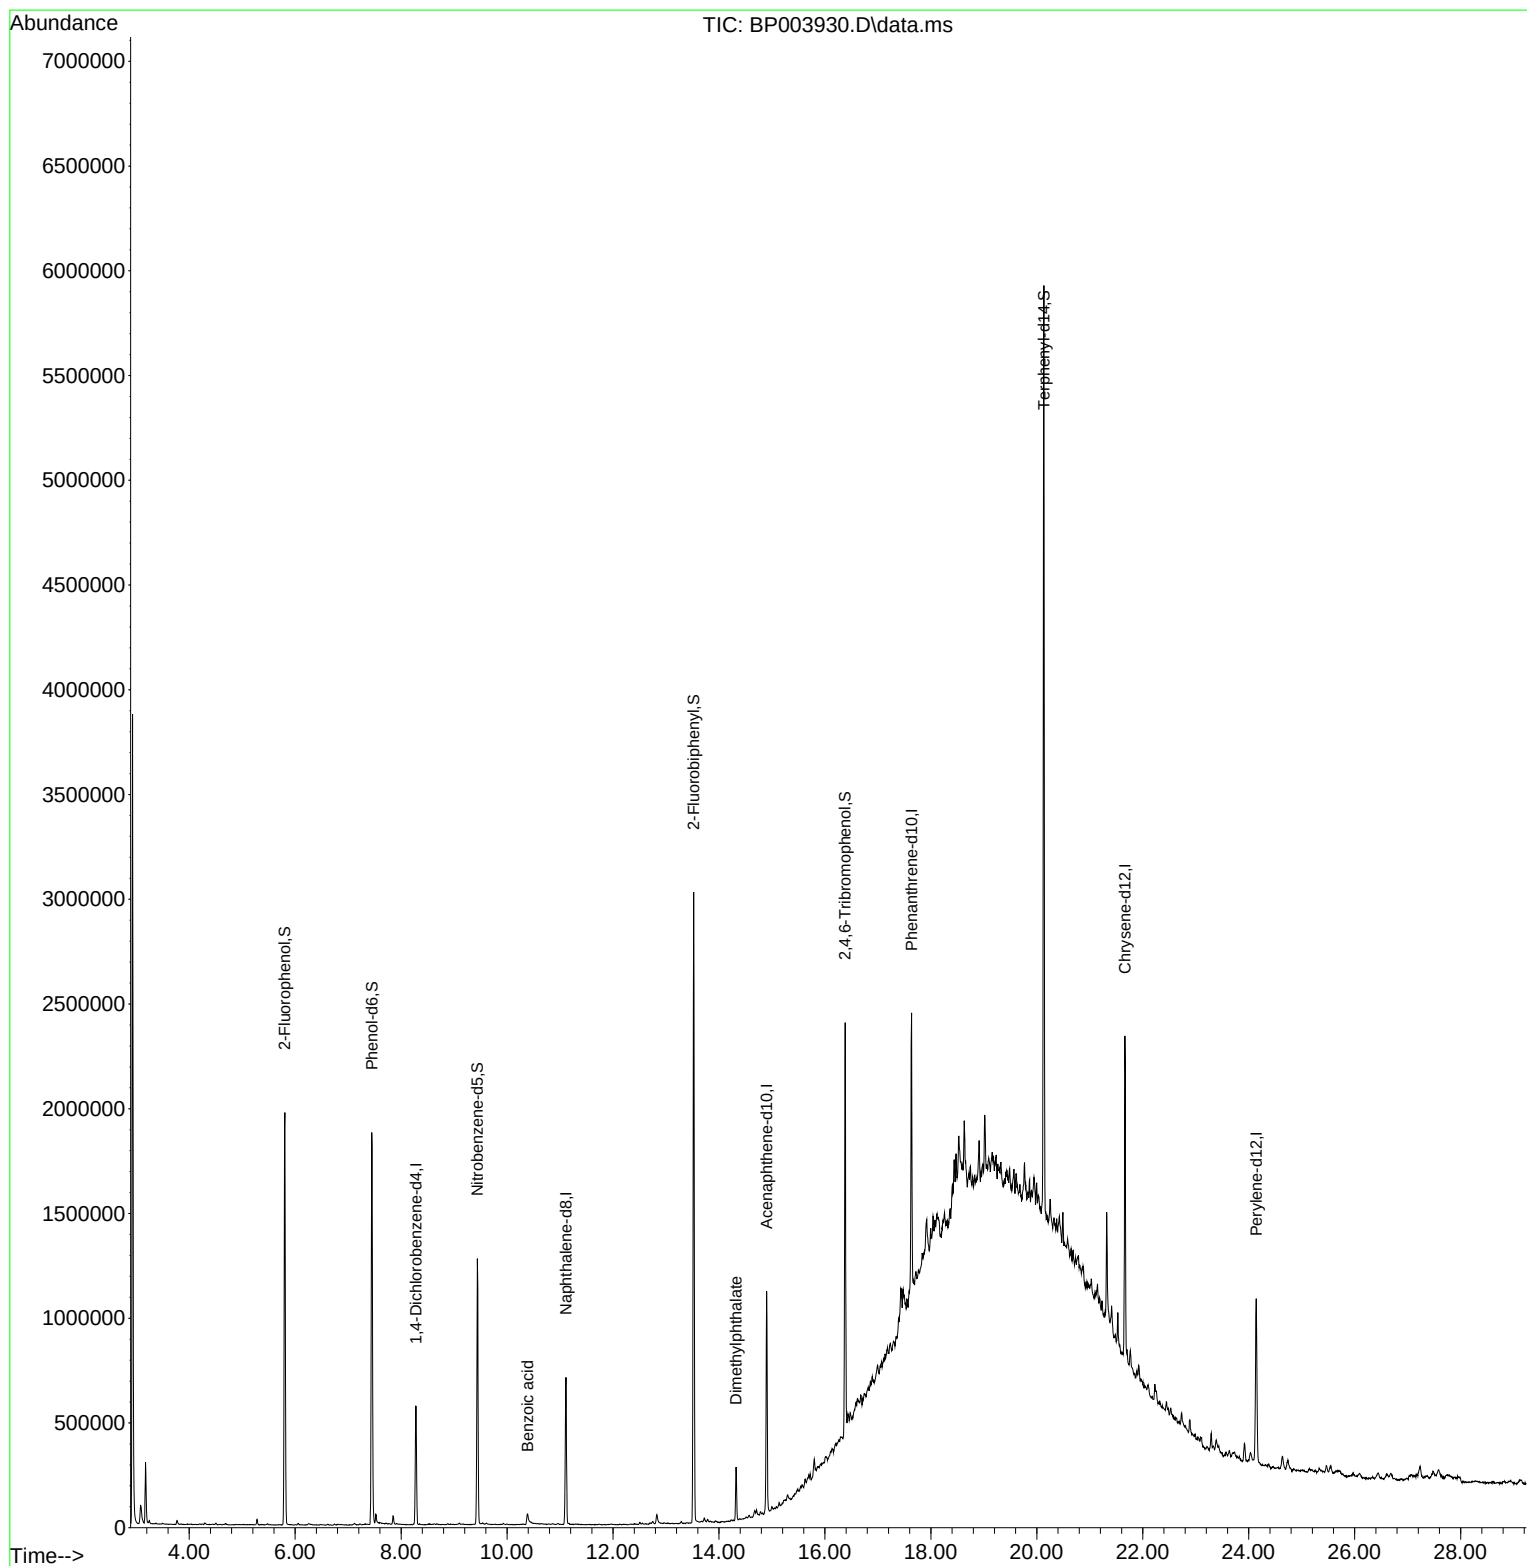


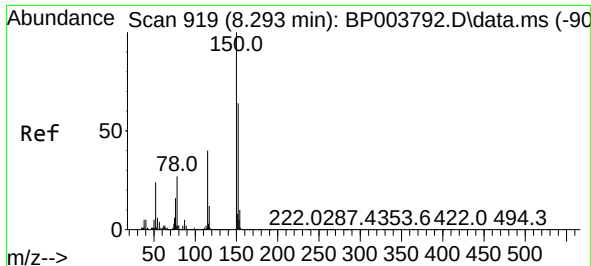


#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.281 min Scan# 917
Delta R.T. 0.000 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30

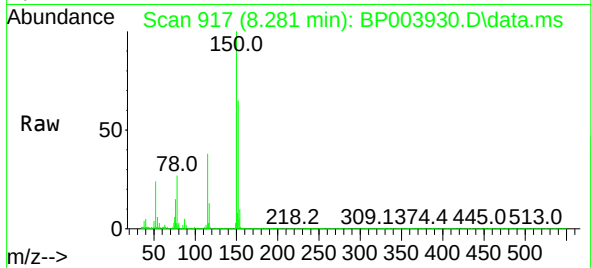



Tgt Ion:152 Resp: 152384
Ion Ratio Lower Upper
152 100
150 153.2 123.8 185.6
115 58.2 43.8 65.6

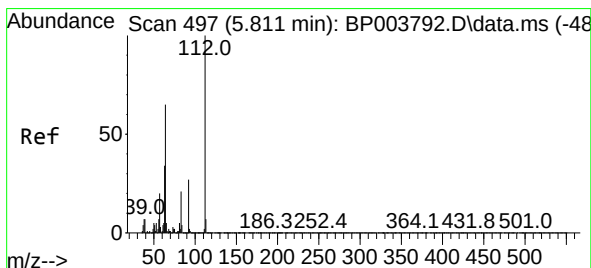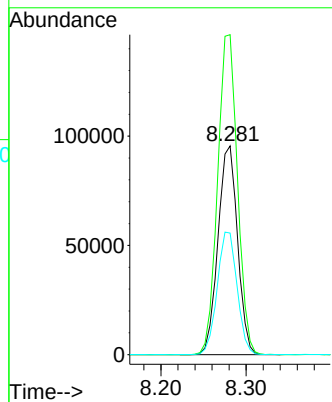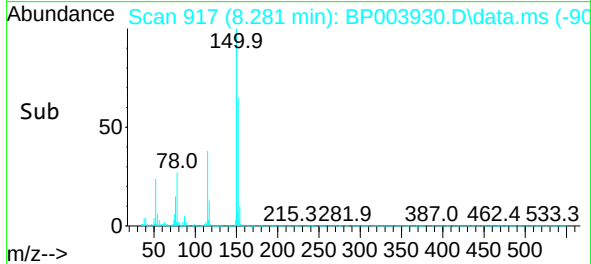

#5
2-Fluorophenol
Concen: 86.44 ng
RT: 5.805 min Scan# 496
Delta R.T. 0.006 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30

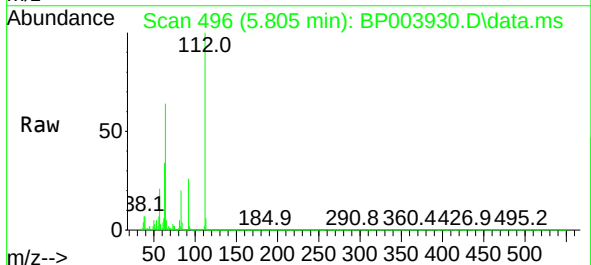


Tgt Ion:112 Resp: 789260
Ion Ratio Lower Upper
112 100
64 64.3 32.8 49.2#
63 34.2 17.0 25.4#

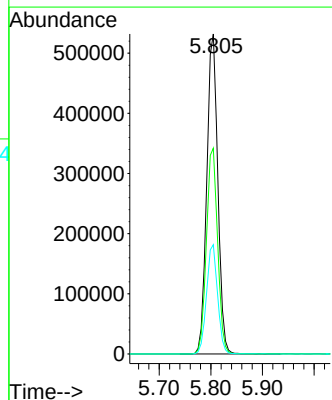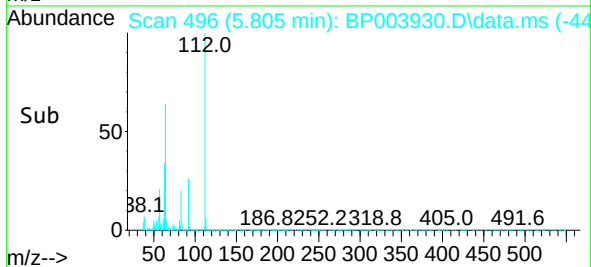

Instrument :
BNA_P
ClientSampleId :
TRANSFORMER-1-(1-4)


Manual Integrations
APPROVED

mohammad
11/12/2020 11:38:54 AM

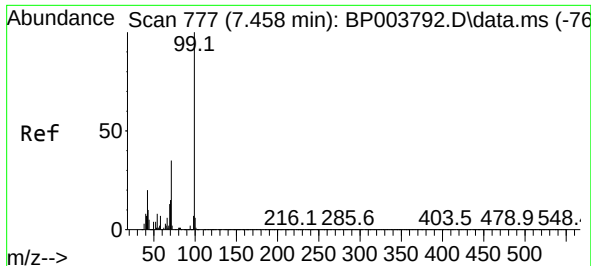

#7
Phenol-d6
Concen: 78.26 ng
RT: 7.446 min Scan# 775
Delta R.T. -0.006 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30




Instrument :
BNA_P
ClientSampleId :
TRANSFORMER-1-(1-4)

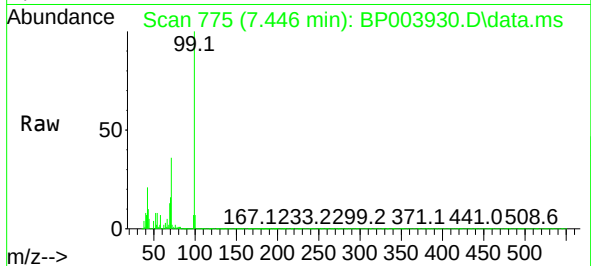


Tgt Ion: 99 Resp: 1025708
Ion Ratio Lower Upper
99 100
42 20.5 8.6 13.0#
71 36.3 23.4 35.2#

Manual Integrations
APPROVED



mohammad
11/12/2020 11:38:54 AM

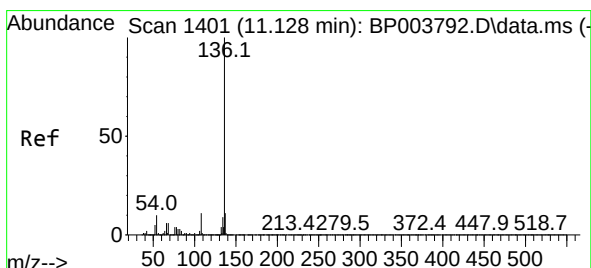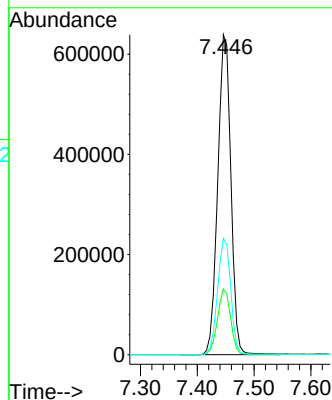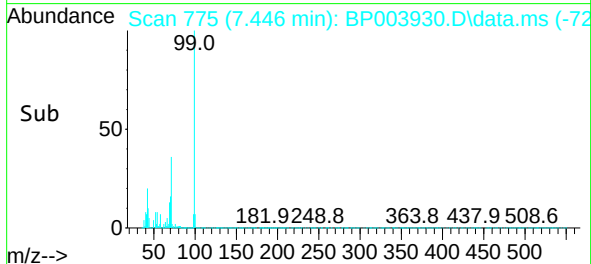


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.110 min Scan# 1398
Delta R.T. -0.000 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30

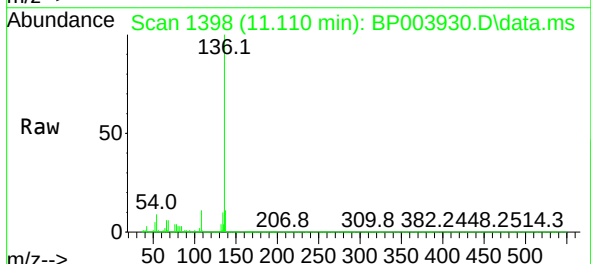


Tgt Ion: 136 Resp: 562343
Ion Ratio Lower Upper
136 100
137 11.2 8.6 13.0
54 9.1 3.6 5.4#
68 5.8 3.3 4.9#

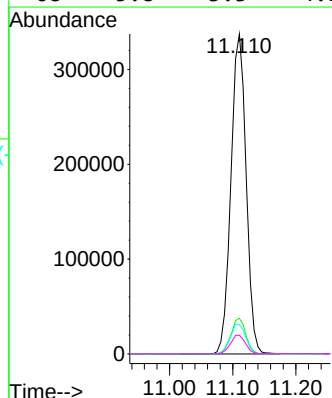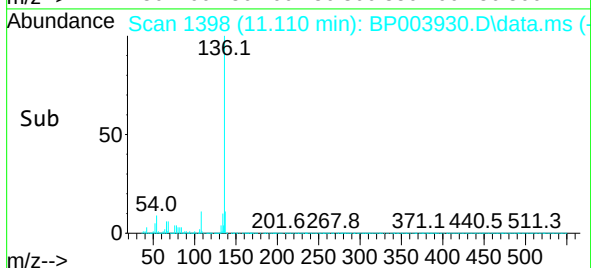

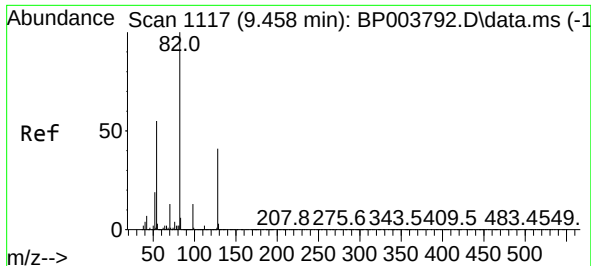

#23
Nitrobenzene-d5
Concen: 60.53 ng
RT: 9.440 min Scan# 1114
Delta R.T. -0.000 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30




Instrument :
BNA_P
ClientSampleId :
TRANSFORMER-1-(1-4)

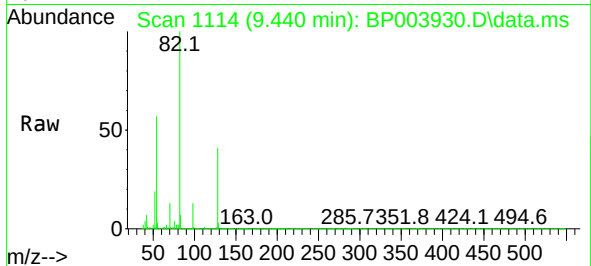


Tgt Ion: 82 Resp: 695033
Ion Ratio Lower Upper
82 100
128 40.9 45.6 68.4#
54 56.6 30.1 45.1#

Manual Integrations
APPROVED



mohammad
11/12/2020 11:38:54 AM

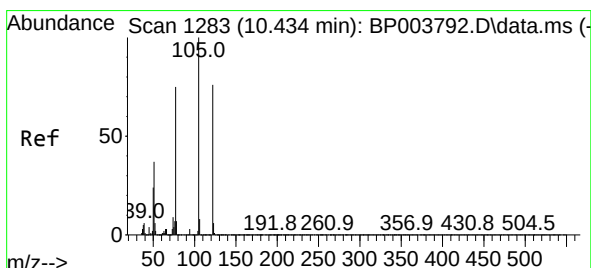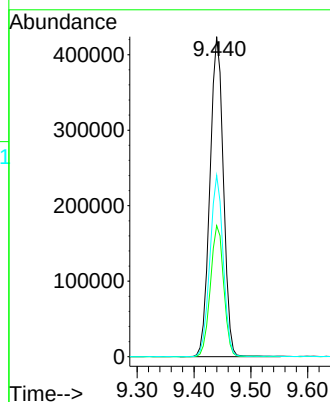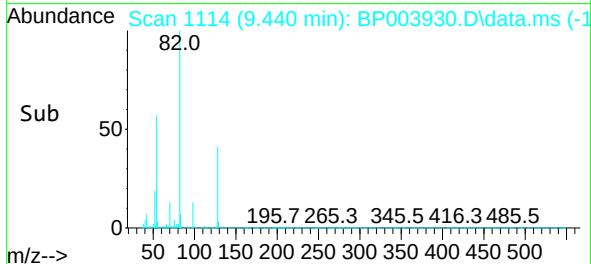


#32
Benzoic acid
Concen: 12.88 ng m
RT: 10.387 min Scan# 1275
Delta R.T. -0.041 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30

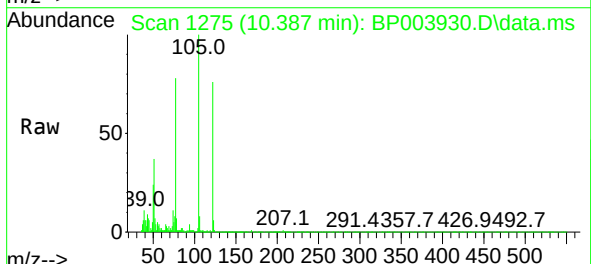


Tgt Ion: 122 Resp: 28848
Ion Ratio Lower Upper
122 100
105 131.0 94.1 134.1
77 102.1 50.1 90.1#

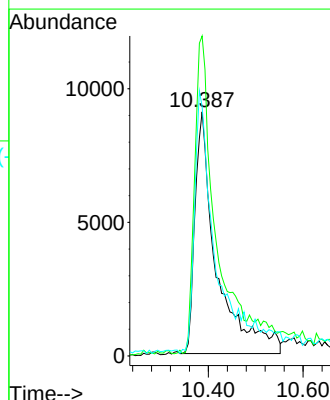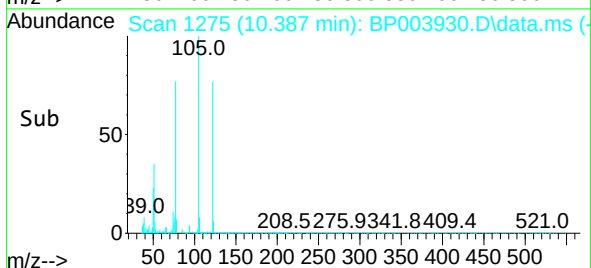

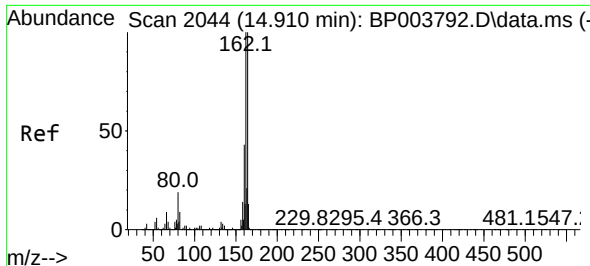

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.898 min Scan# 2042
Delta R.T. -0.006 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30




Instrument :
BNA_P
ClientSampleId :
TRANSFORMER-1-(1-4)

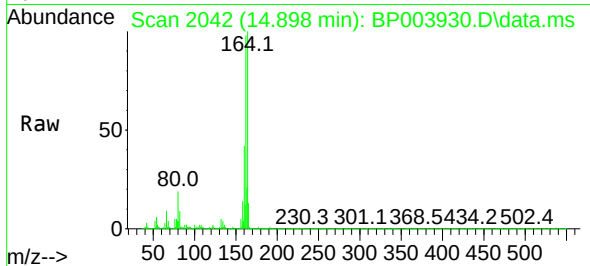


Tgt Ion:164 Resp: 353602
Ion Ratio Lower Upper
164 100
162 98.3 79.4 119.2
160 42.4 36.1 54.1

Manual Integrations
APPROVED



mohammad
11/12/2020 11:38:54 AM

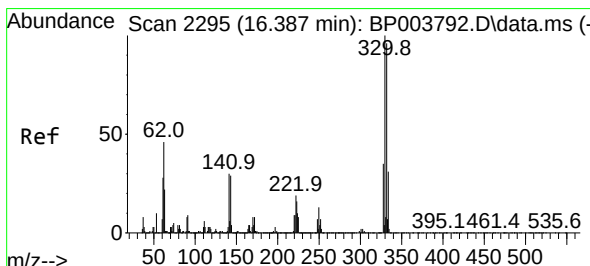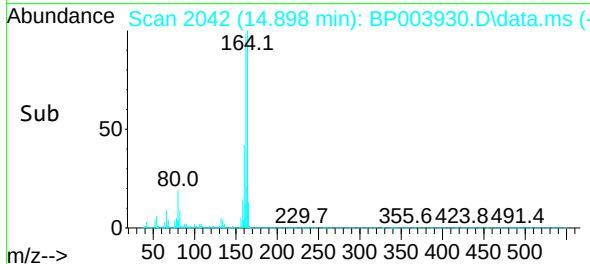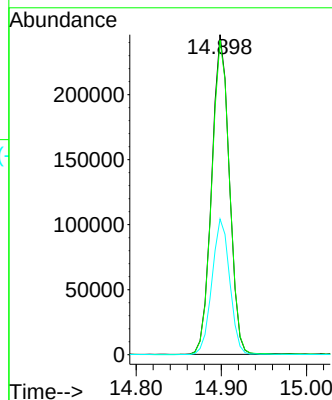


#42
2,4,6-Tribromophenol
Concen: 82.88 ng
RT: 16.381 min Scan# 2294
Delta R.T. -0.000 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30

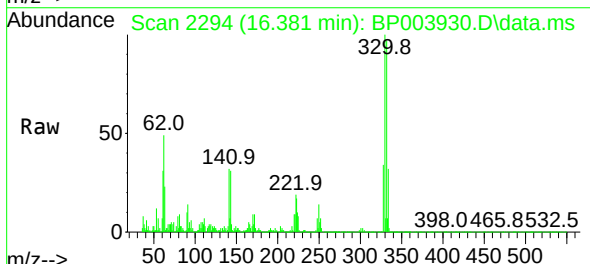


Tgt Ion:330 Resp: 366534
Ion Ratio Lower Upper
330 100
332 96.9 77.1 115.7
141 32.3 23.4 35.2

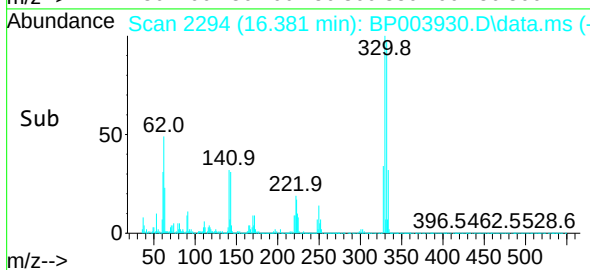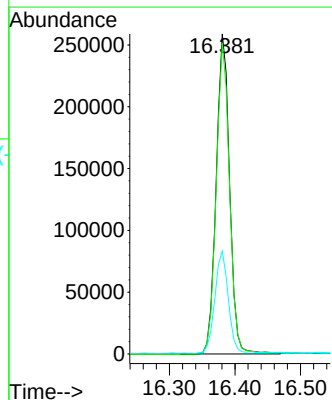

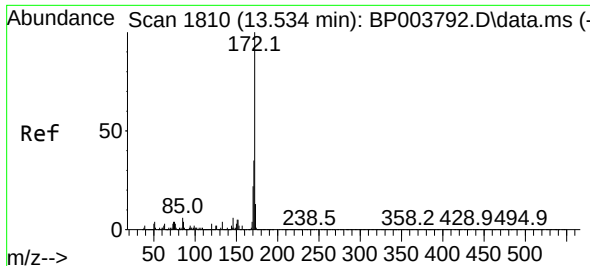

#45
2-Fluorobiphenyl
Concen: 59.53 ng
RT: 13.522 min Scan# 1808
Delta R.T. -0.000 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30




Instrument :
BNA_P
ClientSampleId :
TRANSFORMER-1-(1-4)

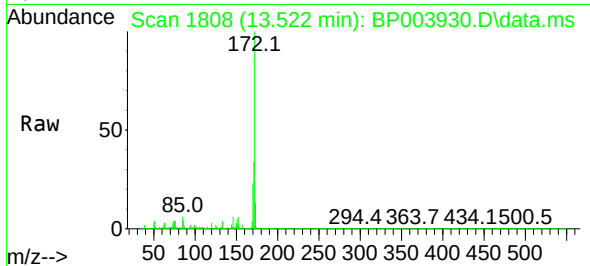


Tgt Ion:172 Resp: 1505689
Ion Ratio Lower Upper
172 100
171 34.4 28.5 42.7
170 22.8 19.2 28.8

Manual Integrations
APPROVED



mohammad
11/12/2020 11:38:54 AM

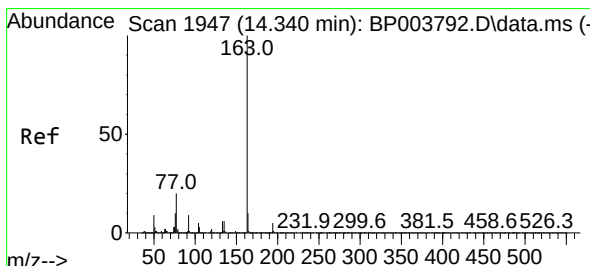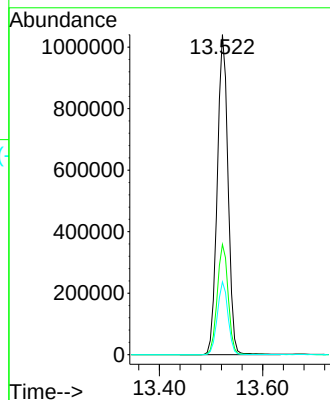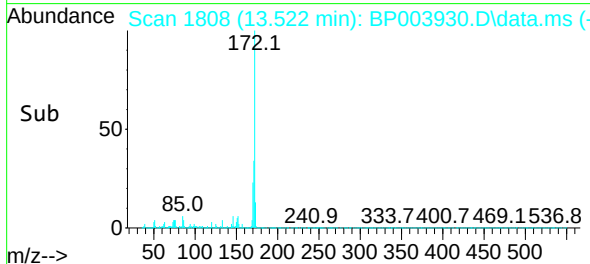


#50
Dimethylphthalate
Concen: 5.69 ng
RT: 14.322 min Scan# 1944
Delta R.T. -0.006 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30

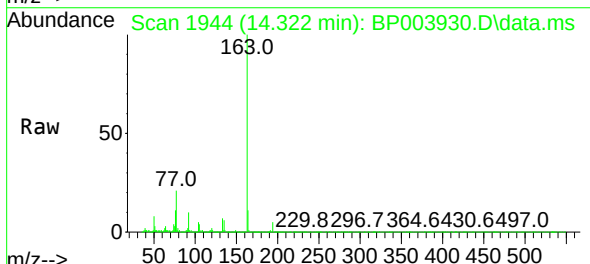


Tgt Ion:163 Resp: 157289
Ion Ratio Lower Upper
163 100
194 4.5 3.3 4.9
164 10.8 8.2 12.2

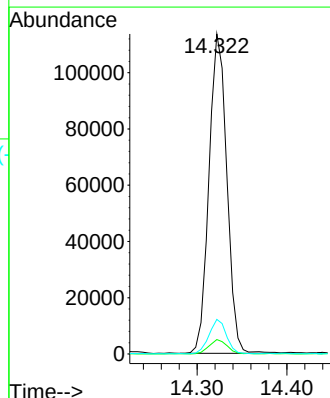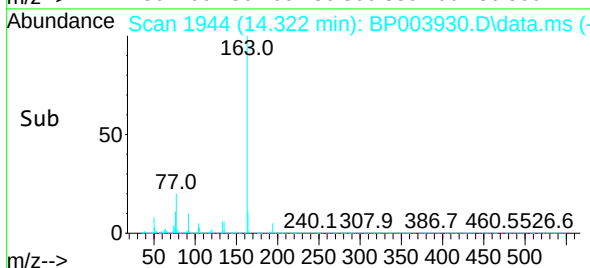

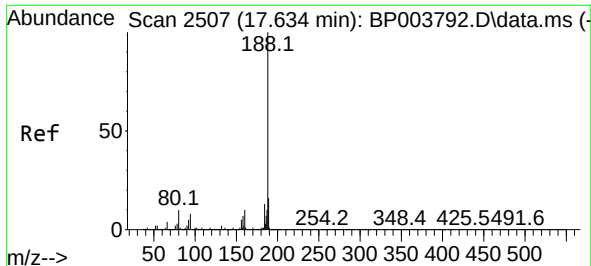

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.634 min Scan# 2507
Delta R.T. 0.006 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30




Instrument :
BNA_P
ClientSampleId :
TRANSFORMER-1-(1-4)

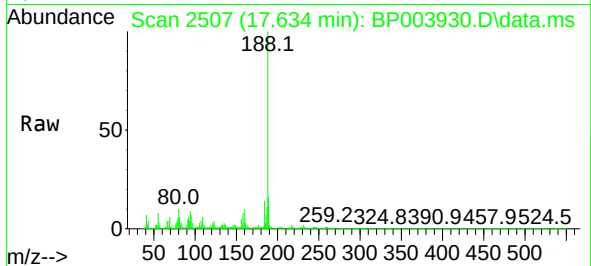

Tgt Ion:188 Resp: 755734
Ion Ratio Lower Upper
188 100
94 9.1 6.2 9.2
80 10.2 6.2 9.2#




Manual Integrations
APPROVED


mohammad
11/12/2020 11:38:54 AM

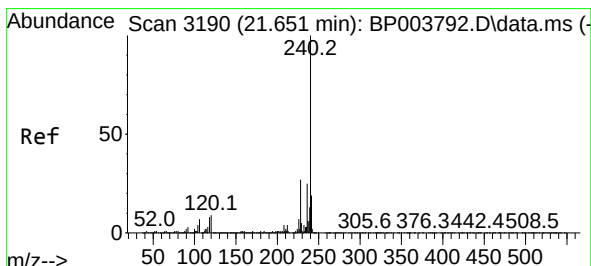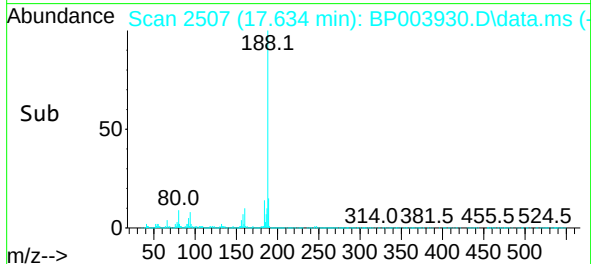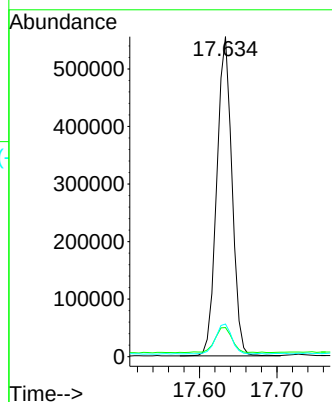

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.663 min Scan# 3192
Delta R.T. 0.006 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30

Tgt Ion:240 Resp: 727483
Ion Ratio Lower Upper
240 100
120 9.7 7.8 11.6
236 25.1 20.8 31.2

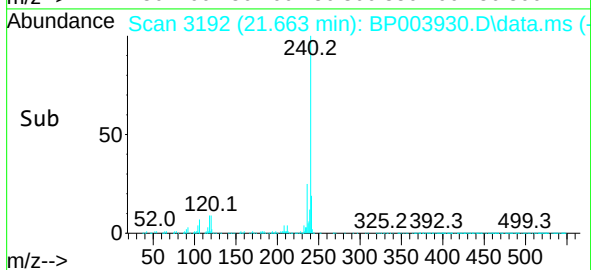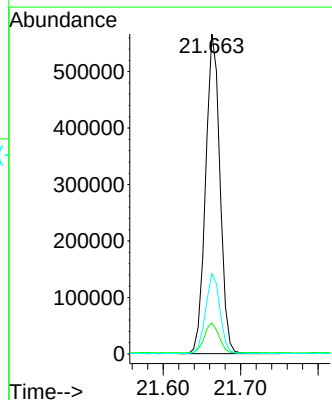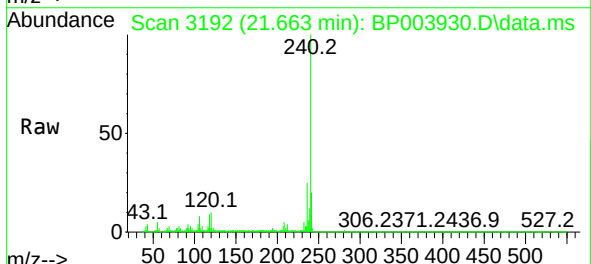

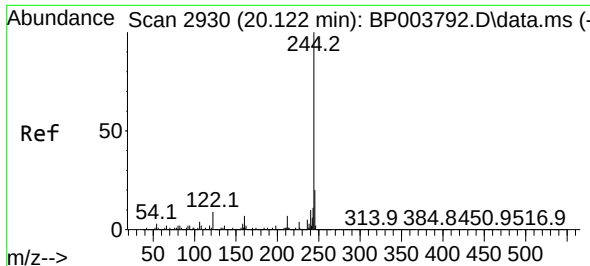





#79
Terphenyl-d14
Concen: 49.90 ng
RT: 20.133 min Scan# 2932
Delta R.T. 0.006 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30

Tgt Ion:244 Resp: 1878882
Ion Ratio Lower Upper
244 100
212 7.4 5.8 8.6
122 9.4 7.8 11.8

Instrument :
BNA_P
ClientSampleId :
TRANSFORMER-1-(1-4)

Manual Integrations
APPROVED

mohammad
11/12/2020 11:38:54 AM

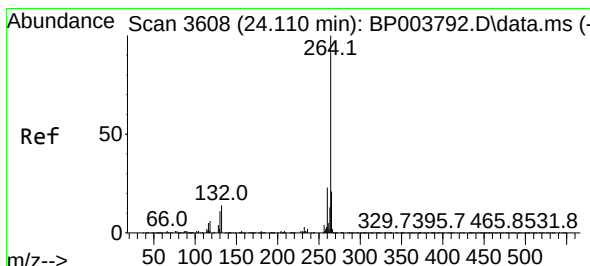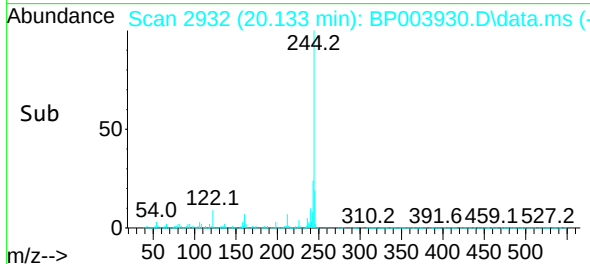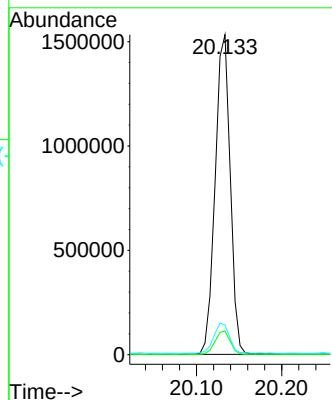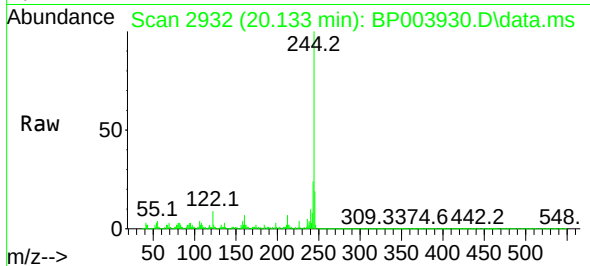

#86
Perylene-d12
Concen: 20.00 ng
RT: 24.139 min Scan# 3613
Delta R.T. 0.012 min
Lab File: BP003930.D
Acq: 11 Nov 2020 20:30

Tgt Ion:264 Resp: 619132
Ion Ratio Lower Upper
264 100
260 23.5 18.8 28.2
265 22.4 17.4 26.2

