
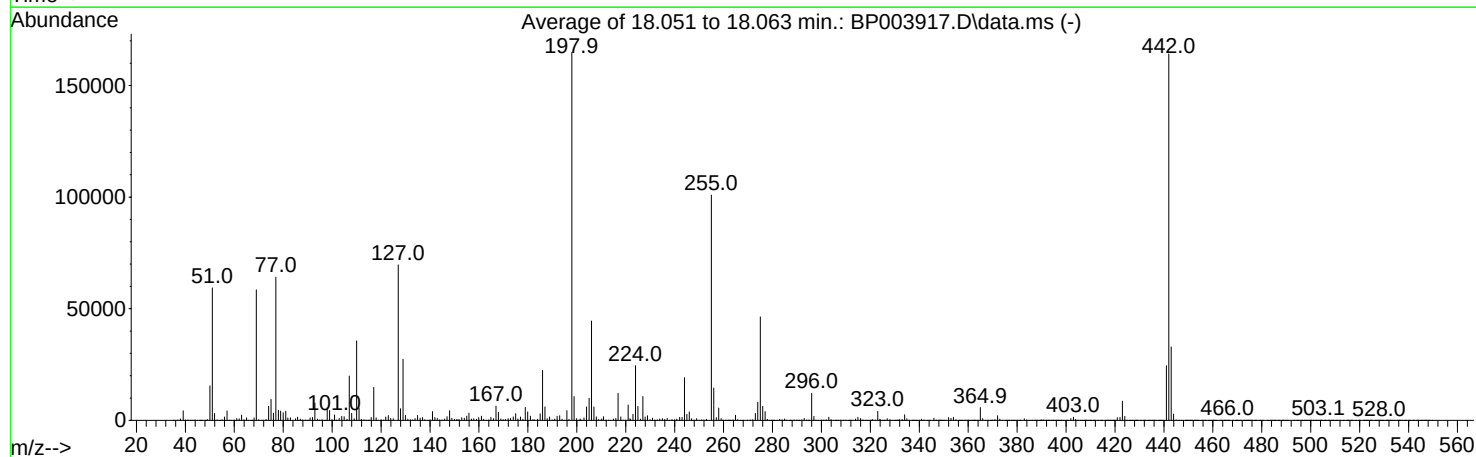


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111120\
 Data File : BP003917.D
 Acq On : 11 Nov 2020 12:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 10 13:41:24 2020

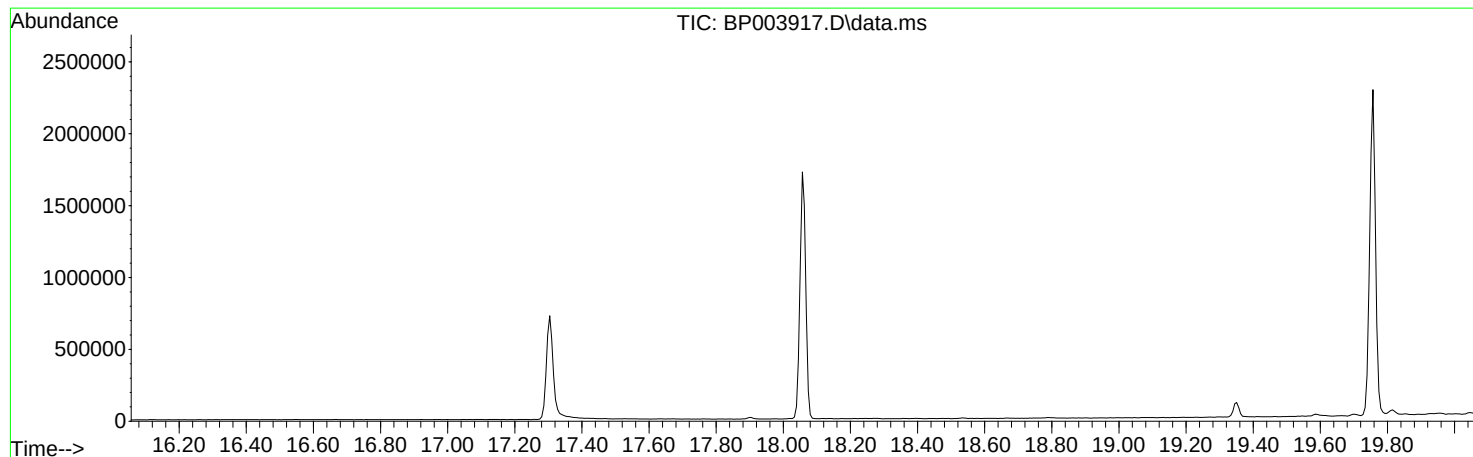

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	59341	PASS
68	69	0.00	2	1.9	1124	PASS
69	198	0.00	100	35.5	58452	PASS
70	69	0.00	2	0.5	303	PASS
127	198	10	80	42.3	69655	PASS
197	198	0.00	2	0.2	410	PASS
198	198	100	100	100.0	164774	PASS
199	198	5	9	6.5	10686	PASS
275	198	10	60	28.1	46355	PASS
365	198	1	100	3.5	5704	PASS
441	198	0.01	100	14.8	24419	PASS
442	198	50	100	99.6	164107	PASS
443	442	15	24	20.0	32883	PASS