
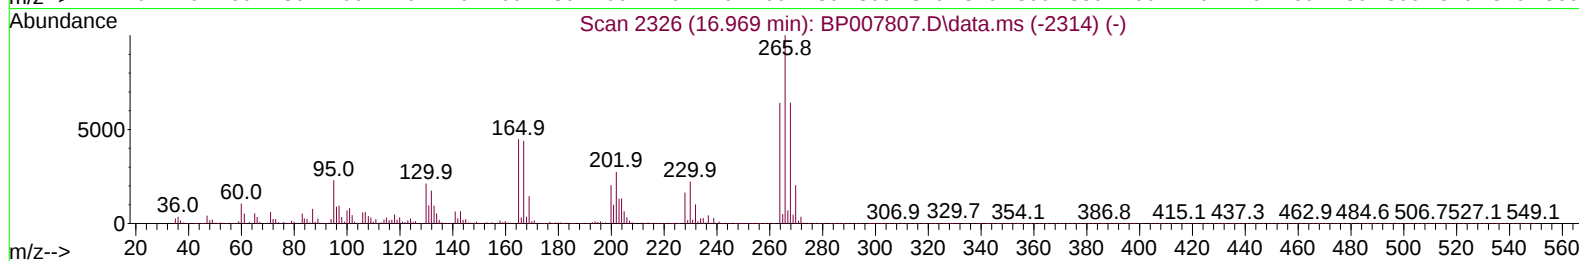
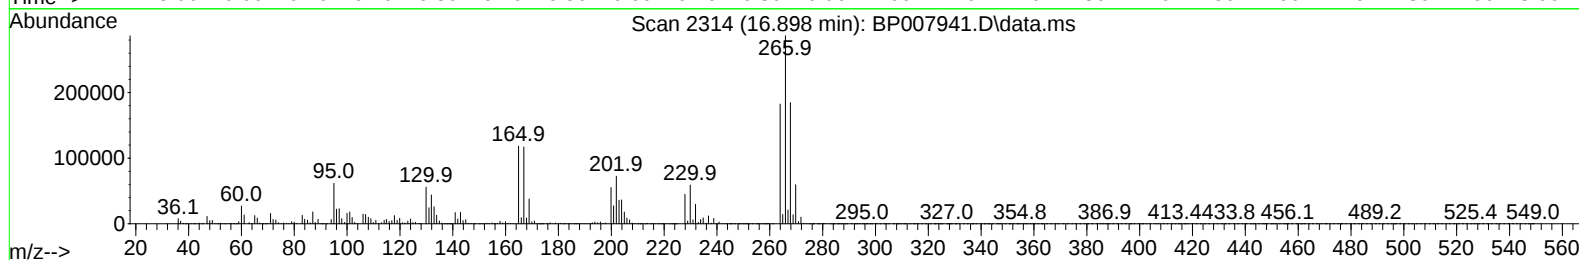


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111121\
 Data File : BP007941.D
 Acq On : 11 Nov 2021 12:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 13:48:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 10:45:24 2021
 Response via : Initial Calibration

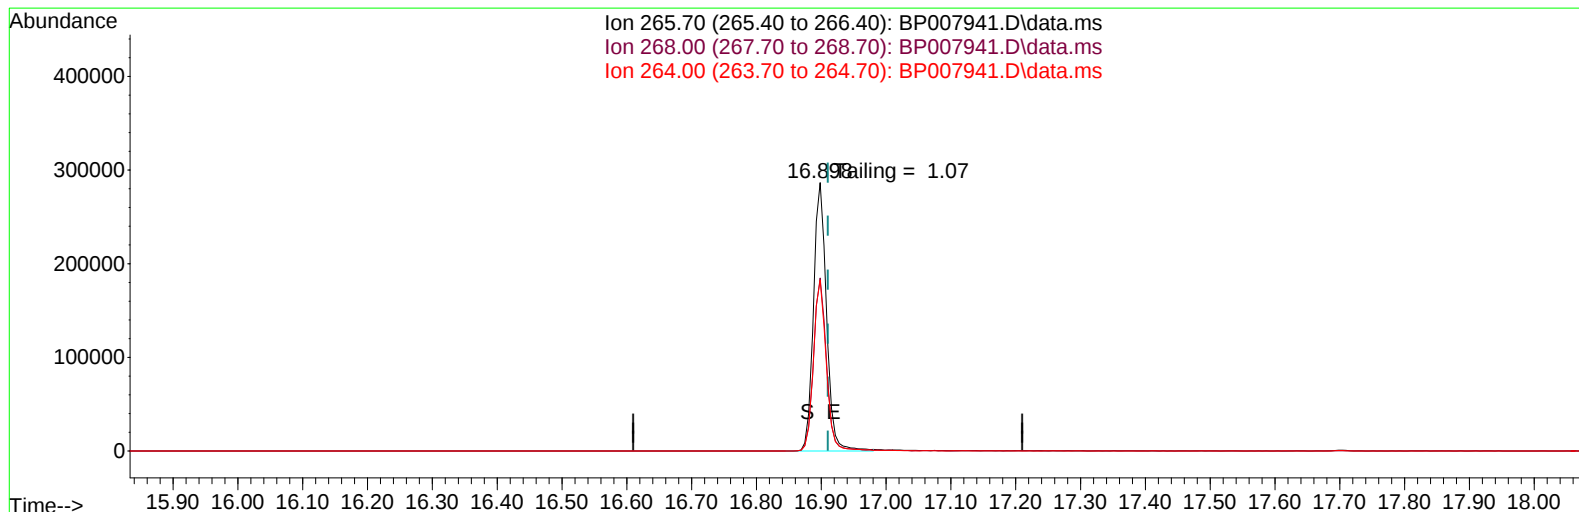

TIC: BP007941.D\data.ms

(70) Pentachlorophenol (C)




16.898min (-0.012) 3405931.18 ng

response 405911

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	64.45
264.00	60.90	63.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111121\
 Data File : BP007941.D
 Acq On : 11 Nov 2021 12:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 13:48:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 09 10:45:24 2021
 Response via : Initial Calibration

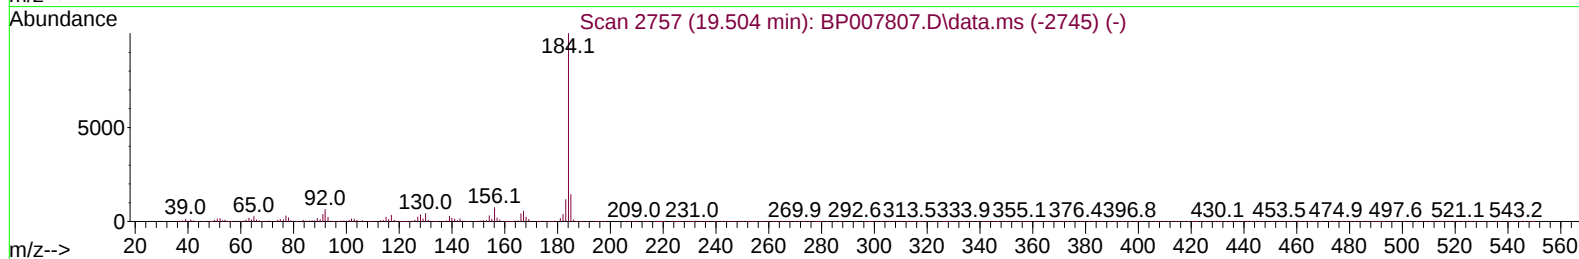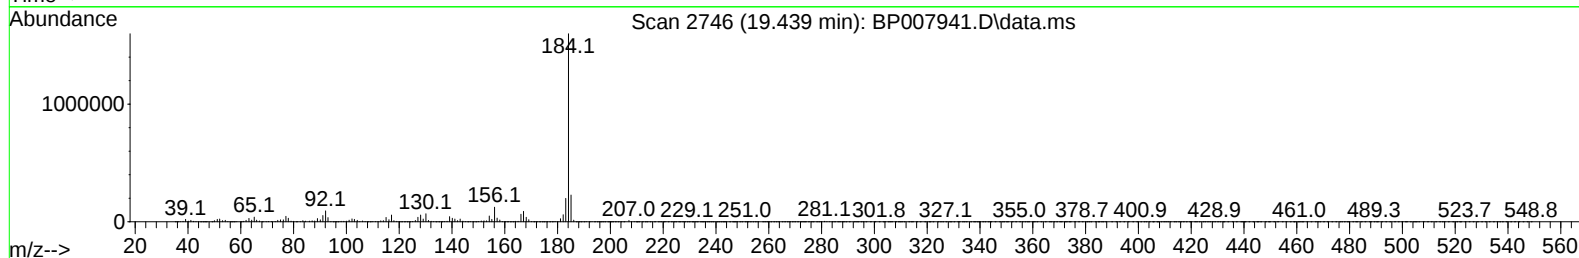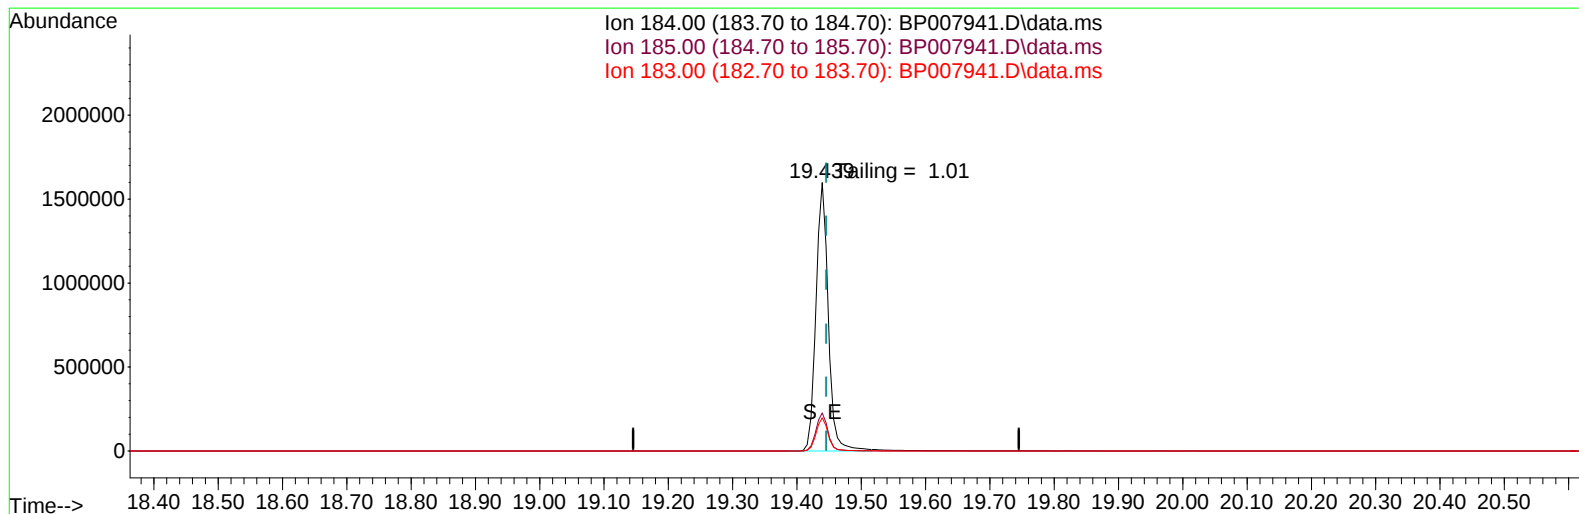

TIC: BP007941.D\data.ms

(77) Benzidine**19.439min (-0.006) 1005693.83 ng****response 2154445**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.23
183.00	11.40	12.42
0.00	0.00	0.00