

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111121\
 Data File : BP007943.D
 Acq On : 11 Nov 2021 13:41
 Operator : CG/JU
 Sample : PB140664BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB140664BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.440	359	366	383	rBV	2517683	3678433	31.05%	8.177%
2	7.028	628	636	655	rVB	2344659	3812005	32.18%	8.474%
3	7.852	768	776	785	rBV	514546	786053	6.64%	1.747%
4	9.010	963	973	984	rBV	1338021	2207405	18.63%	4.907%
5	10.652	1245	1252	1267	rVB	586092	1021442	8.62%	2.271%
6	13.116	1662	1671	1684	rBV	3959375	5949281	50.22%	13.225%
7	14.487	1897	1904	1918	rBV	1052701	1607330	13.57%	3.573%
8	15.981	2149	2158	2175	rBV	3865621	5656231	47.75%	12.574%
9	17.245	2364	2373	2386	rBV	1549460	2189280	18.48%	4.867%
10	19.810	2803	2809	2814	rBV	9273253	11846697	100.00%	26.335%
11	21.339	3063	3069	3077	rBV	2262488	3039266	25.65%	6.756%
12	23.745	3471	3478	3490	rVB2	1555792	3191497	26.94%	7.095%




Sum of corrected areas: 44984920

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111121\
Data File : BP007943.D
Acq On : 11 Nov 2021 13:41
Operator : CG/JU
Sample : PB140664BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140664BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

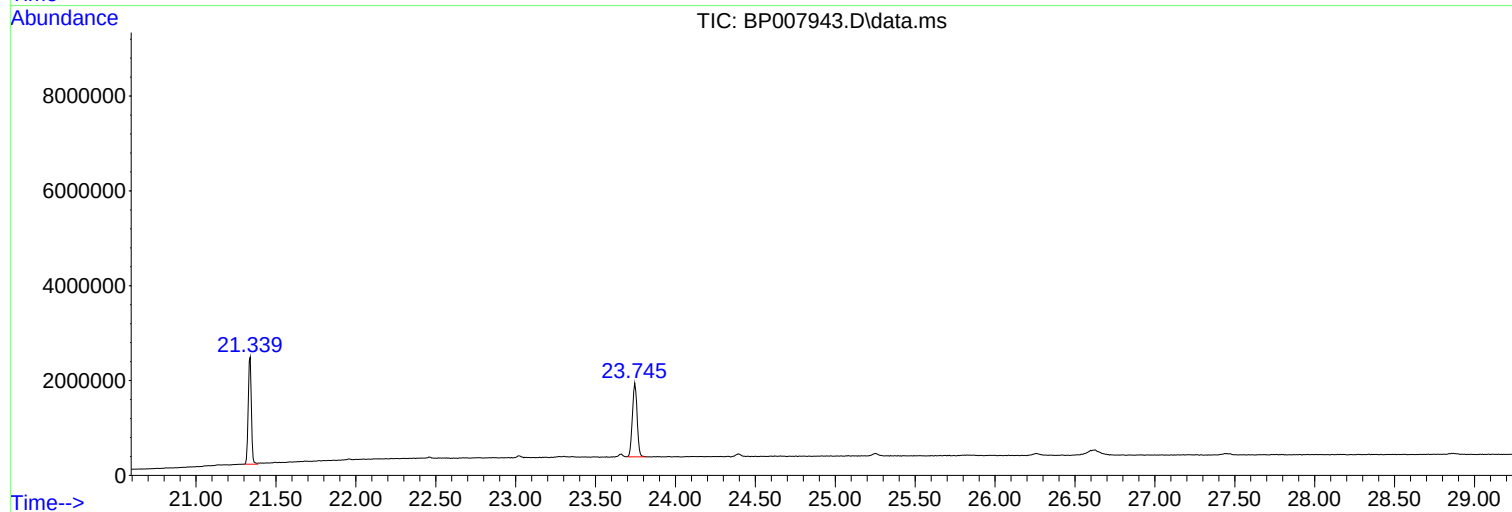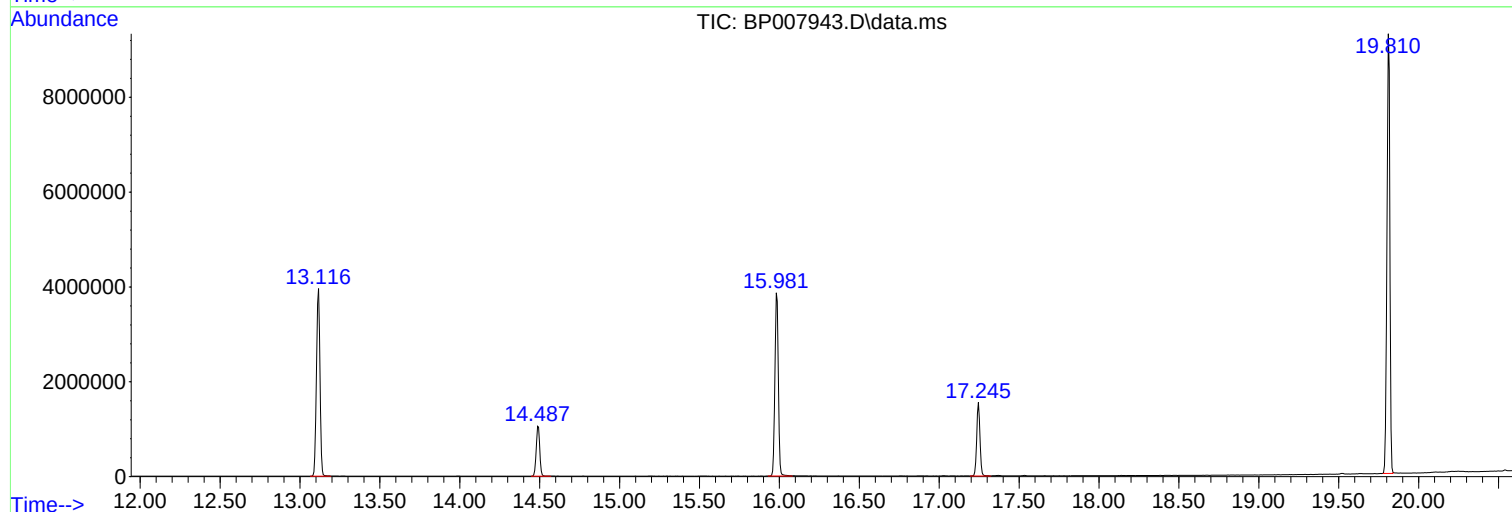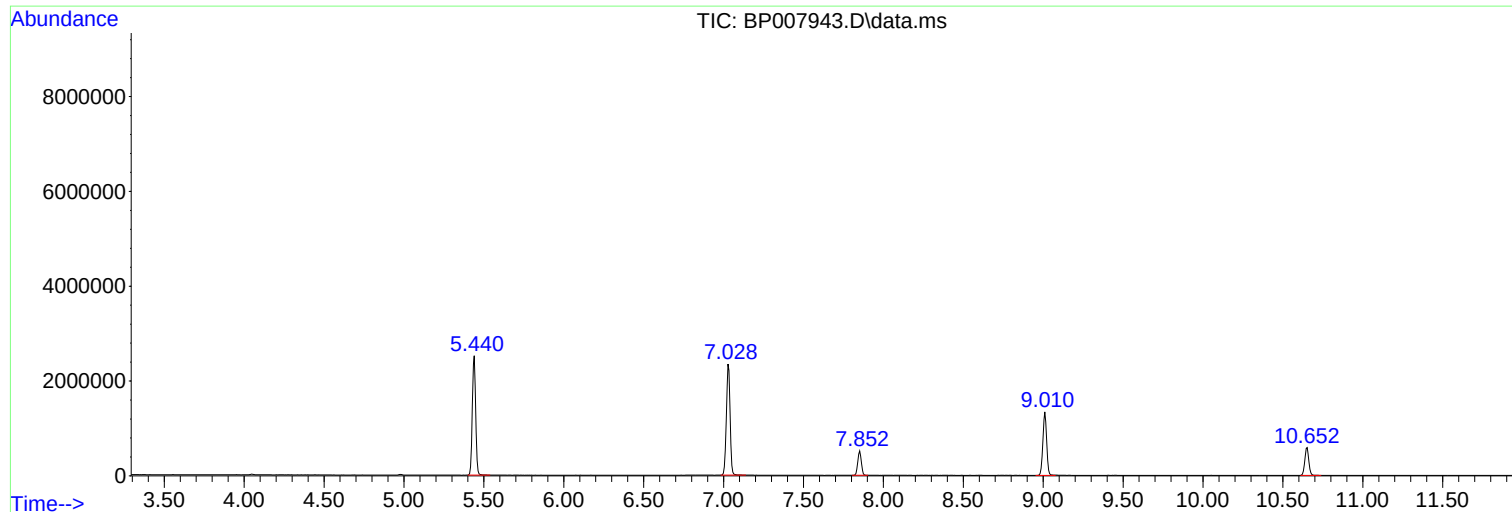

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111121\
Data File : BP007943.D
Acq On : 11 Nov 2021 13:41
Operator : CG/JU
Sample : PB140664BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140664BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111121\
Data File : BP007943.D
Acq On : 11 Nov 2021 13:41
Operator : CG/JU
Sample : PB140664BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140664BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------