
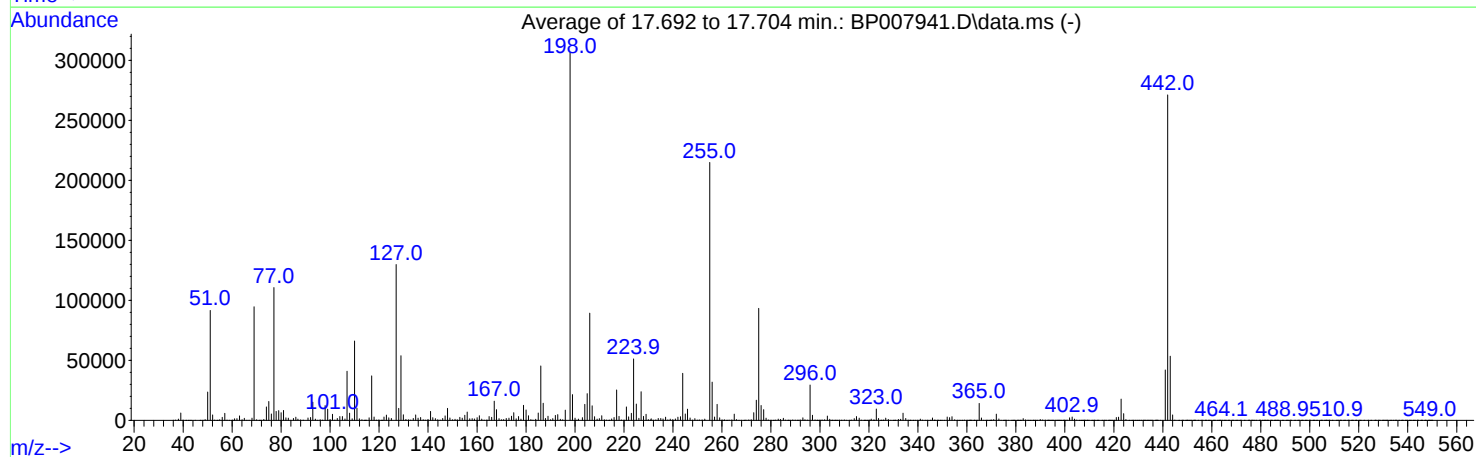


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111121\
 Data File : BP007941.D
 Acq On : 11 Nov 2021 12:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 11 13:53:53 2021

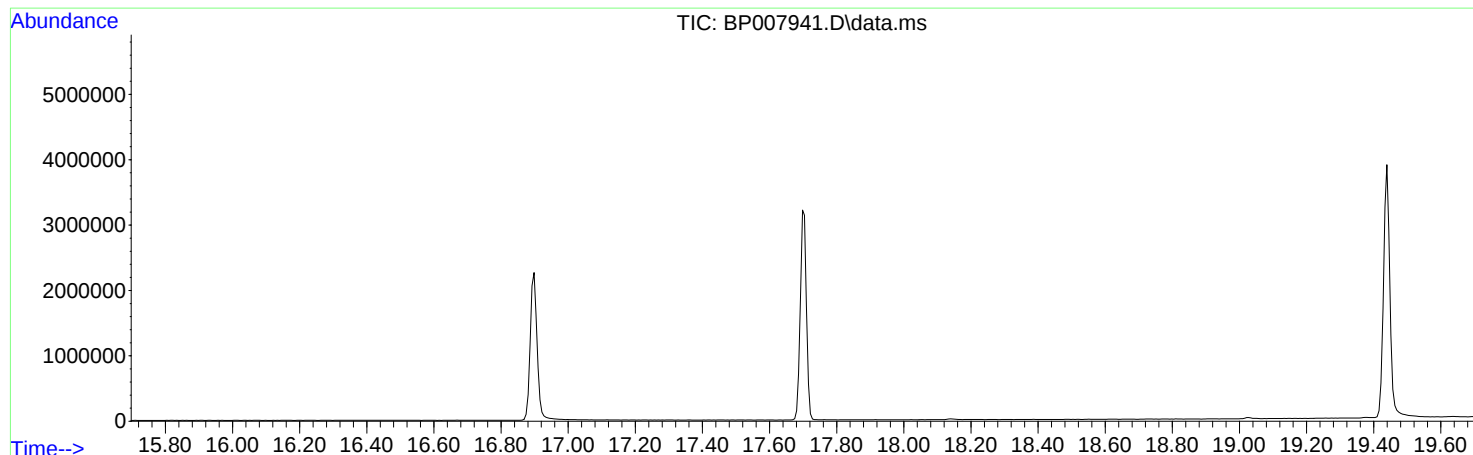




AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	91617	PASS
68	69	0.00	2	2.0	1884	PASS
69	198	0.00	100	30.9	94736	PASS
70	69	0.00	2	0.6	598	PASS
127	198	10	80	42.4	129903	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	306581	PASS
199	198	5	9	7.0	21478	PASS
275	198	10	60	30.4	93320	PASS
365	198	1	100	4.6	14161	PASS
441	198	0.01	100	13.7	42040	PASS
442	442	100	100	100.0	271232	PASS
443	442	15	24	19.7	53467	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111121\
Data File : BP007941.D
Acq On : 11 Nov 2021 12:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 11 13:48:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 10:45:24 2021
Response via : Initial Calibration

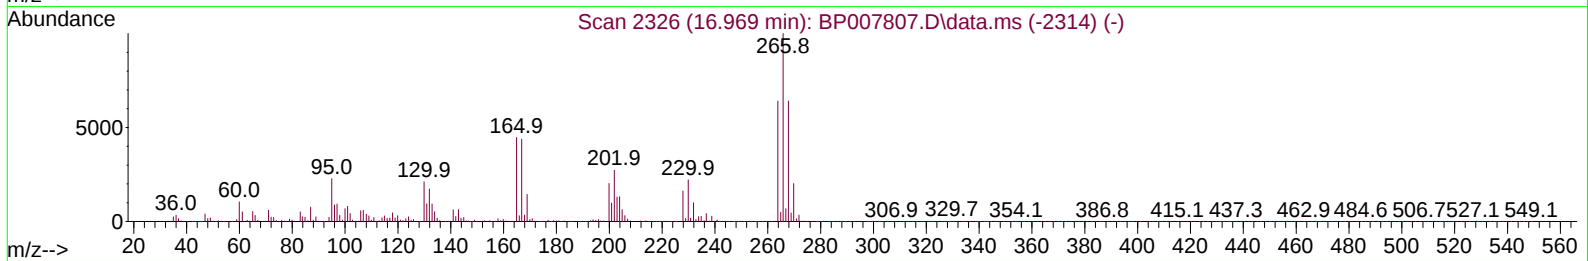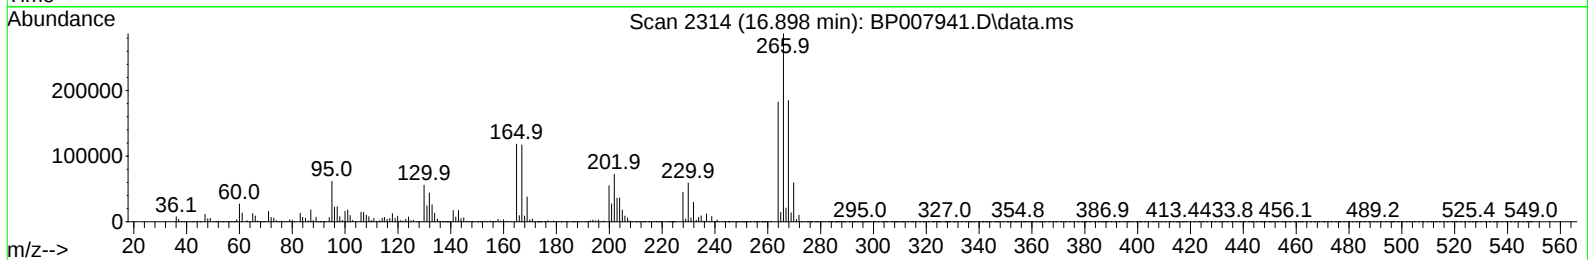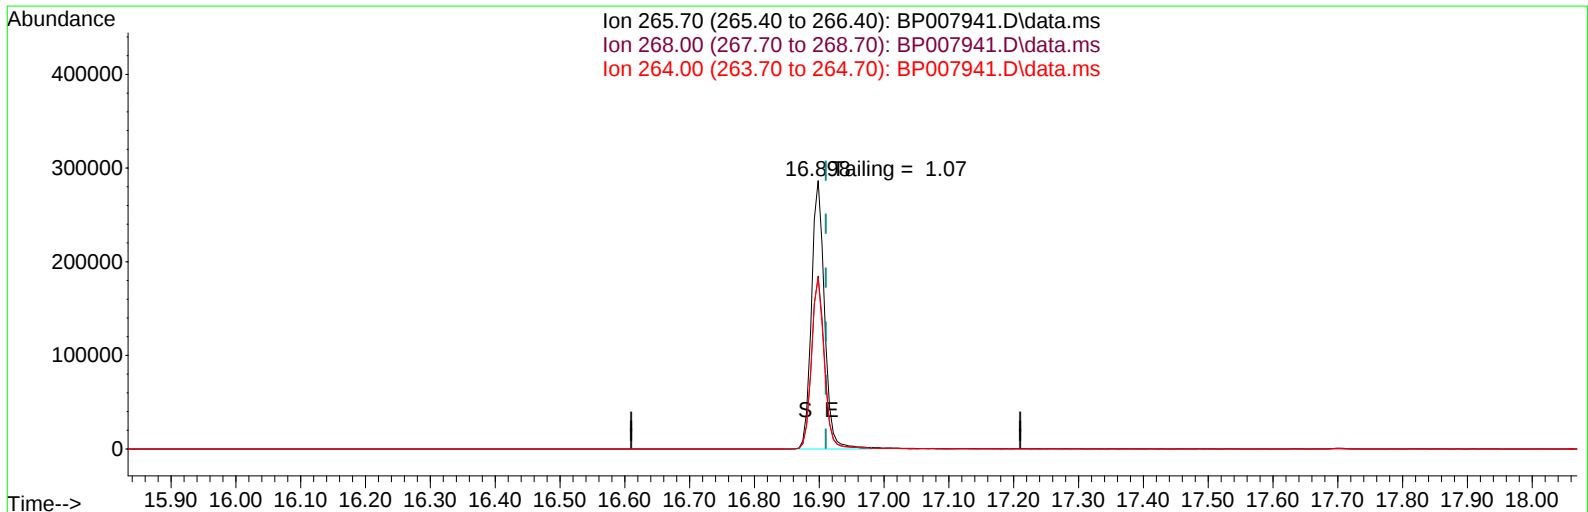

TIC: BP007941.D\data.ms

(70) Pentachlorophenol (C)

16.898min (-0.012) 3405931.18 ng




response 405911

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.60	64.45
264.00	60.90	63.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111121\
Data File : BP007941.D
Acq On : 11 Nov 2021 12:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 11 13:48:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 09 10:45:24 2021
Response via : Initial Calibration

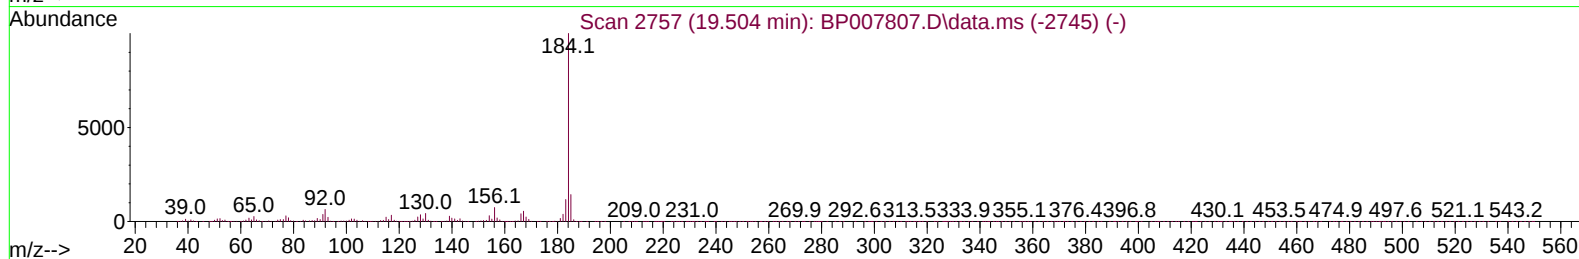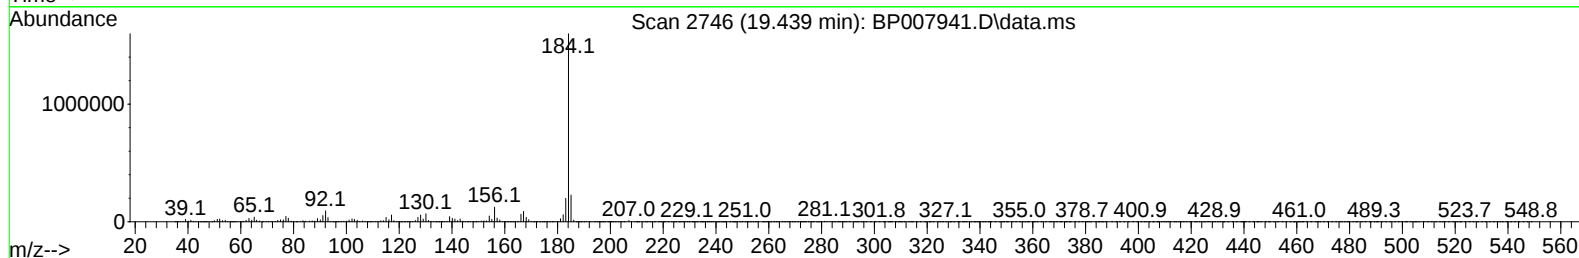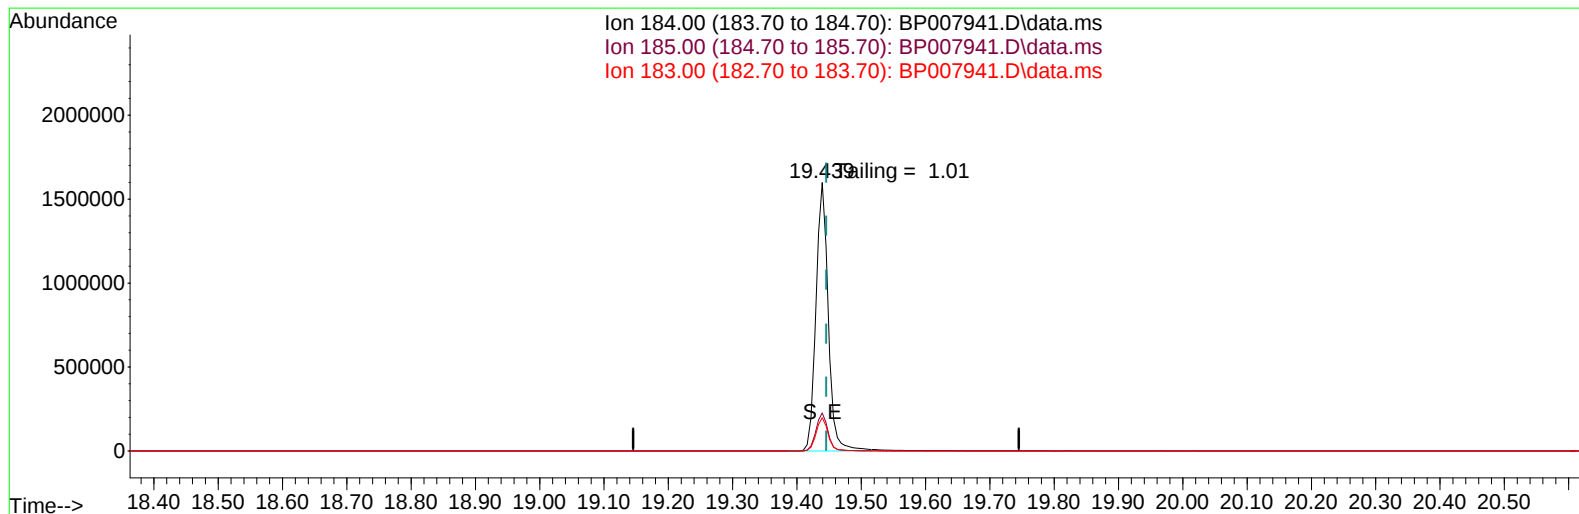

TIC: BP007941.D\data.ms

(77) Benzidine

19.439min (-0.006) 1005693.83 ng

response 2154445

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.23
183.00	11.40	12.42
0.00	0.00	0.00

Instrument :
BNA_P
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2021	BNA_P	BP007941.D
Compound Name	Response	Retention Time
DDT	1263635	20.64
DDD	19950	20.21
DDE	2052	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22002	1285637	1.71

Instrument :
BNA_P
ClientSampleId :
DFTPP