

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111122\
 Data File : BP012612.D
 Acq On : 11 Nov 2022 11:45
 Operator : CG/JU
 Sample : PB148940BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK940

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.223	36	40	48	rVB	61377	87498	1.06%	0.127%
2	3.646	110	112	128	rBV	282743	535001	6.49%	0.779%
3	3.952	161	164	168	rVB	11673	14298	0.17%	0.021%
4	6.952	667	674	693	rBV	864838	1554782	18.87%	2.264%
5	7.105	693	700	715	rVB	792070	1324877	16.08%	1.929%
6	7.299	724	733	744	rBV	942826	1557965	18.91%	2.268%
7	7.763	805	812	824	rBV	742585	1255795	15.24%	1.828%
8	8.487	928	935	960	rBV	1095041	2010407	24.40%	2.927%
9	8.934	1004	1011	1030	rBV	919092	1588927	19.28%	2.313%
10	9.652	1125	1133	1151	rBV	731394	1303732	15.82%	1.898%
11	10.199	1218	1226	1261	rBV	1013516	2025158	24.58%	2.948%
12	10.563	1280	1288	1302	rBV	1169244	2028509	24.62%	2.953%
13	10.716	1307	1314	1339	rBV	643226	1411444	17.13%	2.055%
14	12.181	1553	1563	1572	rBV2	14184	38641	0.47%	0.056%
15	13.316	1750	1756	1759	rVB8	5292	9680	0.12%	0.014%
16	13.834	1833	1844	1857	rBV	2107242	3175031	38.53%	4.623%
17	14.110	1884	1891	1911	rBV	2552032	3837139	46.57%	5.587%
18	14.416	1936	1943	1961	rBV	1929634	2901602	35.21%	4.225%
19	14.669	1979	1986	2010	rBV	482525	1471945	17.86%	2.143%
20	15.416	2106	2113	2127	rBV	3261074	4950170	60.08%	7.207%
21	15.557	2131	2137	2150	rVV	961252	1533194	18.61%	2.232%
22	15.657	2151	2154	2166	rVB6	22270	47824	0.58%	0.070%
23	16.851	2353	2357	2362	rBV8	5115	10066	0.12%	0.015%
24	16.969	2373	2377	2383	rBV4	5410	9434	0.11%	0.014%
25	17.181	2407	2413	2424	rBV	2467293	3604703	43.75%	5.248%
26	17.281	2424	2430	2446	rVV2	3679618	5694579	69.11%	8.291%
27	18.081	2562	2566	2574	rBV7	22319	46040	0.56%	0.067%
28	19.104	2736	2740	2744	rBV2	47913	68168	0.83%	0.099%
29	19.175	2748	2752	2757	rBV	50221	73807	0.90%	0.107%
30	19.528	2806	2812	2827	rBV	5079799	7006959	85.04%	10.202%
31	21.280	3105	3110	3121	rBV	3463065	4622605	56.10%	6.730%
32	23.504	3481	3488	3504	rBV2	3951763	8239787	100.00%	11.997%
33	23.657	3508	3514	3527	rVB2	2236583	4644741	56.37%	6.762%




Sum of corrected areas: 68684508

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111122\
Data File : BP012612.D
Acq On : 11 Nov 2022 11:45
Operator : CG/JU
Sample : PB148940BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

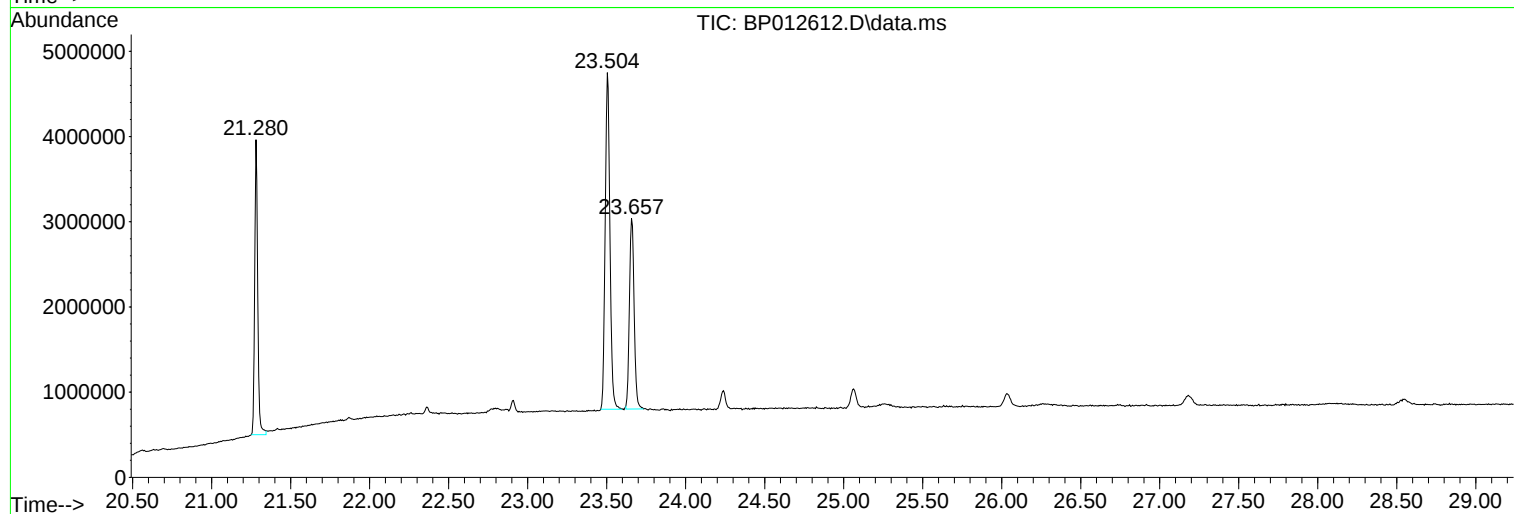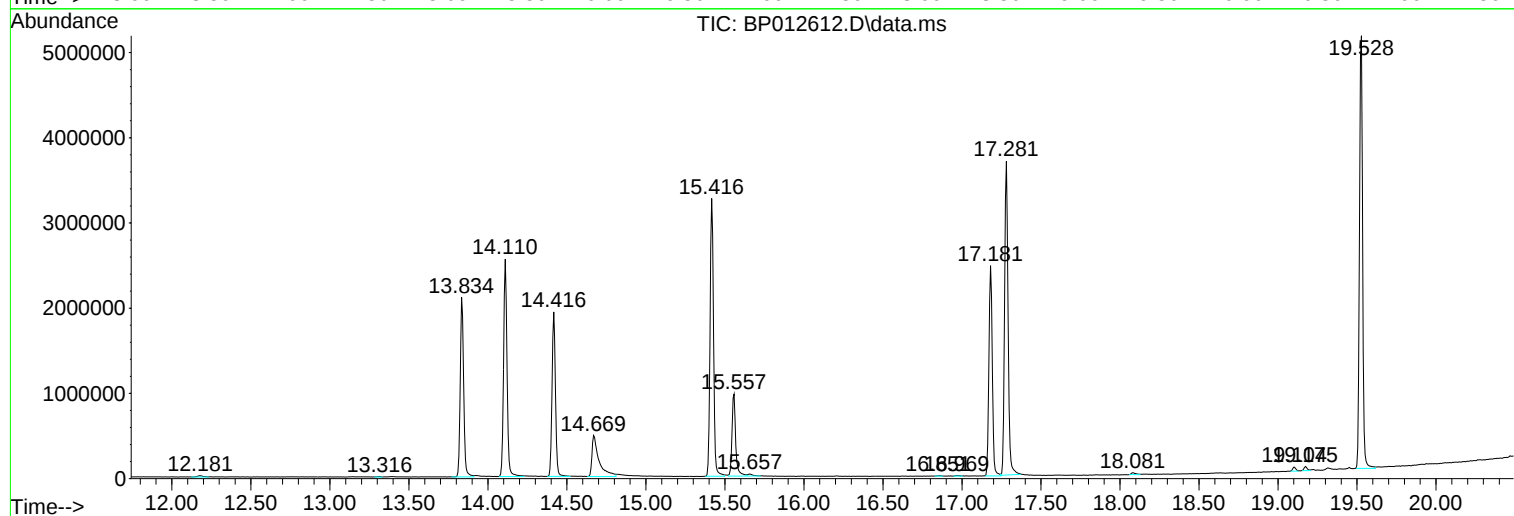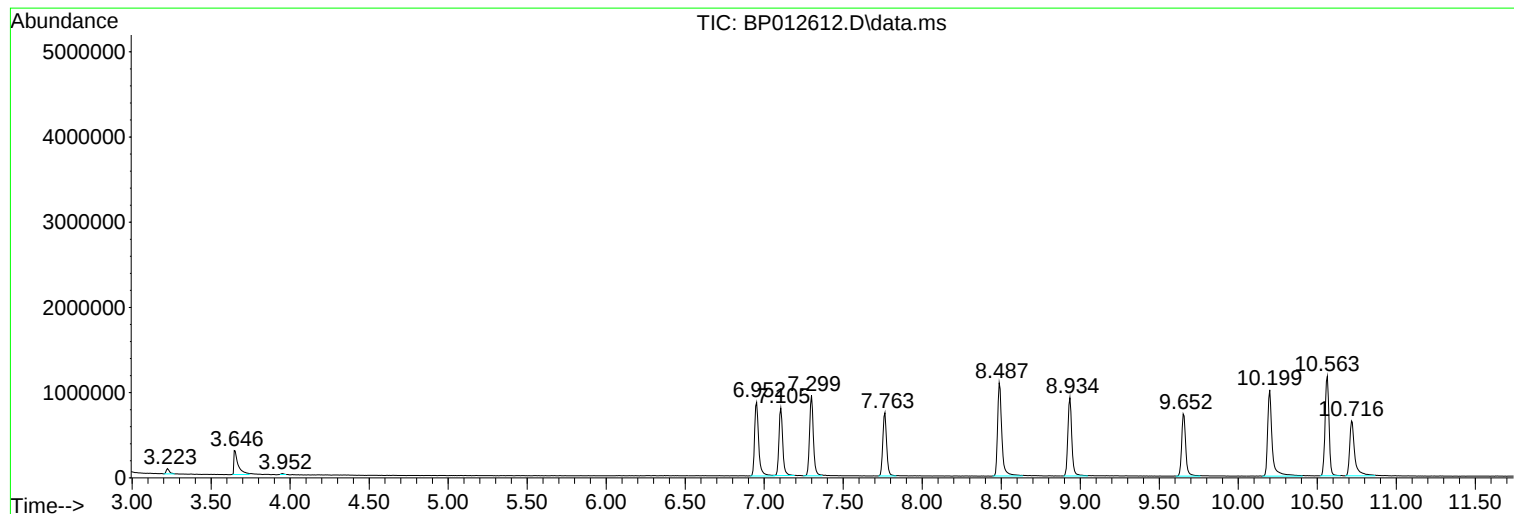

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111122\
Data File : BP012612.D
Acq On : 11 Nov 2022 11:45
Operator : CG/JU
Sample : PB148940BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111122\
Data File : BP012612.D
Acq On : 11 Nov 2022 11:45
Operator : CG/JU
Sample : PB148940BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc