
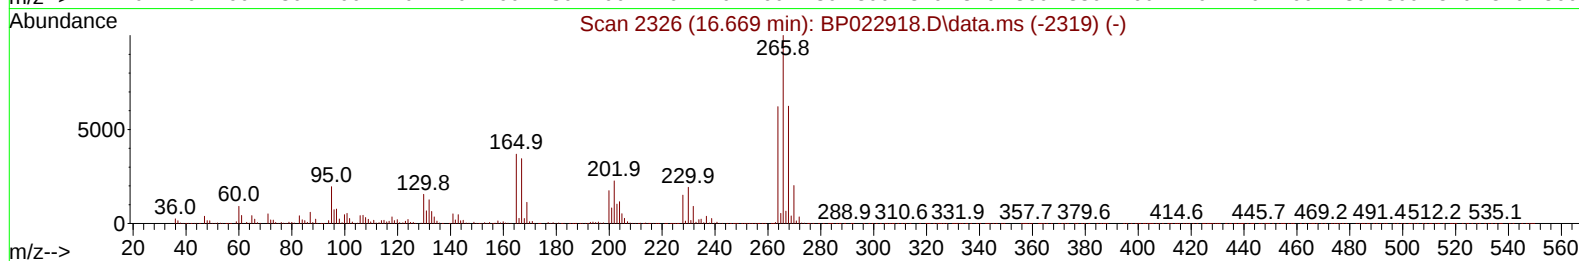
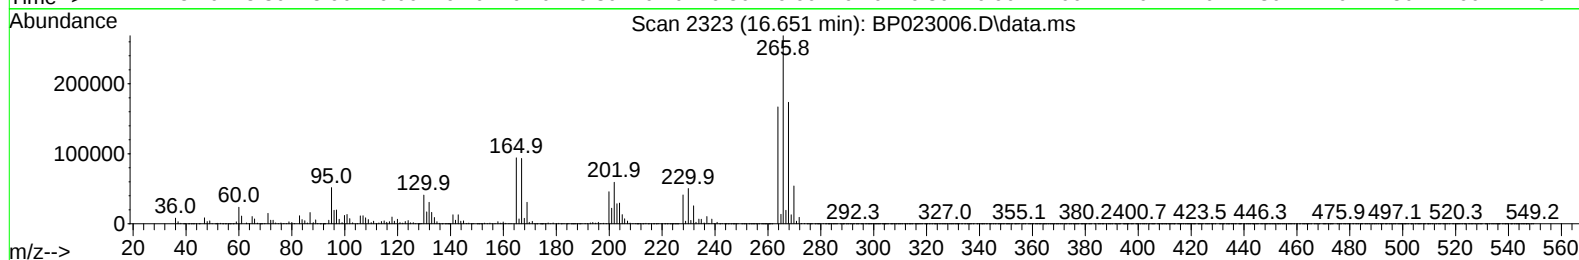


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111124\
Data File : BP023006.D
Acq On : 11 Nov 2024 09:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 11:10:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 23:36:11 2024
Response via : Initial Calibration

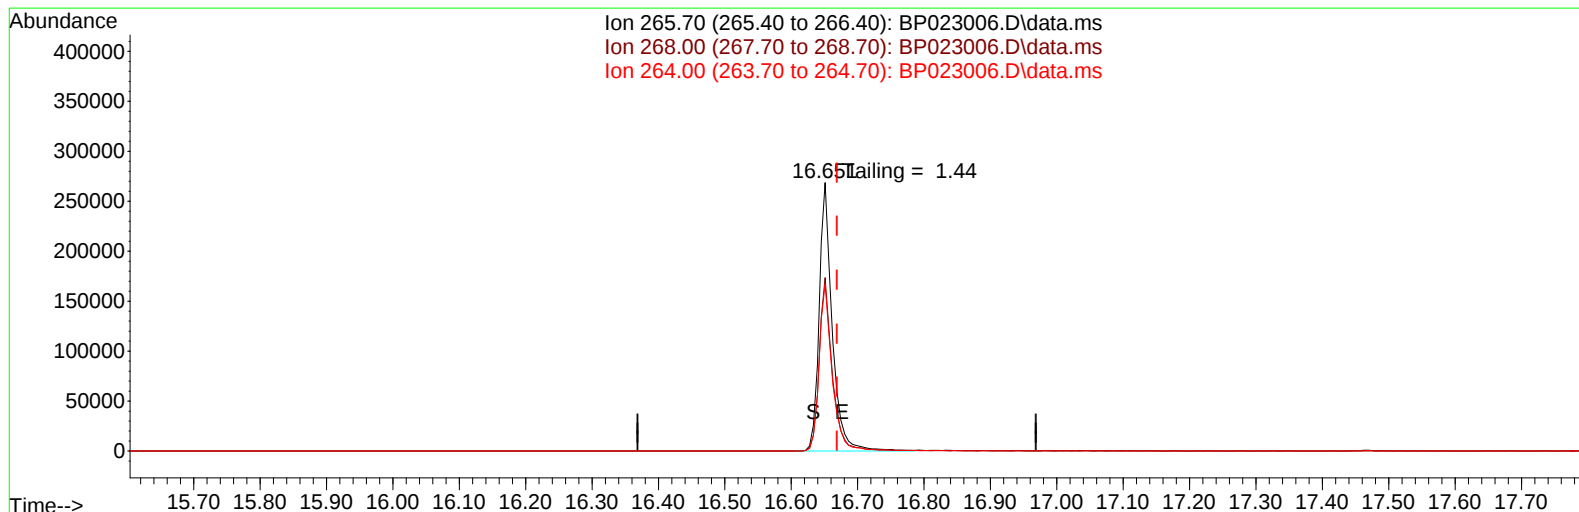

TIC: BP023006.D\data.ms

(70) Pentachlorophenol (C)




16.651min (-0.018) 169028.31 ng

response 368155

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.57
264.00	62.10	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111124\
Data File : BP023006.D
Acq On : 11 Nov 2024 09:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 11:10:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 23:36:11 2024
Response via : Initial Calibration

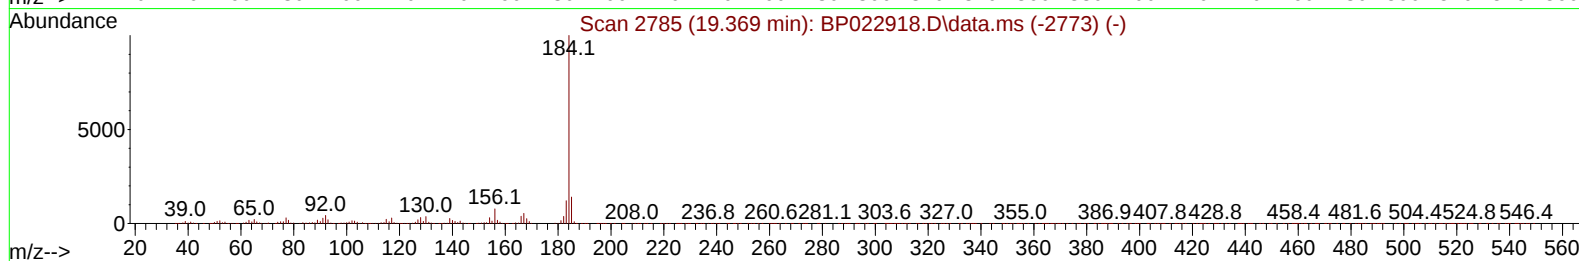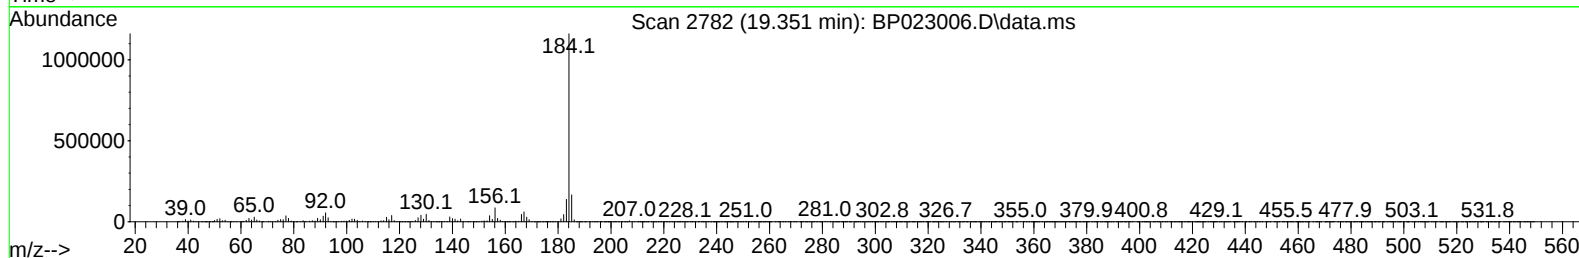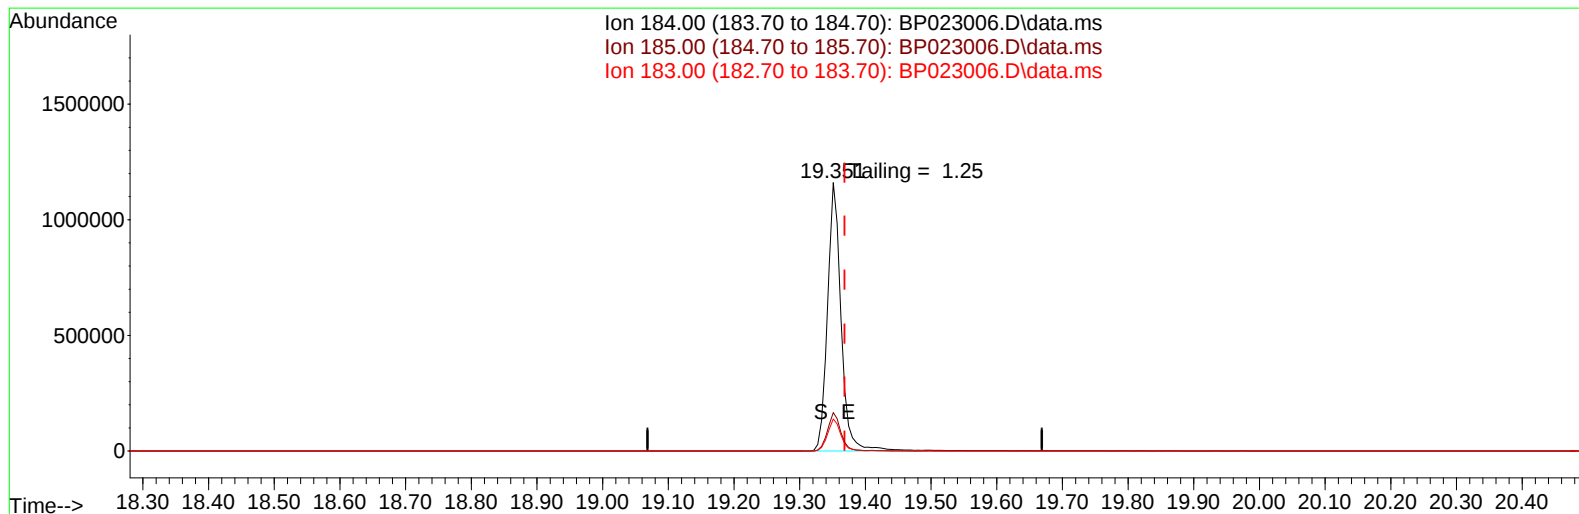

TIC: BP023006.D\data.ms

(77) Benzidine**19.351min (-0.018) 8900.91 ng****response 1665635**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.33
183.00	12.10	11.92
0.00	0.00	0.00