
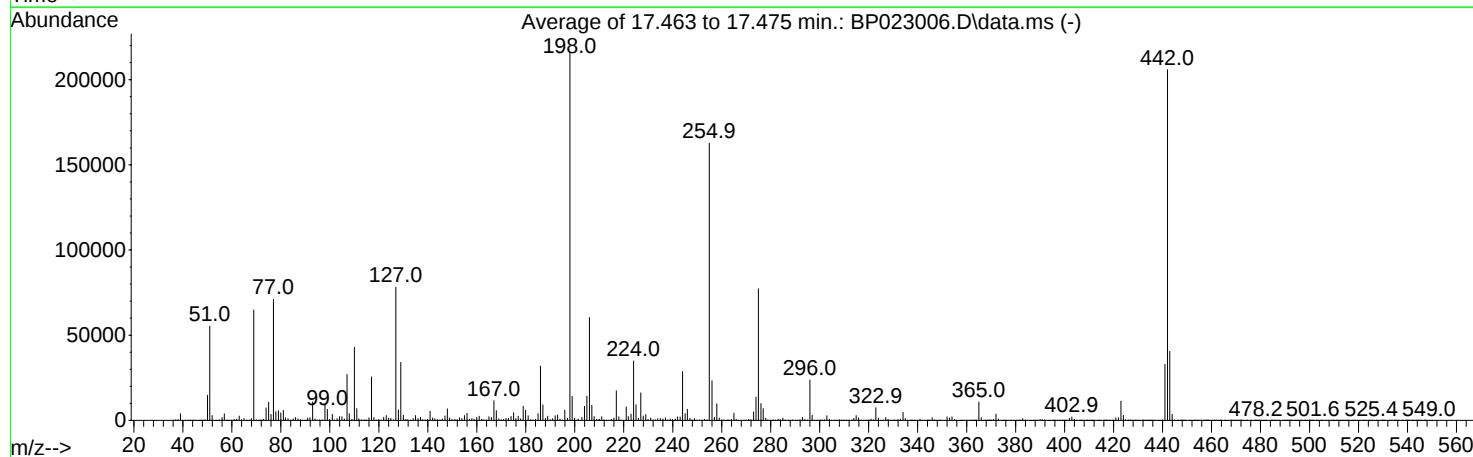


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111124\
Data File : BP023006.D
Acq On : 11 Nov 2024 09:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 07 23:36:11 2024

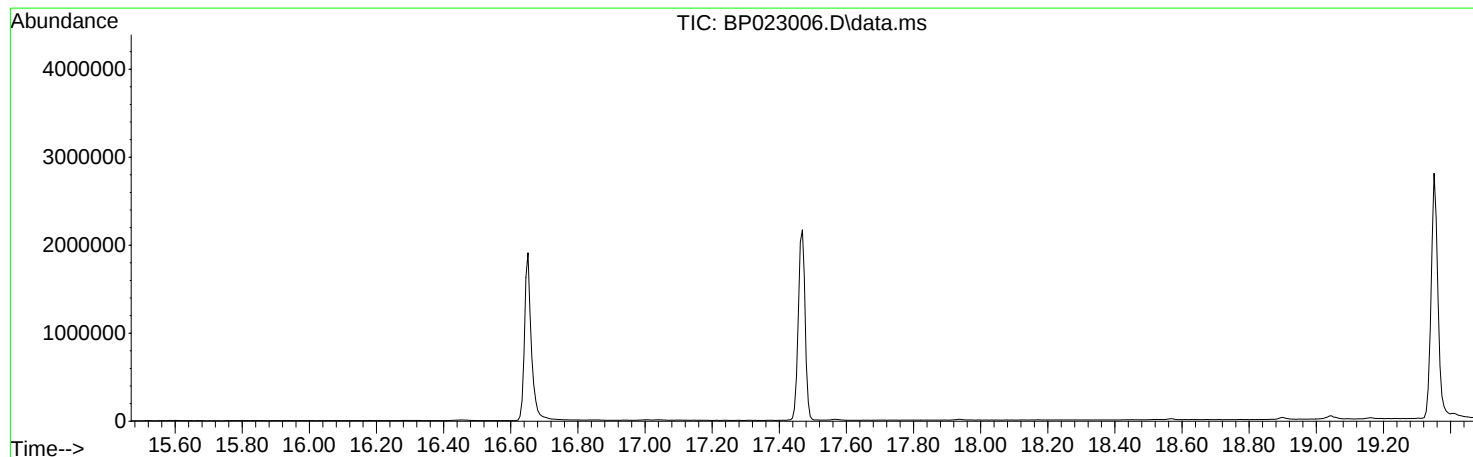




AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	55301	PASS
68	69	0.00	2	1.7	1083	PASS
69	198	0.00	100	30.0	64796	PASS
70	69	0.00	2	0.6	363	PASS
127	198	10	80	36.2	78118	PASS
197	198	0.00	2	0.5	1173	PASS
198	198	100	100	100.0	215957	PASS
199	198	5	9	6.5	14081	PASS
275	198	10	60	35.8	77265	PASS
365	198	1	100	5.0	10783	PASS
441	198	0.01	100	15.2	32844	PASS
442	442	100	100	100.0	205907	PASS
443	442	15	24	19.7	40483	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111124\
Data File : BP023006.D
Acq On : 11 Nov 2024 09:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 11 11:10:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 23:36:11 2024
Response via : Initial Calibration

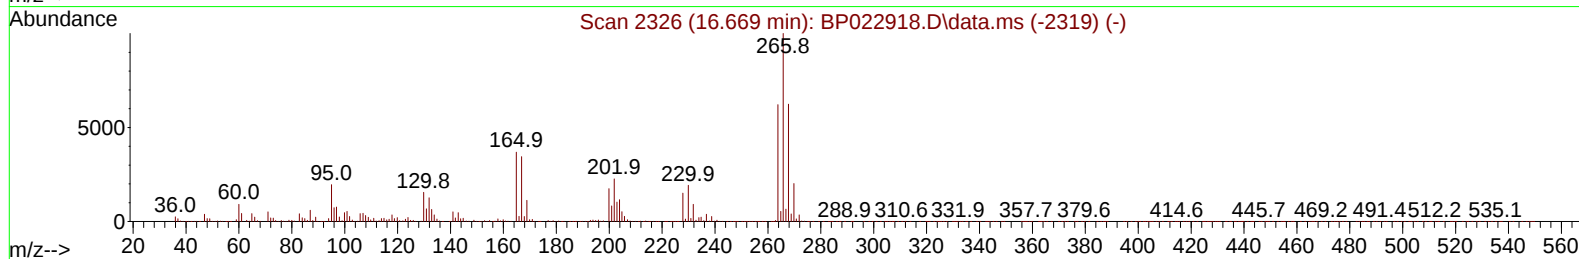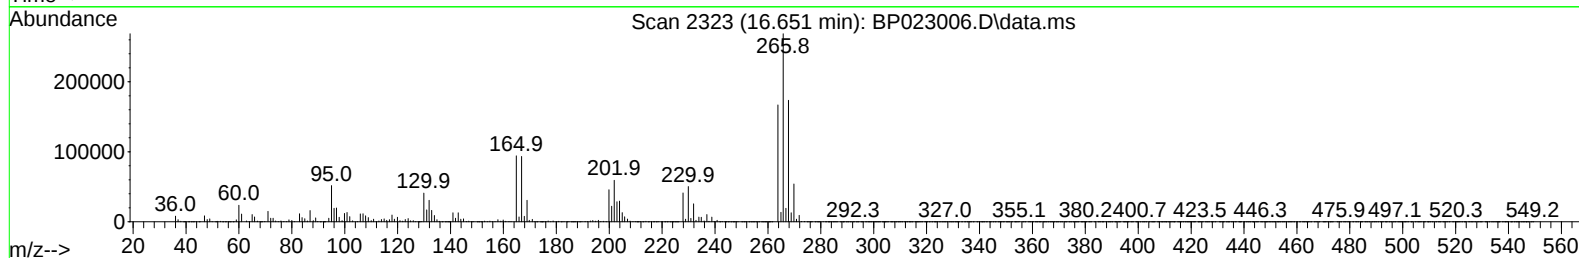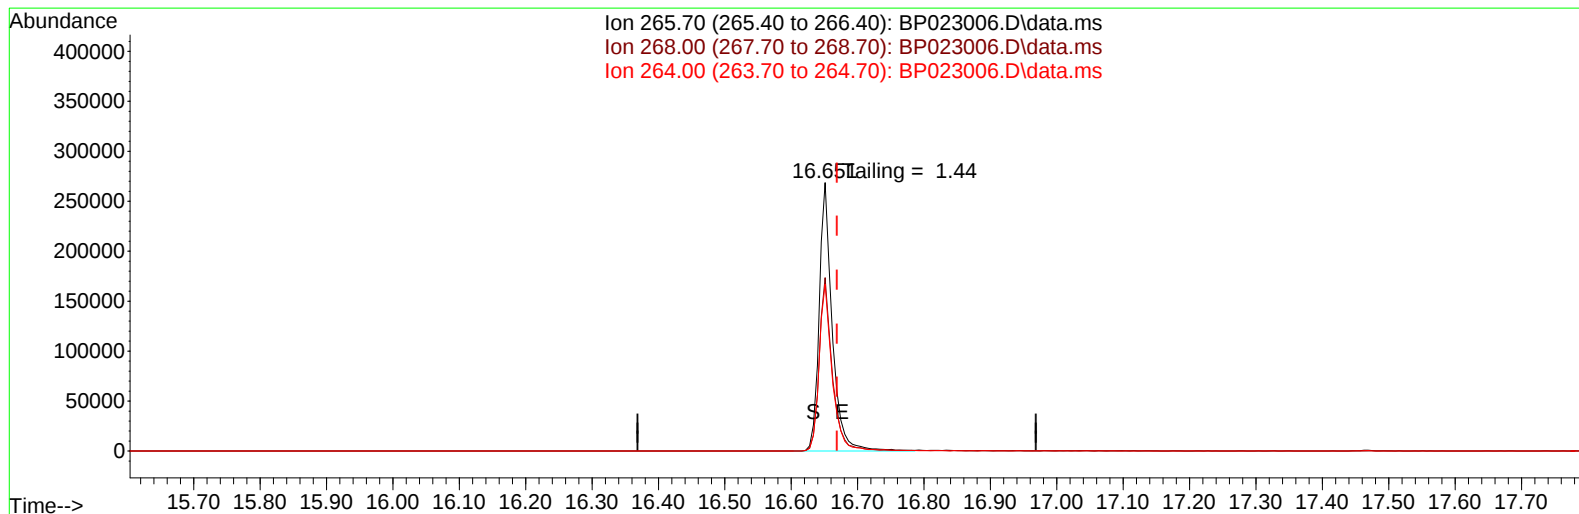

TIC: BP023006.D\data.ms

(70) Pentachlorophenol (C)

16.651min (-0.018) 169028.31 ng




response 368155

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.57
264.00	62.10	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111124\
Data File : BP023006.D
Acq On : 11 Nov 2024 09:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 11 11:10:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP110724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 23:36:11 2024
Response via : Initial Calibration

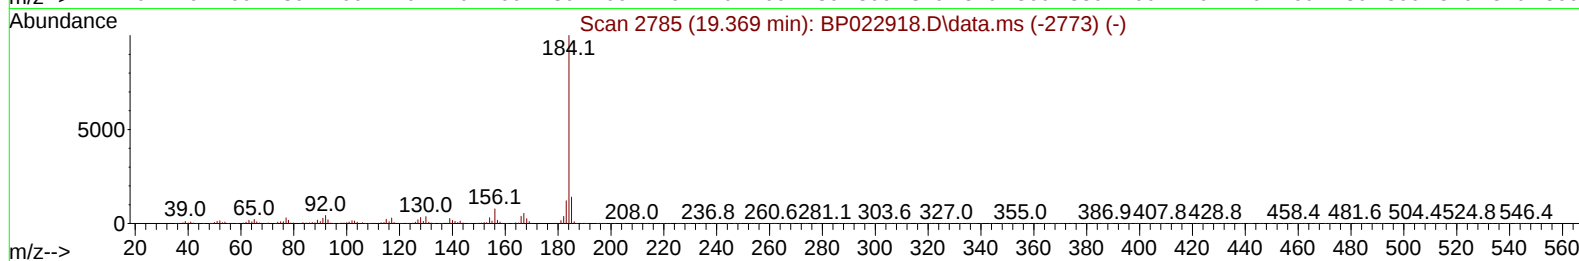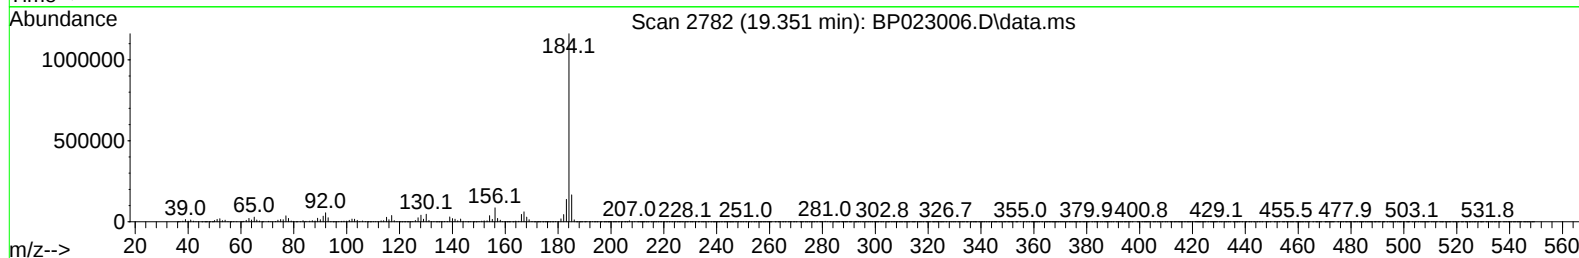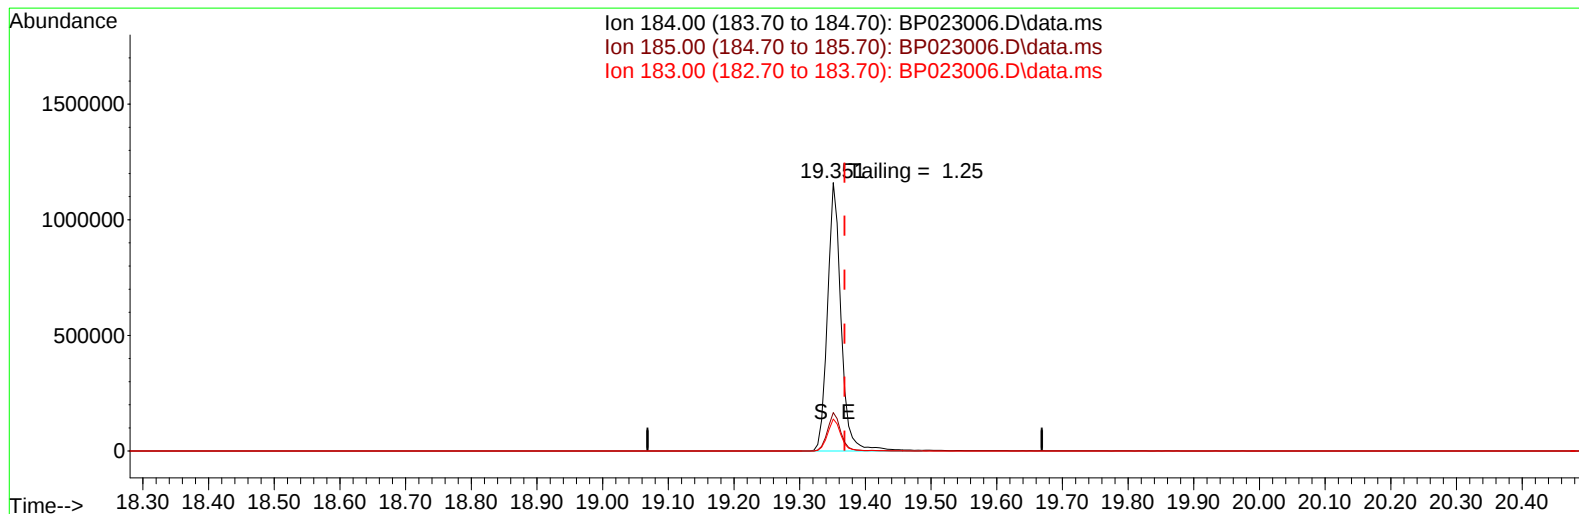

TIC: BP023006.D\data.ms

(77) Benzidine

19.351min (-0.018) 8900.91 ng

response 1665635

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.33
183.00	12.10	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2024	BNA_P	<u>BP023006.D</u>
Compound Name	Response	Retention Time
DDT	979661	20.639
DDD	21289	20.192
DDE	2543	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23832	1003493	2.37

Instrument :
BNA_P
ClientSampleId :
DFTPP