




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023017.D
Acq On : 11 Nov 2024 17:03
Operator : RC/JU
Sample : PB164672BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK672

Manual IntegrationsAPPROVED

Quant Time: Nov 12 00:55:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 11 22:00:58 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/14/2024

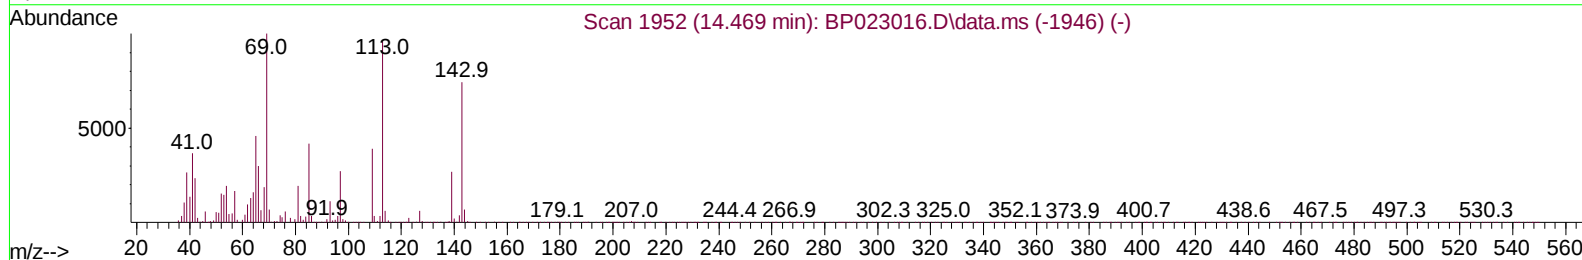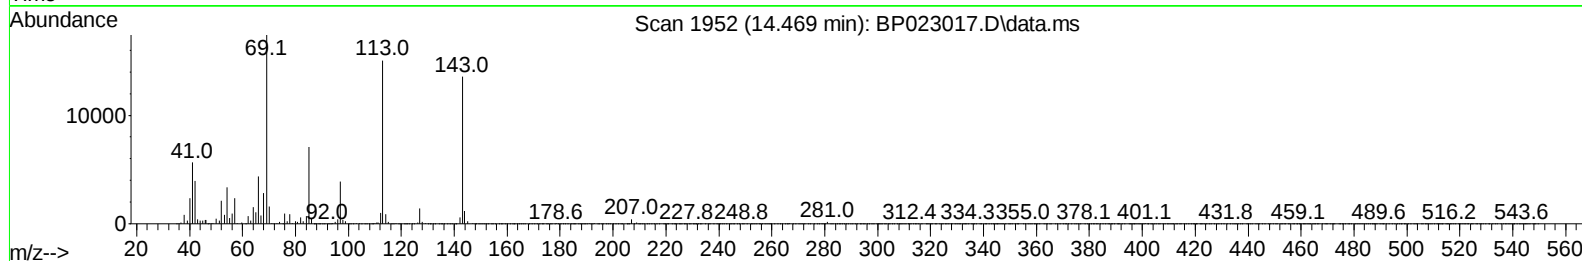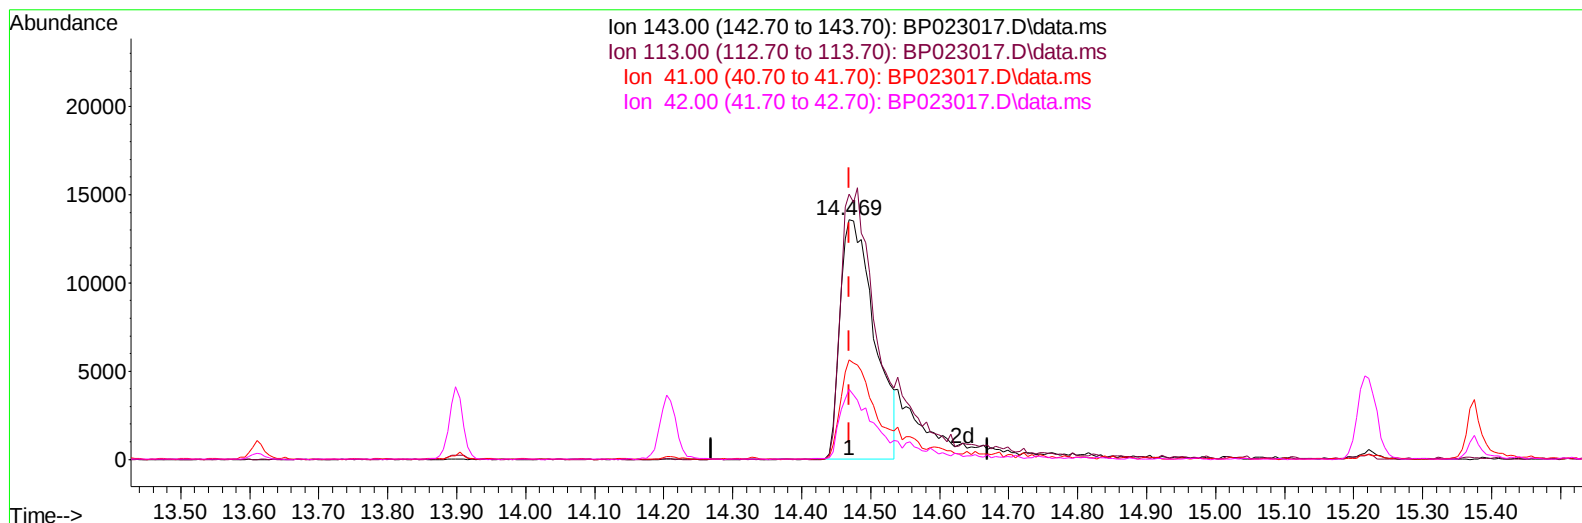

TIC: BP023017.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.469min (-0.000) 23.30 ng/u1

response 46744

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	110.92
41.00	39.20	41.62
42.00	25.90	29.29




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023017.D
Acq On : 11 Nov 2024 17:03
Operator : RC/JU
Sample : PB164672BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK672

Manual IntegrationsAPPROVED

Quant Time: Nov 12 00:55:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 11 22:00:58 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/14/2024

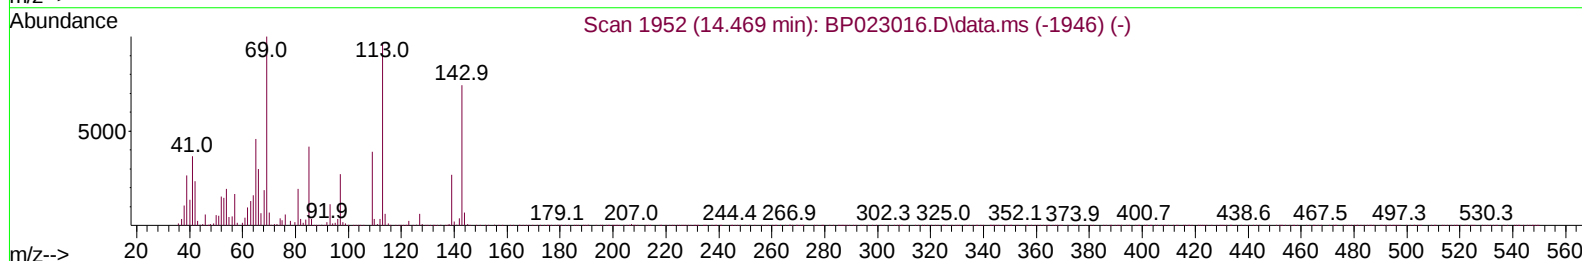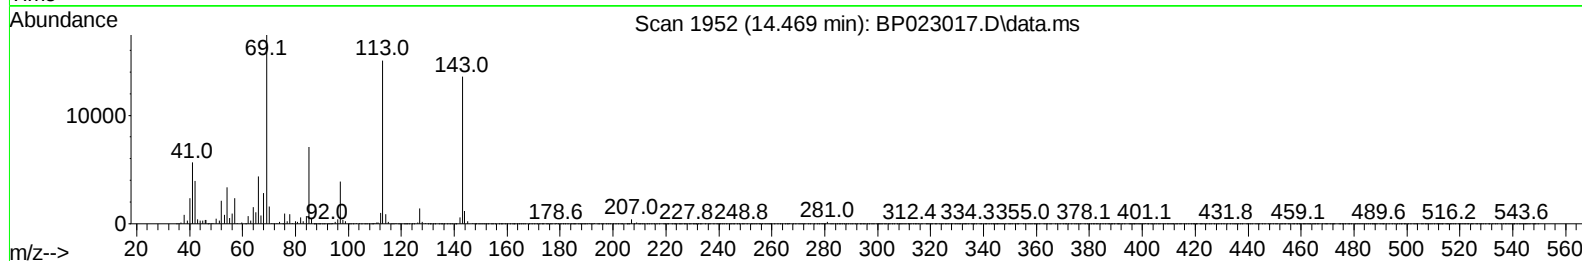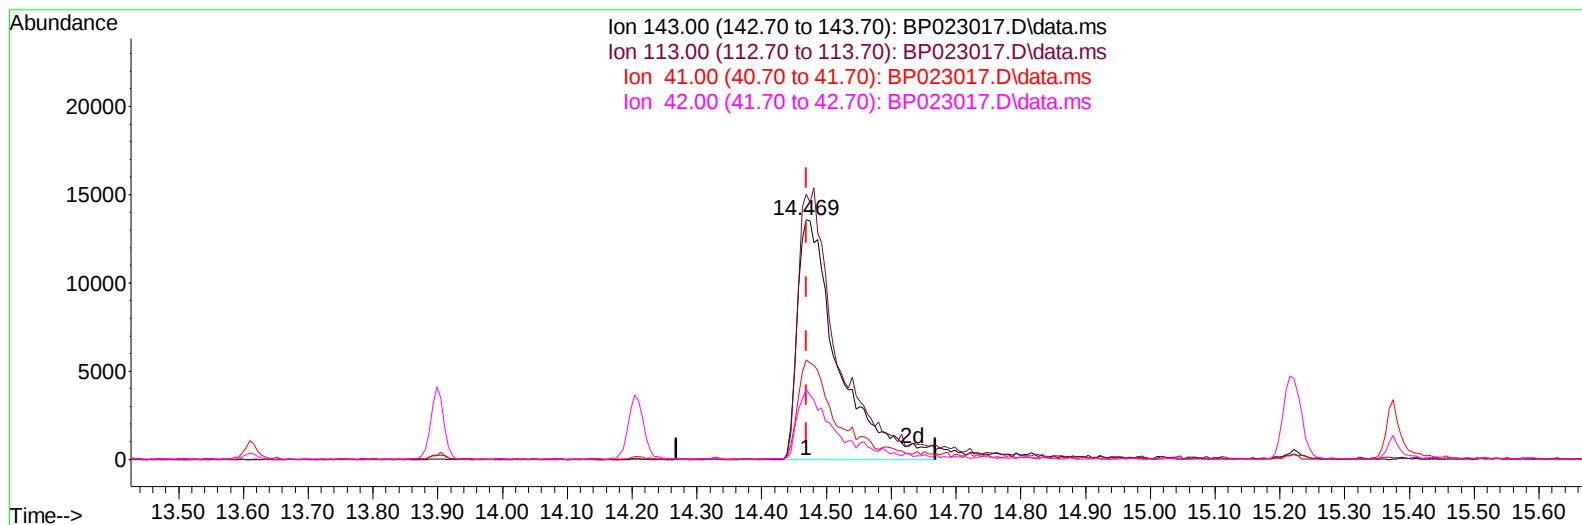

TIC: BP023017.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.469min (-0.000) 29.47 ng/ul m

response 59106

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	110.92
41.00	39.20	41.62
42.00	25.90	29.29

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023017.D
 Acq On : 11 Nov 2024 17:03
 Operator : RC/JU
 Sample : PB164672BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK672

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/13/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 12 00:58:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 11 22:00:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	59723	20.000	ng/ul	0.00
20) Naphthalene-d8	10.340	136	225561	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.204	164	185199	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.016	188	487121	20.000	ng/ul	0.00
79) Chrysene-d12	21.463	240	560442	20.000	ng/ul	0.00
88) Perylene-d12	24.704	264	623440	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	8501	6.842	ng/uL	0.00
4) Pyridine-d5	3.552	84	107433	29.103	ng/ul	0.00
7) Phenol-d5	6.793	99	131643	29.814	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.928	67	79887	30.795	ng/ul	0.00
11) 2-Chlorophenol-d4	7.140	132	100528	31.087	ng/ul	0.00
15) 4-Methylphenol-d8	8.299	113	107226	29.510	ng/ul	0.00
21) Nitrobenzene-d5	8.728	128	51083	32.531	ng/ul	0.00
24) 2-Nitrophenol-d4	9.446	143	58626	31.316	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.993	165	112976	28.817	ng/ul	0.01
31) 4-Chloroaniline-d4	10.493	131	130516	27.905	ng/ul	0.00
46) Dimethylphthalate-d6	13.610	166	463189	34.701	ng/ul	0.00
49) Acenaphthylene-d8	13.898	160	458809	32.943	ng/ul	0.00
54) 4-Nitrophenol-d4	14.469	143	59106m	29.466	ng/ul	0.00
60) Fluorene-d10	15.222	176	392242	33.517	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.375	200	79412	27.214	ng/ul	0.00
73) Anthracene-d10	17.128	188	702120	34.042	ng/ul	0.02
81) Pyrene-d10	19.504	212	894841	34.664	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.463	264	1007603	33.930	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023017.D
Acq On : 11 Nov 2024 17:03
Operator : RC/JU
Sample : PB164672BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK672

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 12 00:58:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 11 22:00:58 2024
Response via : Initial Calibration

