




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023047.D
Acq On : 12 Nov 2024 15:14
Operator : RC/JU
Sample : P4741-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27L6

Manual IntegrationsAPPROVED

Quant Time: Nov 12 23:59:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 11 22:00:58 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

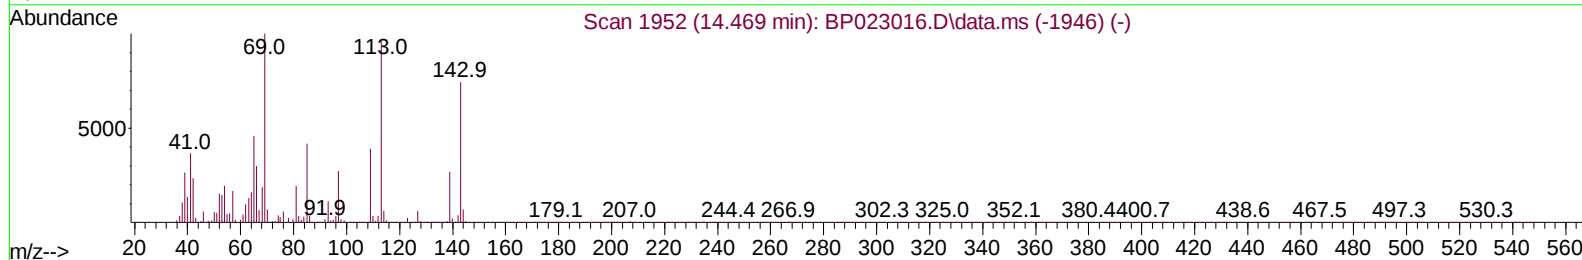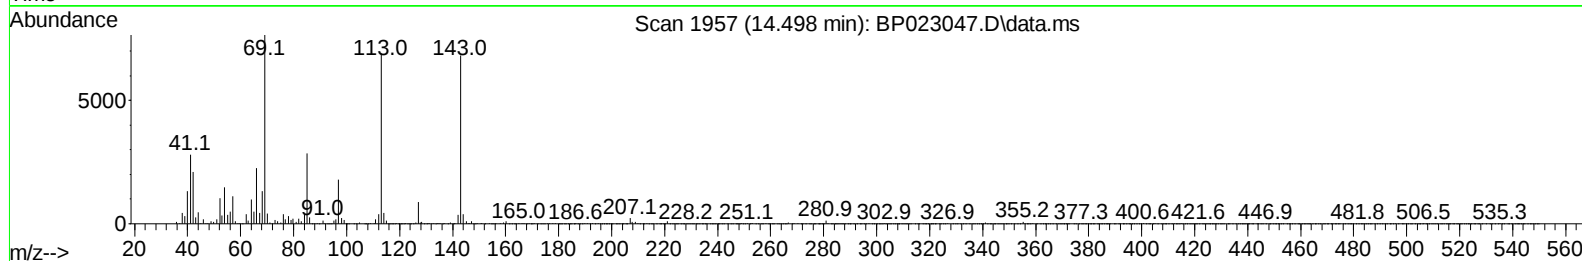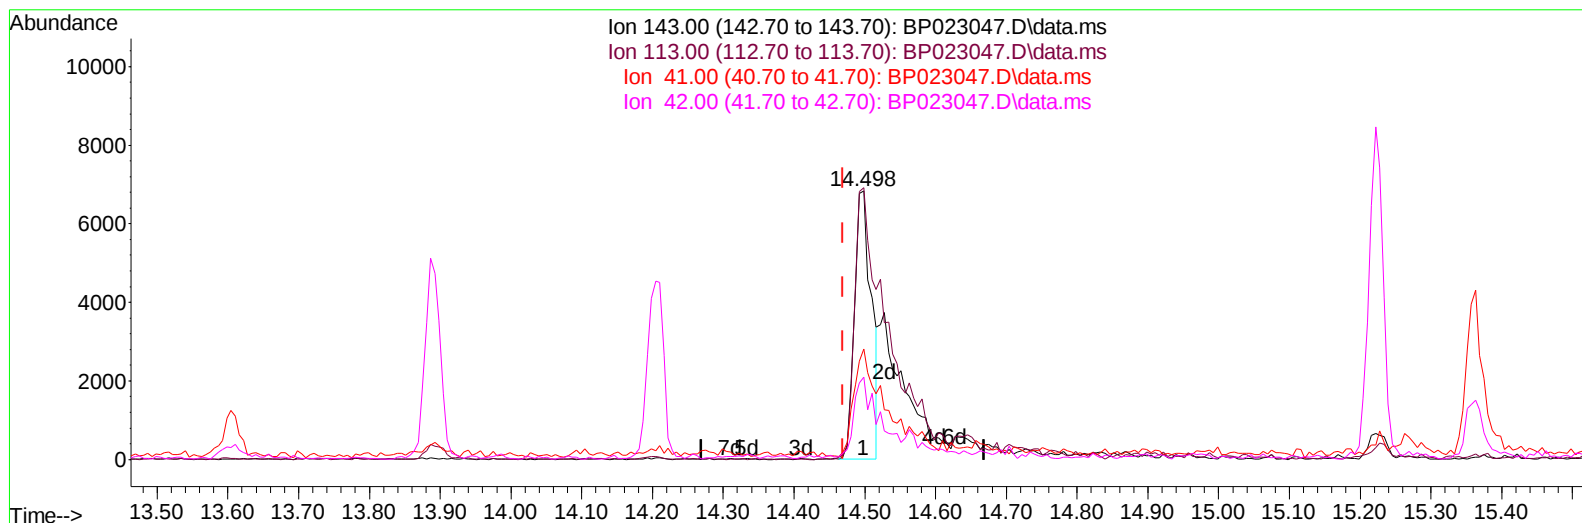

TIC: BP023047.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.498min (+ 0.029) 4.89 ng/u1

response 11418

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	101.14
41.00	39.20	41.13
42.00	25.90	30.67




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023047.D
Acq On : 12 Nov 2024 15:14
Operator : RC/JU
Sample : P4741-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27L6

Manual IntegrationsAPPROVED

Quant Time: Nov 12 23:59:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 11 22:00:58 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

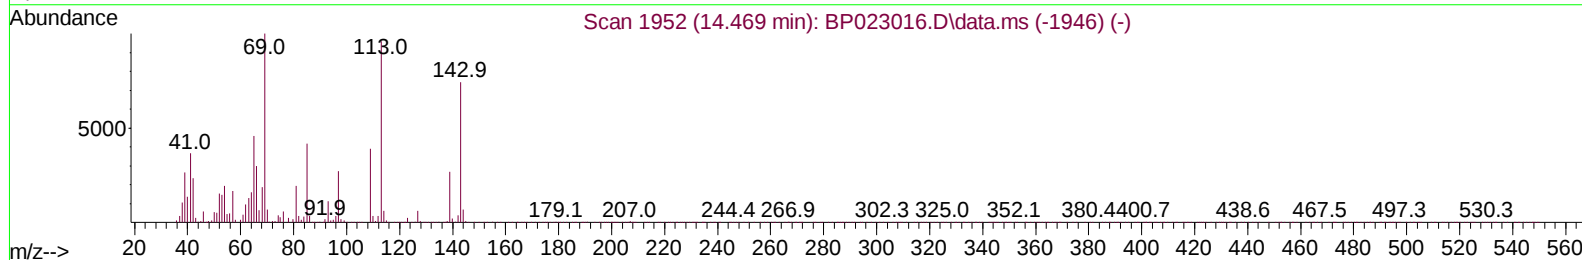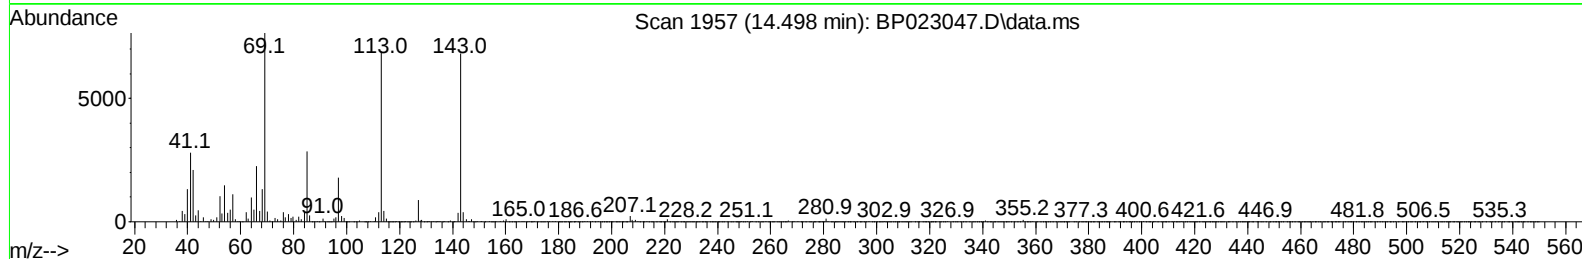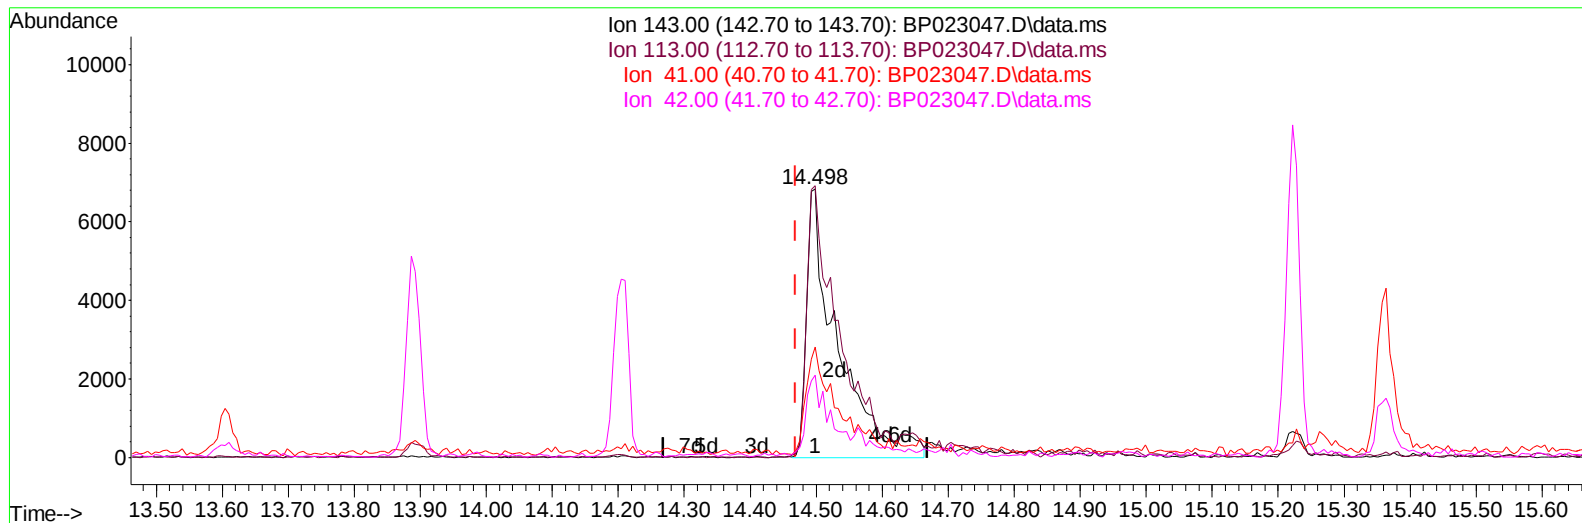

TIC: BP023047.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.498min (+ 0.029) 9.52 ng/ul m

response 22234

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	101.14
41.00	39.20	41.13
42.00	25.90	30.67

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023047.D
 Acq On : 12 Nov 2024 15:14
 Operator : RC/JU
 Sample : P4741-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E27L6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 13 01:51:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 11 22:00:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	67501	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.334	136	266720	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.210	164	215684	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.016	188	536178	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	635034	20.000	ng/ul	-0.02
88) Perylene-d12	24.645	264	762266	20.000	ng/ul	-0.06
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	7196	5.124	ng/uL	0.00
4) Pyridine-d5	3.558	84	51139	12.257	ng/ul	0.00
7) Phenol-d5	6.793	99	76860	15.401	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.928	67	103093	35.161	ng/ul	0.00
11) 2-Chlorophenol-d4	7.128	132	122545	33.529	ng/ul	0.00
15) 4-Methylphenol-d8	8.293	113	115814	28.201	ng/ul	0.00
21) Nitrobenzene-d5	8.722	128	64451	34.710	ng/ul	0.00
24) 2-Nitrophenol-d4	9.440	143	80083	36.176	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.981	165	162440	35.040	ng/ul	0.00
31) 4-Chloroaniline-d4	10.481	131	137622	24.884	ng/ul	0.00
46) Dimethylphthalate-d6	13.604	166	593090	38.153	ng/ul	0.00
49) Acenaphthylene-d8	13.887	160	579241	35.711	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.498	143	22234m	9.517	ng/ul	0.03
60) Fluorene-d10	15.222	176	509968	37.418	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	107640	33.512	ng/ul	0.00
73) Anthracene-d10	17.104	188	913312	40.230	ng/ul	0.00
81) Pyrene-d10	19.492	212	1164546	39.813	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.433	264	1485272	40.906	ng/ul	-0.04

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023047.D
Acq On : 12 Nov 2024 15:14
Operator : RC/JU
Sample : P4741-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27L6

Manual IntegrationsAPPROVED

Quant Time: Nov 13 01:51:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 11 22:00:58 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

