




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023053.D
Acq On : 12 Nov 2024 19:17
Operator : RC/JU
Sample : P4741-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27L3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 13 00:04:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 23:59:19 2024
Response via : Initial Calibration

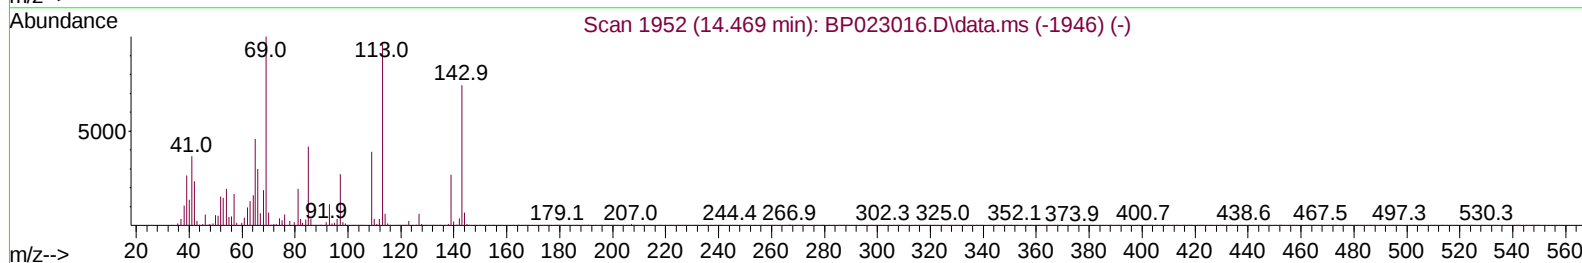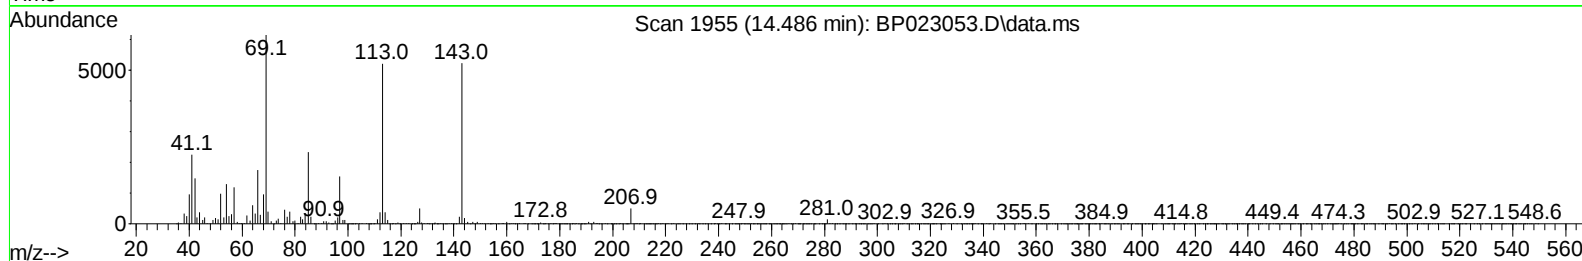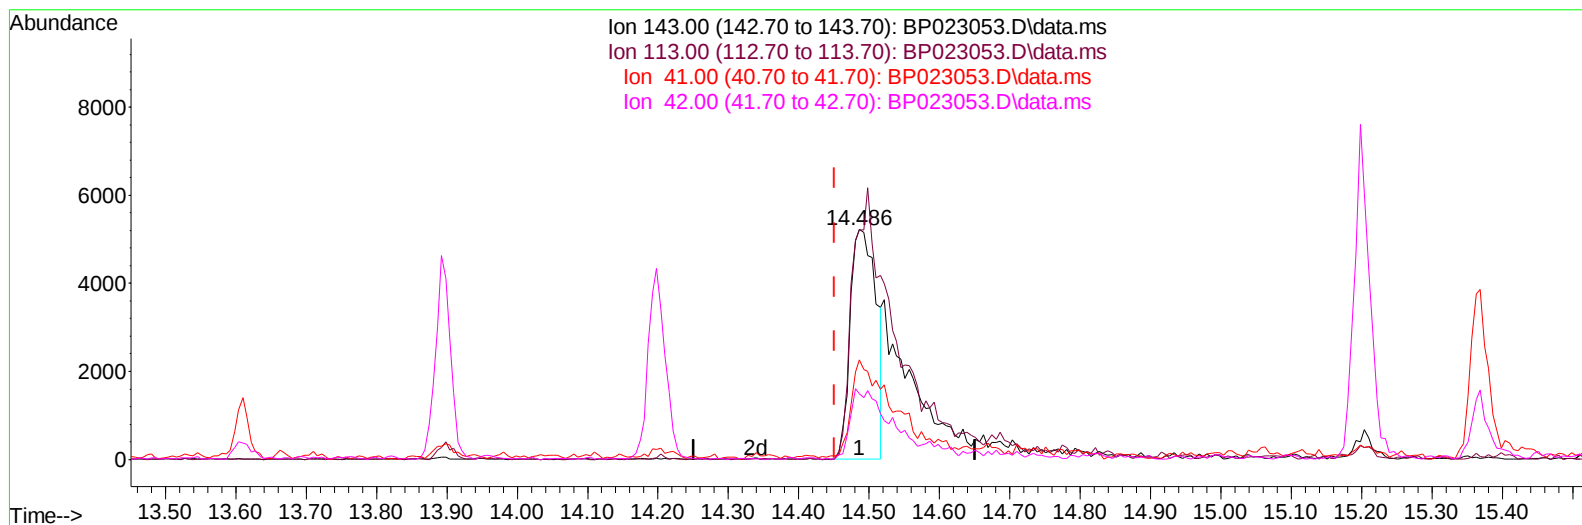

TIC: BP023053.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.486min (+ 0.035) 5.56 ng/u1

response 13274

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	99.85
41.00	39.20	43.23
42.00	25.90	28.43




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023053.D
Acq On : 12 Nov 2024 19:17
Operator : RC/JU
Sample : P4741-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27L3

Manual IntegrationsAPPROVED

Quant Time: Nov 13 00:04:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 23:59:19 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

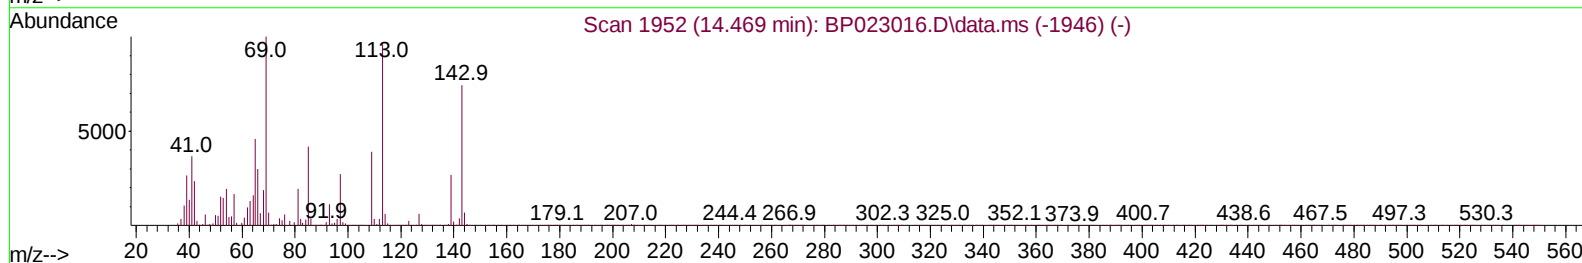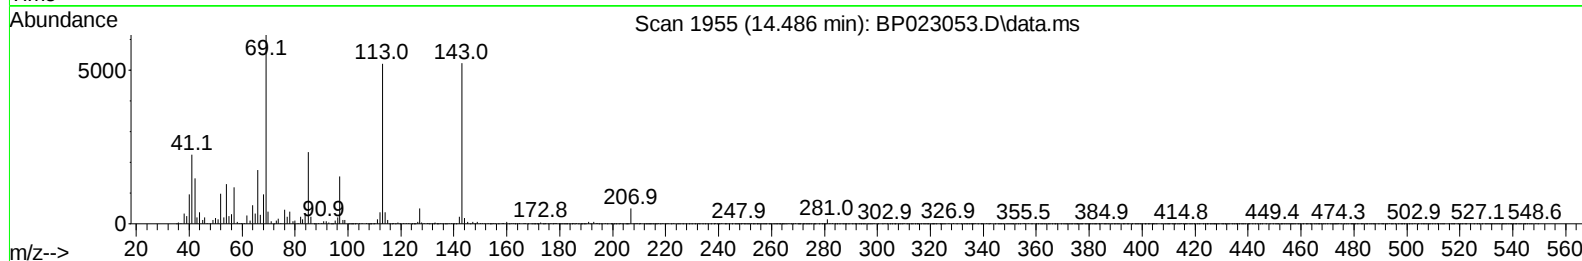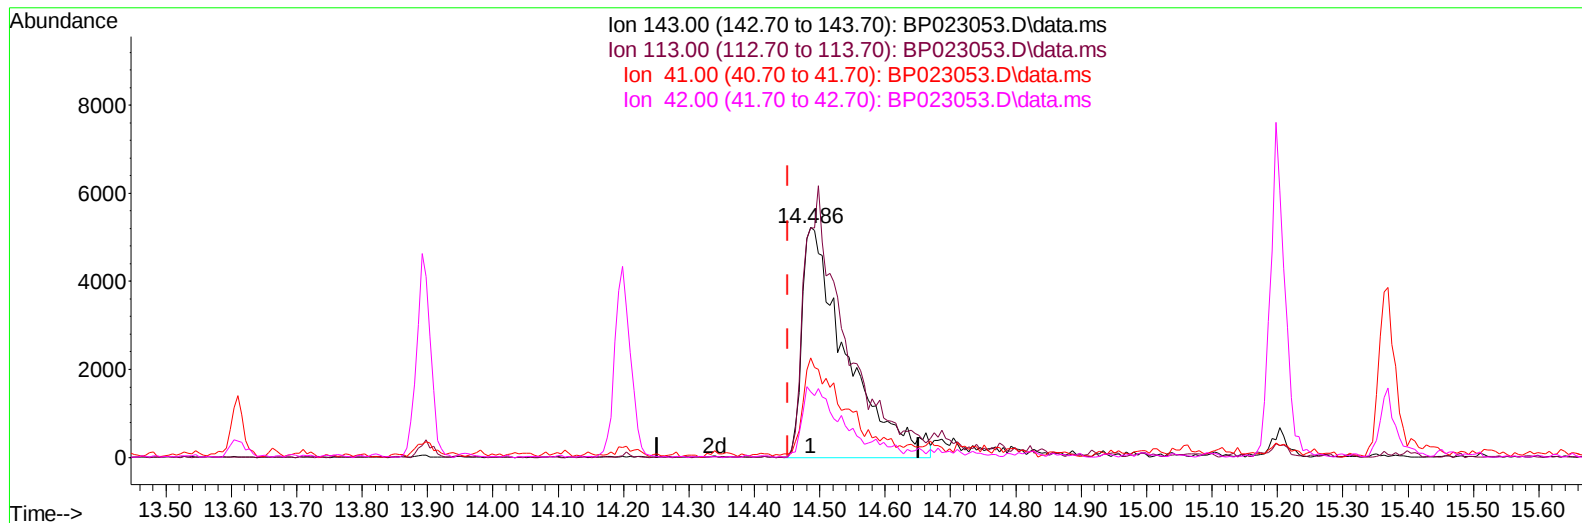

TIC: BP023053.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.486min (+ 0.035) 10.33 ng/ul m

response 24653

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	99.85
41.00	39.20	43.23
42.00	25.90	28.43

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023053.D
 Acq On : 12 Nov 2024 19:17
 Operator : RC/JU
 Sample : P4741-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E27L3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 13 02:12:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 12 23:59:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	71565	20.000	ng/ul	0.00
20) Naphthalene-d8	10.334	136	276712	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.198	164	220326	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.998	188	563279	20.000	ng/ul	-0.01
79) Chrysene-d12	21.445	240	679638	20.000	ng/ul	0.00
88) Perylene-d12	24.668	264	846566	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	7598	5.103	ng/uL	0.00
4) Pyridine-d5	3.563	84	26441	5.977	ng/ul	0.01
7) Phenol-d5	6.793	99	61082	11.545	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.934	67	96960	31.191	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132	113954	29.407	ng/ul	0.00
15) 4-Methylphenol-d8	8.298	113	106069	24.361	ng/ul	0.00
21) Nitrobenzene-d5	8.734	128	61757	32.058	ng/ul	0.00
24) 2-Nitrophenol-d4	9.440	143	74910	32.618	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.981	165	148165	30.807	ng/ul	0.00
31) 4-Chloroaniline-d4	10.487	131	102584	17.879	ng/ul	0.00
46) Dimethylphthalate-d6	13.610	166	560279	35.283	ng/ul	0.00
49) Acenaphthylene-d8	13.892	160	531488	32.077	ng/ul	0.00
54) 4-Nitrophenol-d4	14.486	143	24653m	10.331	ng/ul	0.03
60) Fluorene-d10	15.204	176	487133	34.989	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	101556	30.097	ng/ul	-0.01
73) Anthracene-d10	17.110	188	863700	36.214	ng/ul	-0.01
81) Pyrene-d10	19.492	212	1139030	36.385	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.439	264	1468699	36.421	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023053.D
Acq On : 12 Nov 2024 19:17
Operator : RC/JU
Sample : P4741-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27L3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 13 02:12:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 23:59:19 2024
Response via : Initial Calibration

