




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023055.D
Acq On : 12 Nov 2024 20:38
Operator : RC/JU
Sample : P4687-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CP2

Manual IntegrationsAPPROVED

Quant Time: Nov 13 02:17:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 23:59:19 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

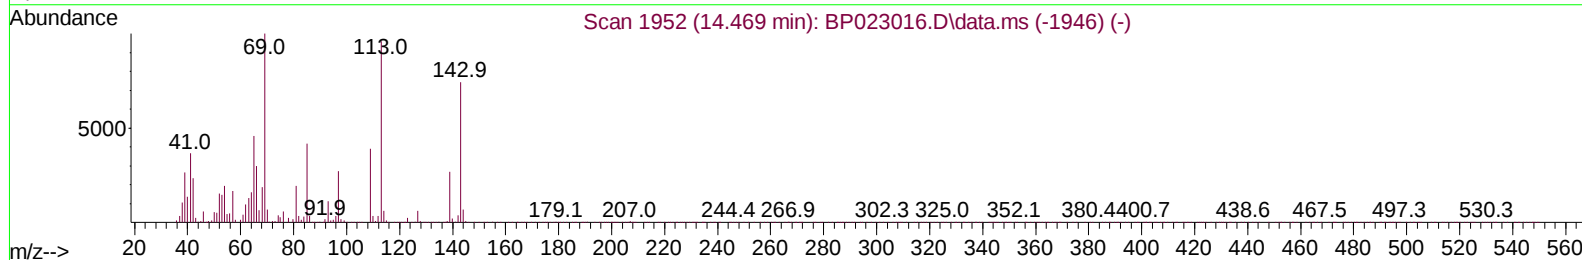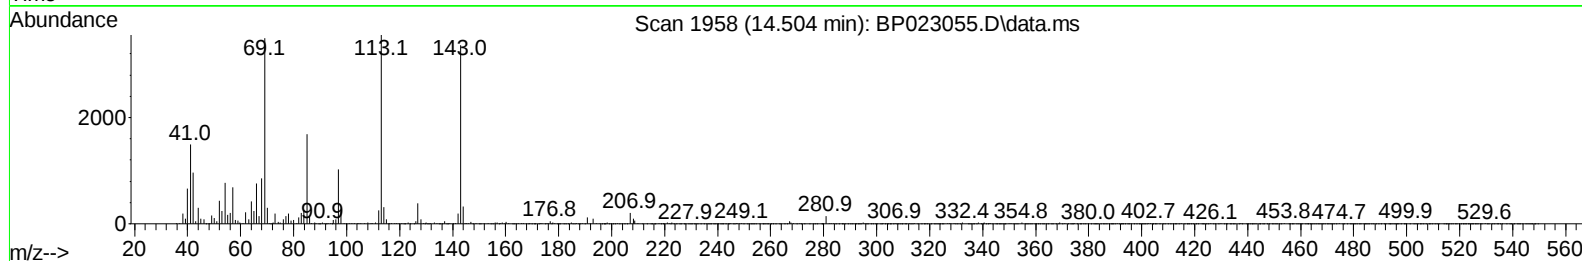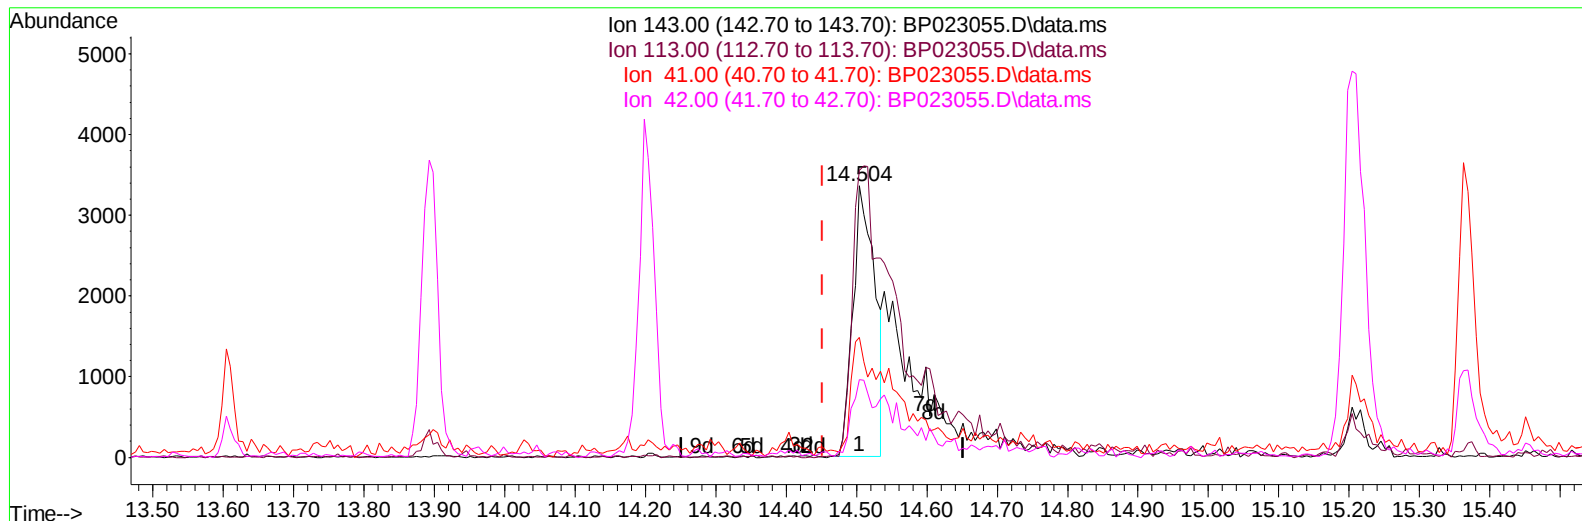

TIC: BP023055.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.504min (+ 0.053) 3.45 ng/u1

response 7152

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	105.68
41.00	39.20	44.34
42.00	25.90	28.64




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023055.D
Acq On : 12 Nov 2024 20:38
Operator : RC/JU
Sample : P4687-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CP2

Manual IntegrationsAPPROVED

Quant Time: Nov 13 02:17:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 23:59:19 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

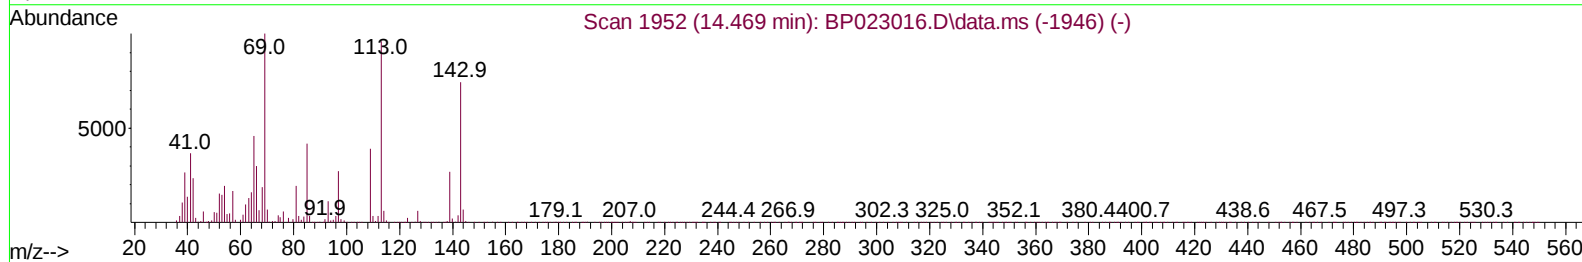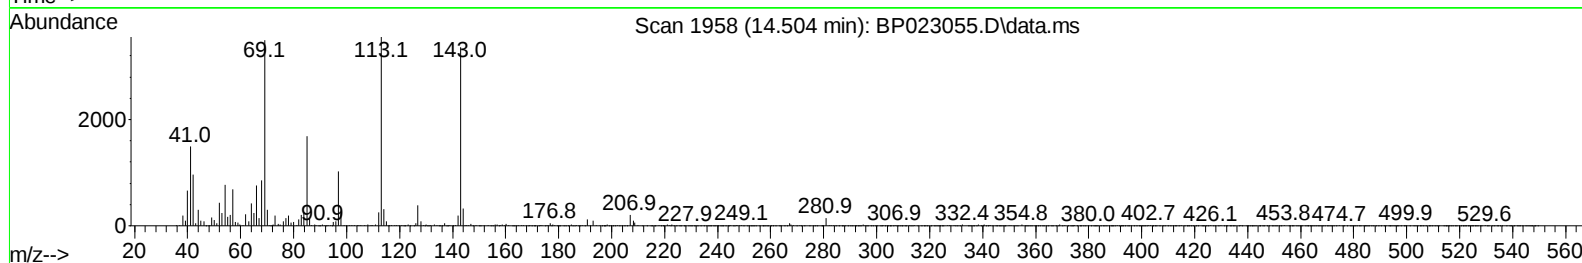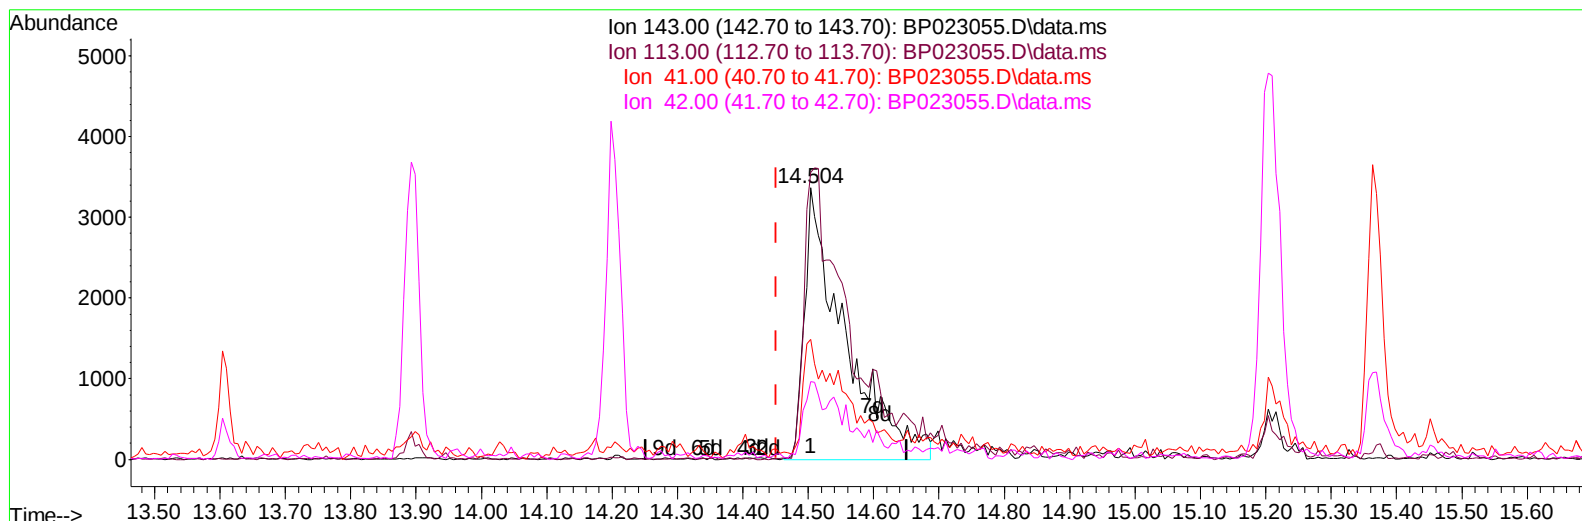

TIC: BP023055.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.504min (+ 0.053) 6.90 ng/ul m

response 14323

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	105.68
41.00	39.20	44.34
42.00	25.90	28.64

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023055.D
 Acq On : 12 Nov 2024 20:38
 Operator : RC/JU
 Sample : P4687-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CP2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 13 02:18:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 12 23:59:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	61363	20.000	ng/ul	0.00
20) Naphthalene-d8	10.340	136	243689	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.204	164	191611	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.998	188	493657	20.000	ng/ul	-0.01
79) Chrysene-d12	21.439	240	585390	20.000	ng/ul	-0.01
88) Perylene-d12	24.662	264	710760	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	5765	4.516	ng/uL	0.00
4) Pyridine-d5	3.564	84	26428	6.968	ng/ul	0.01
7) Phenol-d5	6.799	99	33732	7.435	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.934	67	77927	29.236	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132	88819	26.732	ng/ul	0.00
15) 4-Methylphenol-d8	8.299	113	69894	18.722	ng/ul	0.00
21) Nitrobenzene-d5	8.728	128	48616	28.657	ng/ul	0.00
24) 2-Nitrophenol-d4	9.440	143	58477	28.913	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.981	165	124759	29.455	ng/ul	0.00
31) 4-Chloroaniline-d4	10.487	131	120653	23.877	ng/ul	0.00
46) Dimethylphthalate-d6	13.610	166	437317	31.667	ng/ul	0.00
49) Acenaphthylene-d8	13.892	160	428589	29.743	ng/ul	0.00
54) 4-Nitrophenol-d4	14.504	143	14323m	6.901	ng/ul	0.05
60) Fluorene-d10	15.204	176	374824	30.957	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.369	200	89117	30.135	ng/ul	0.00
73) Anthracene-d10	17.110	188	784133	37.515	ng/ul	-0.01
81) Pyrene-d10	19.486	212	1014815	37.637	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.439	264	1307652	38.624	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023055.D
Acq On : 12 Nov 2024 20:38
Operator : RC/JU
Sample : P4687-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CP2

Manual IntegrationsAPPROVED

Quant Time: Nov 13 02:18:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 23:59:19 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

