




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023065.D
Acq On : 13 Nov 2024 04:03
Operator : RC/JU
Sample : PB164834BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK834

Manual IntegrationsAPPROVED

Quant Time: Nov 13 04:51:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

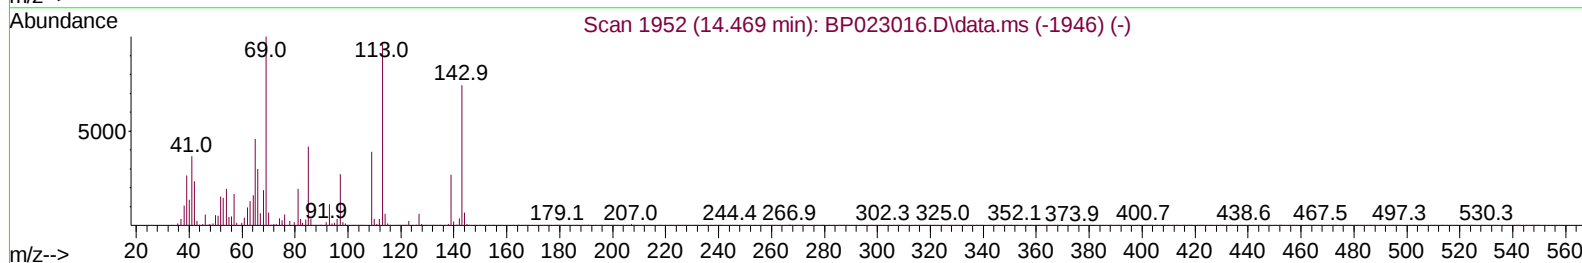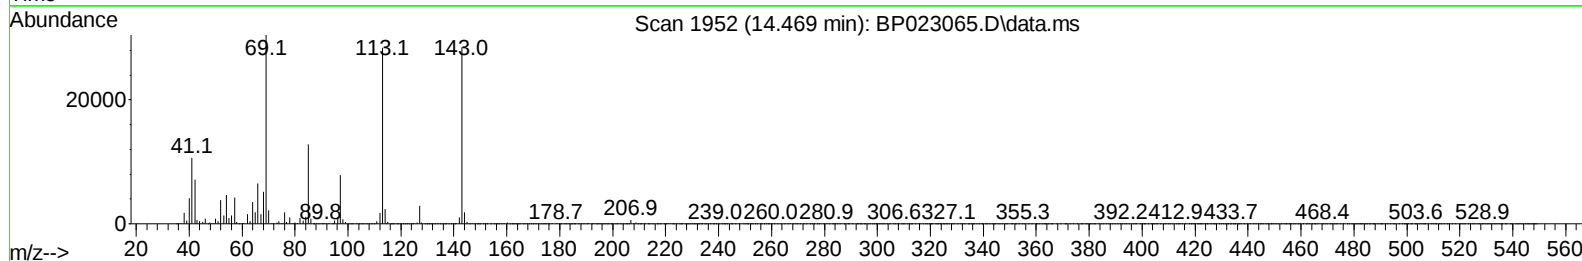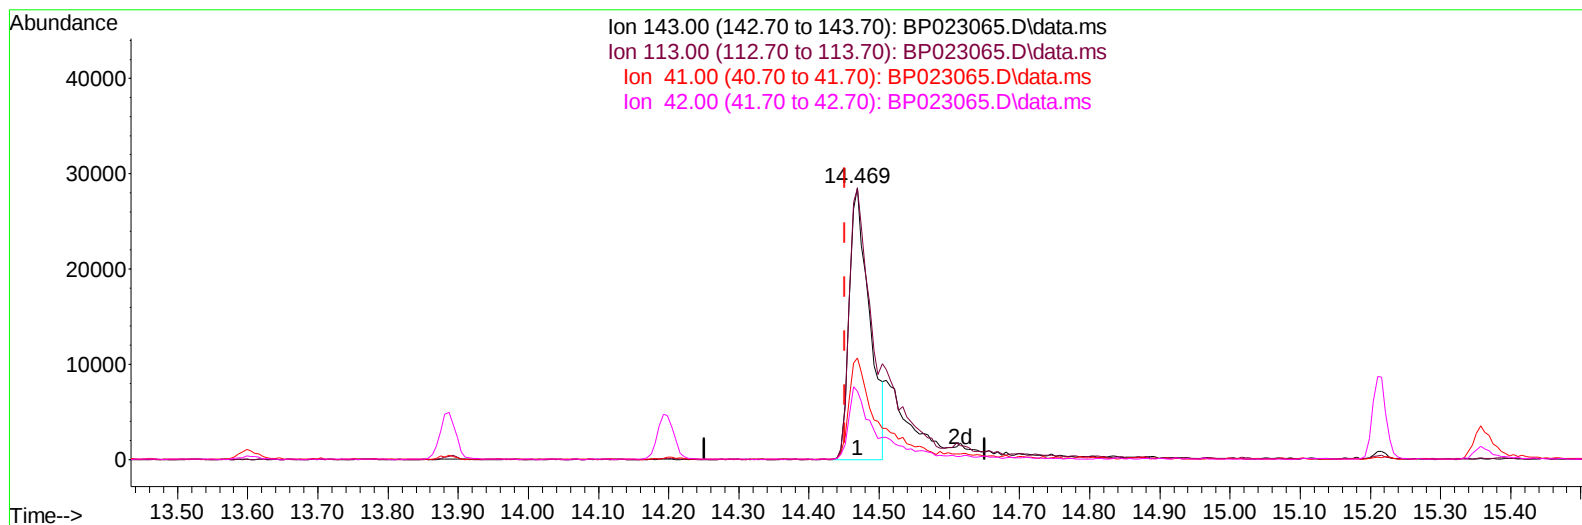

TIC: BP023065.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.469min (+ 0.018) 19.76 ng/u1

response 57164

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	99.75
41.00	39.20	37.33
42.00	25.90	25.15




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023065.D
Acq On : 13 Nov 2024 04:03
Operator : RC/JU
Sample : PB164834BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK834

Manual IntegrationsAPPROVED

Quant Time: Nov 13 04:51:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

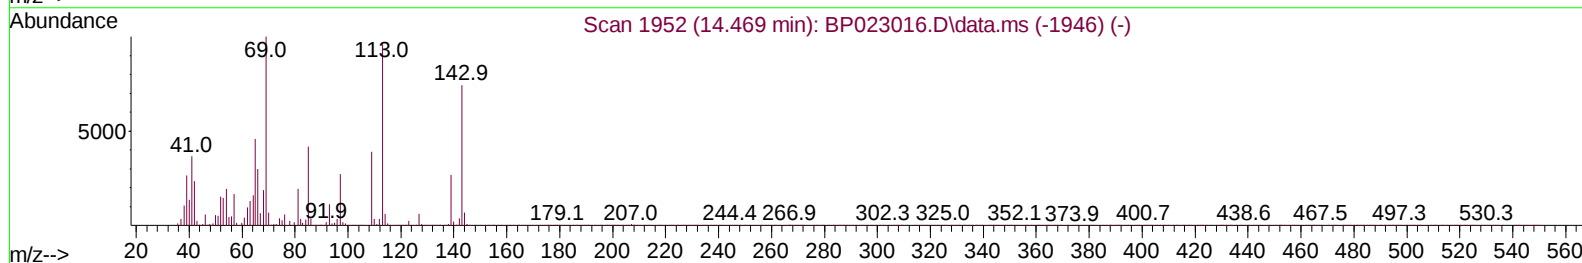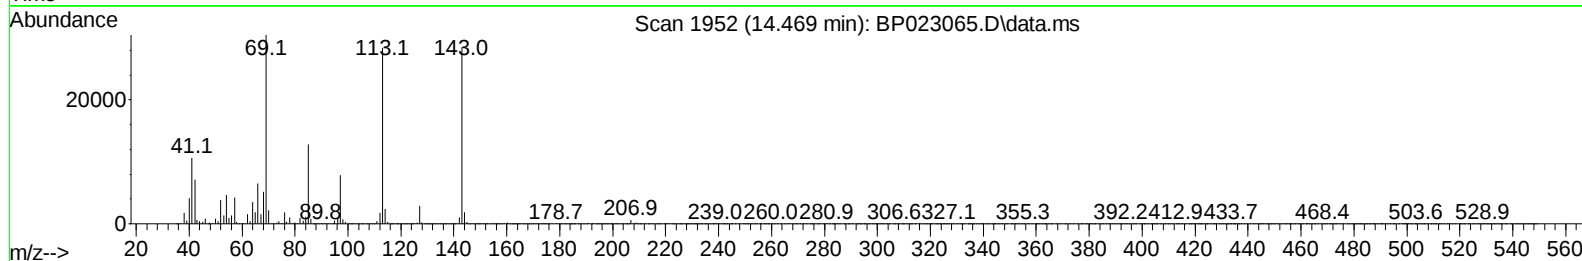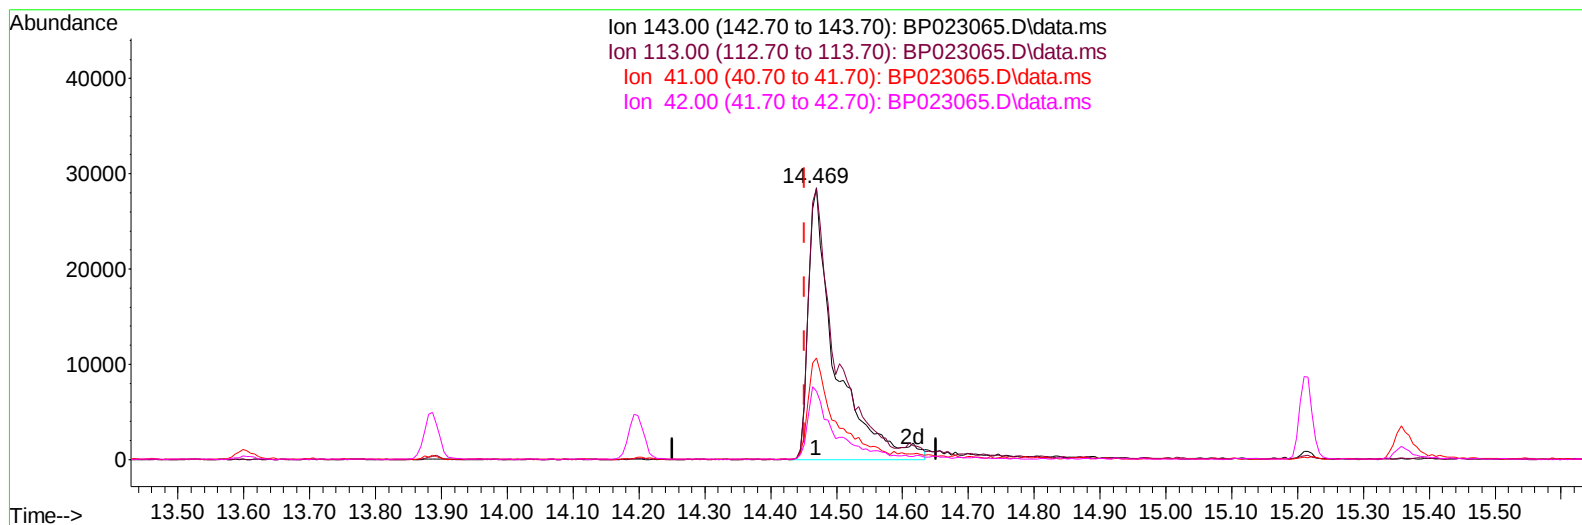

TIC: BP023065.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.469min (+ 0.018) 27.90 ng/ul m

response 80687

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	99.75
41.00	39.20	37.33
42.00	25.90	25.15

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023065.D
 Acq On : 13 Nov 2024 04:03
 Operator : RC/JU
 Sample : PB164834BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK834

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 13 05:17:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	82766	20.000	ng/ul	0.00
20) Naphthalene-d8	10.334	136	327994	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.198	164	267044	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.010	188	690699	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	758610	20.000	ng/ul	0.00
88) Perylene-d12	24.651	264	866364	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	10984	6.379	ng/uL	0.00
4) Pyridine-d5	3.552	84	138949	27.161	ng/ul	0.00
7) Phenol-d5	6.787	99	172308	28.159	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.940	67	109293	30.400	ng/ul	0.01
11) 2-Chlorophenol-d4	7.128	132	134904	30.102	ng/ul	0.00
15) 4-Methylphenol-d8	8.299	113	147860	29.364	ng/ul	0.00
21) Nitrobenzene-d5	8.734	128	69483	30.430	ng/ul	0.01
24) 2-Nitrophenol-d4	9.446	143	82715	30.385	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	9.981	165	153985	27.011	ng/ul	0.01
31) 4-Chloroaniline-d4	10.487	131	190135	27.956	ng/ul	0.00
46) Dimethylphthalate-d6	13.604	166	619871	32.207	ng/ul	0.00
49) Acenaphthylene-d8	13.887	160	624240	31.084	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.469	143	80687m	27.896	ng/ul	0.02
60) Fluorene-d10	15.216	176	536026	31.766	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	105104	25.402	ng/ul	0.00
73) Anthracene-d10	17.104	188	928047	31.734	ng/ul	-0.01
81) Pyrene-d10	19.498	212	1198159	34.290	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.427	264	1351033	32.738	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023065.D
Acq On : 13 Nov 2024 04:03
Operator : RC/JU
Sample : PB164834BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK834

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 13 05:17:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

