

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023070.D
 Acq On : 13 Nov 2024 07:26
 Operator : RC/JU
 Sample : P4687-24
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CP8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/14/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 13 07:53:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	78159	20.000	ng/u1	0.00
20) Naphthalene-d8	10.334	136	299951	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.204	164	249473	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.004	188	645444	20.000	ng/u1	-0.01
79) Chrysene-d12	21.439	240	760446	20.000	ng/u1	0.00
88) Perylene-d12	24.657	264	916803	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	7943	4.885	ng/uL	0.00
4) Pyridine-d5	3.558	84	46277	9.579	ng/u1	0.01
7) Phenol-d5	6.793	99	55471	9.600	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	6.928	67	102721	30.257	ng/u1	0.00
11) 2-Chlorophenol-d4	7.134	132	120396	28.449	ng/u1	0.00
15) 4-Methylphenol-d8	8.299	113	100730	21.183	ng/u1	0.00
21) Nitrobenzene-d5	8.728	128	65707	31.466	ng/u1	0.00
24) 2-Nitrophenol-d4	9.440	143	78993	31.731	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.981	165	167738	32.174	ng/u1	0.01
31) 4-Chloroaniline-d4	10.481	131	163144	26.230	ng/u1	0.00
46) Dimethylphthalate-d6	13.616	166	650186	36.161	ng/u1	0.00
49) Acenaphthylene-d8	13.898	160	608298	32.423	ng/u1	0.00
54) 4-Nitrophenol-d4	14.498	143	26510m	9.811	ng/u1	0.05
60) Fluorene-d10	15.210	176	551276	34.970	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.369	200	118188	30.567	ng/u1	0.00
73) Anthracene-d10	17.116	188	993455	36.352	ng/u1	0.00
81) Pyrene-d10	19.492	212	1288584	36.789	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.427	264	1601188	36.665	ng/u1	-0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.345	149	30161	1.487	ng/u1	Qvalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023070.D
Acq On : 13 Nov 2024 07:26
Operator : RC/JU
Sample : P4687-24
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
C0CP8

Quant Time: Nov 13 07:53:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/14/2024
Supervised By :mohammad ahmed 11/14/2024

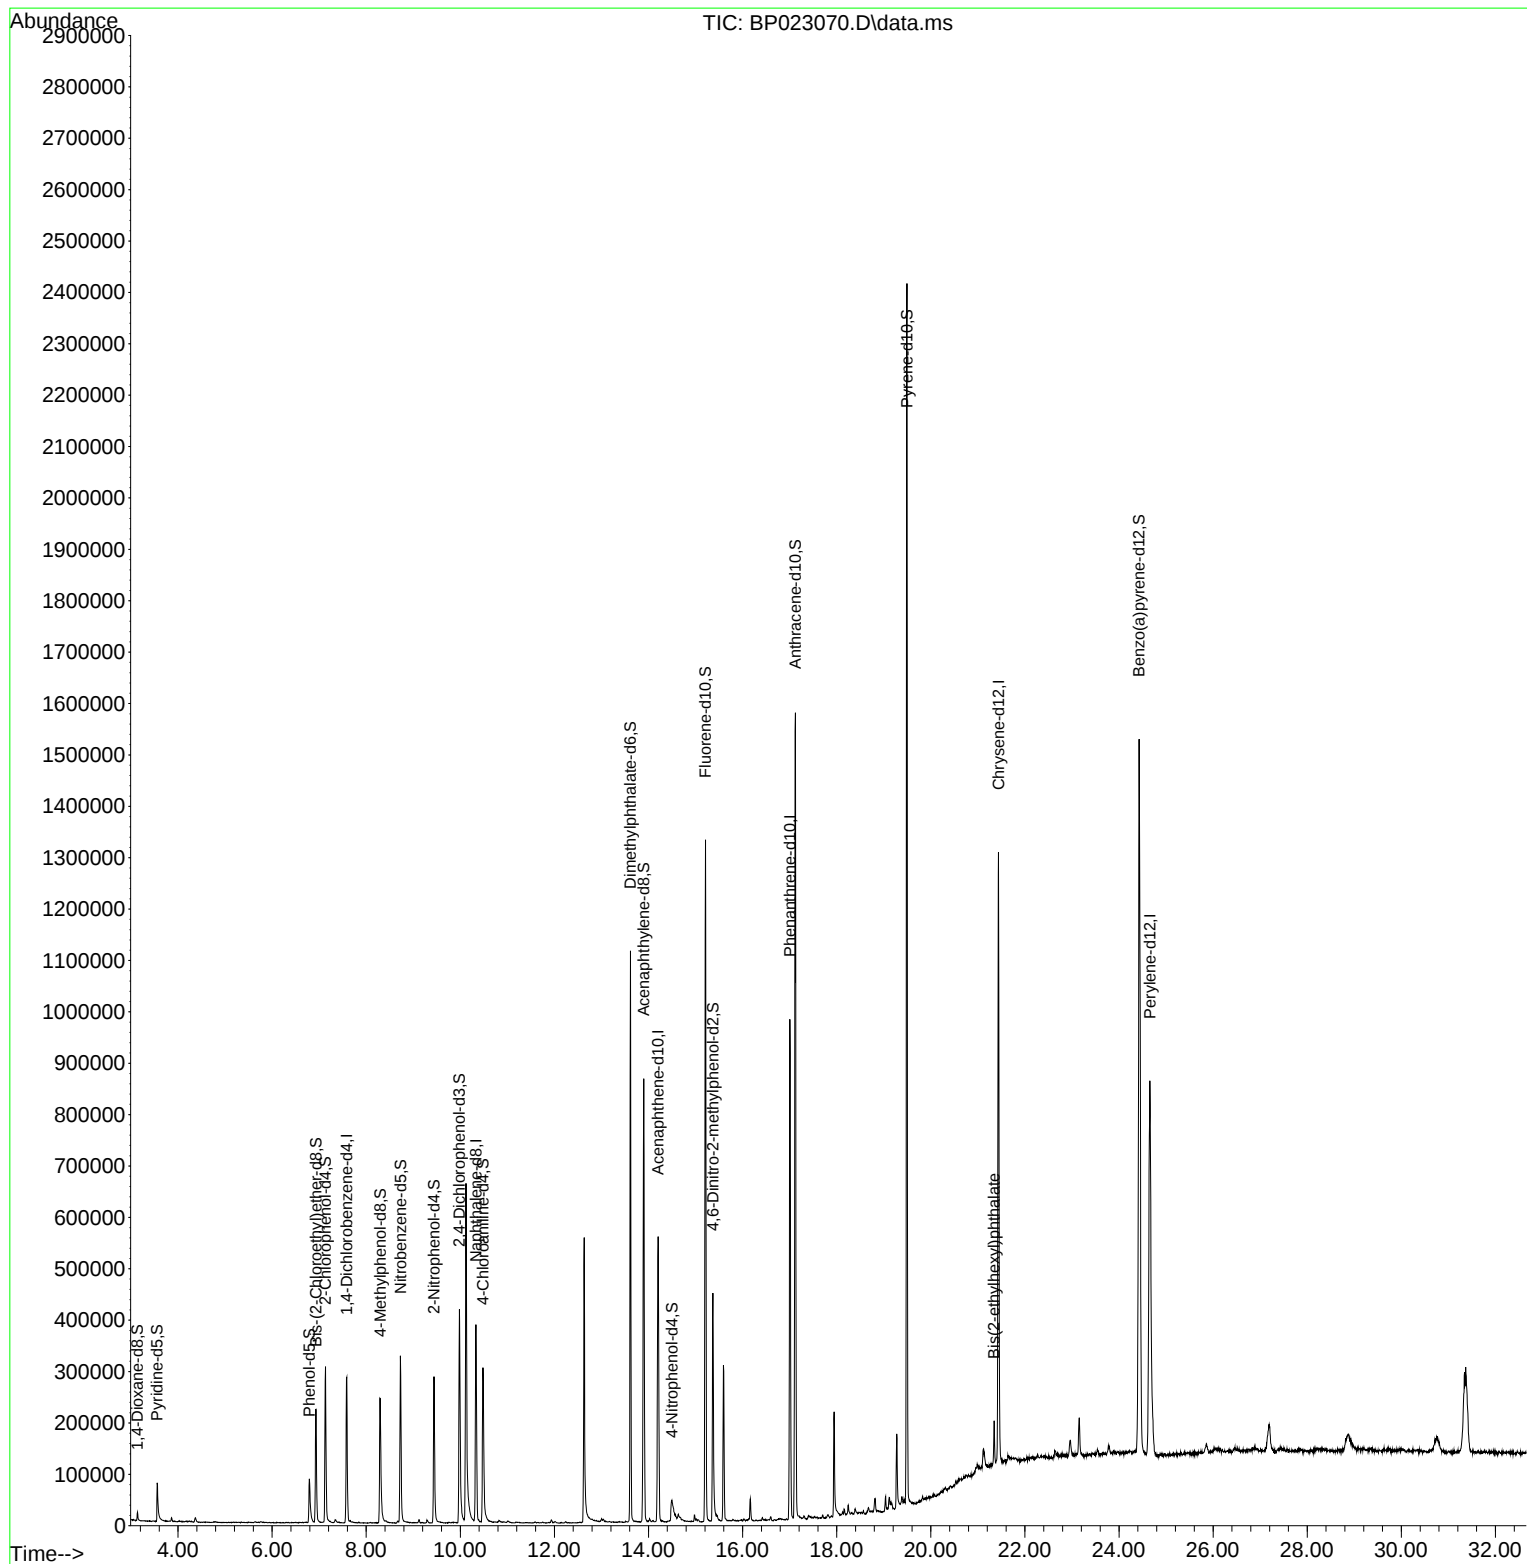

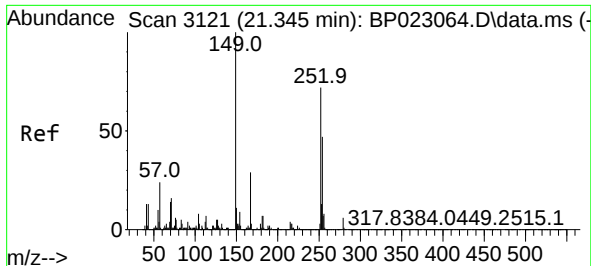

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.487 ng/ul
 RT: 21.345 min Scan# 3121
 Delta R.T. -0.000 min
 Lab File: BP023070.D
 Acq: 13 Nov 2024 07:26

Instrument :
 BNA_P
 ClientSampleId :
 C0CP8

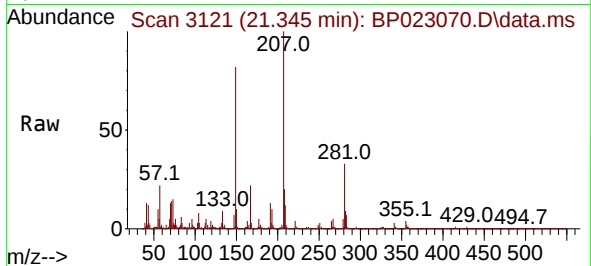

Tgt Ion:149 Resp: 3016
 Ion Ratio Lower Upper
 149 100
 167 27.0 24.5 36.7
 279 6.3 5.5 8.3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/14/2024
 Supervised By :mohammad ahmed 11/14/2024

