

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023026.D
 Acq On : 11 Nov 2024 23:09
 Operator : RC/JU
 Sample : P4668-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COAE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	34	rVB2	10718	14922	0.70%	0.094%
2	3.581	98	101	115	rBV	10912	28540	1.34%	0.180%
3	3.863	145	149	154	rVB5	3936	6201	0.29%	0.039%
4	4.363	229	234	240	rBV	18530	26255	1.24%	0.166%
5	6.728	633	636	642	rVV6	1778	2505	0.12%	0.016%
6	6.799	642	648	665	rVV	36754	88806	4.18%	0.560%
7	6.934	665	671	687	rVB	157065	257784	12.13%	1.626%
8	7.134	699	705	720	rBV	179096	313934	14.78%	1.981%
9	7.587	775	782	792	rBV	179591	314956	14.82%	1.987%
10	7.669	794	796	803	rVB7	1853	2934	0.14%	0.019%
11	8.299	895	903	919	rBV	143812	281897	13.27%	1.778%
12	8.728	970	976	988	rBV	204134	370684	17.45%	2.339%
13	9.116	1037	1042	1048	rBV9	1559	3152	0.15%	0.020%
14	9.446	1091	1098	1116	rBV	171267	326702	15.38%	2.061%
15	9.987	1182	1190	1207	rBV	197896	474032	22.31%	2.991%
16	10.334	1241	1249	1259	rBV	262810	431111	20.29%	2.720%
17	10.498	1270	1277	1292	rBV	63295	170266	8.01%	1.074%
18	11.957	1520	1525	1528	rBV4	2722	4280	0.20%	0.027%
19	12.534	1619	1623	1629	rBV8	2401	4941	0.23%	0.031%
20	12.798	1661	1668	1674	rBV8	3053	6529	0.31%	0.041%
21	13.616	1800	1807	1824	rBV	567468	823606	38.77%	5.196%
22	13.892	1846	1854	1873	rBV2	502672	844683	39.76%	5.329%
23	14.198	1899	1906	1917	rBV	389950	644408	30.33%	4.066%
24	14.522	1955	1961	1965	rBV5	13672	31253	1.47%	0.197%
25	14.634	1978	1980	1988	rVB9	2645	3413	0.16%	0.022%
26	14.710	1988	1993	1998	rVB	9836	13732	0.65%	0.087%
27	15.022	2041	2046	2049	rBV6	1714	2679	0.13%	0.017%
28	15.051	2049	2051	2059	rVB9	1464	2709	0.13%	0.017%
29	15.210	2071	2078	2088	rBV	716470	1185754	55.81%	7.481%
30	15.310	2093	2095	2100	rVB5	2070	2446	0.12%	0.015%
31	15.381	2100	2107	2119	rBV	217015	382295	17.99%	2.412%
32	15.469	2119	2122	2129	rVB6	6724	11846	0.56%	0.075%
33	16.022	2214	2216	2223	rVB8	1428	2141	0.10%	0.014%
34	17.010	2377	2384	2395	rBV	589979	886082	41.71%	5.590%
35	17.122	2395	2403	2418	rVV	801322	1387351	65.30%	8.753%
36	17.957	2541	2545	2553	rBV7	10414	17756	0.84%	0.112%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023026.D
Acq On : 11 Nov 2024 23:09
Operator : RC/JU
Sample : P4668-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	19.051	2728	2731	2736	rBV3	12614	16499	0.78%	0.104%
38	19.122	2740	2743	2750	rVB	11891	16468	0.78%	0.104%
39	19.292	2768	2772	2776	rBV6	9428	16629	0.78%	0.105%
40	19.498	2801	2807	2824	rVB	1274043	1801558	84.80%	11.366%
41	21.457	3135	3140	3151	rVB2	692756	1166879	54.92%	7.362%
42	24.468	3643	3652	3667	rVB	831000	2124502	100.00%	13.404%
43	24.698	3683	3691	3708	rVB	504123	1335178	62.85%	8.424%




Sum of corrected areas: 15850298

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023026.D
Acq On : 11 Nov 2024 23:09
Operator : RC/JU
Sample : P4668-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

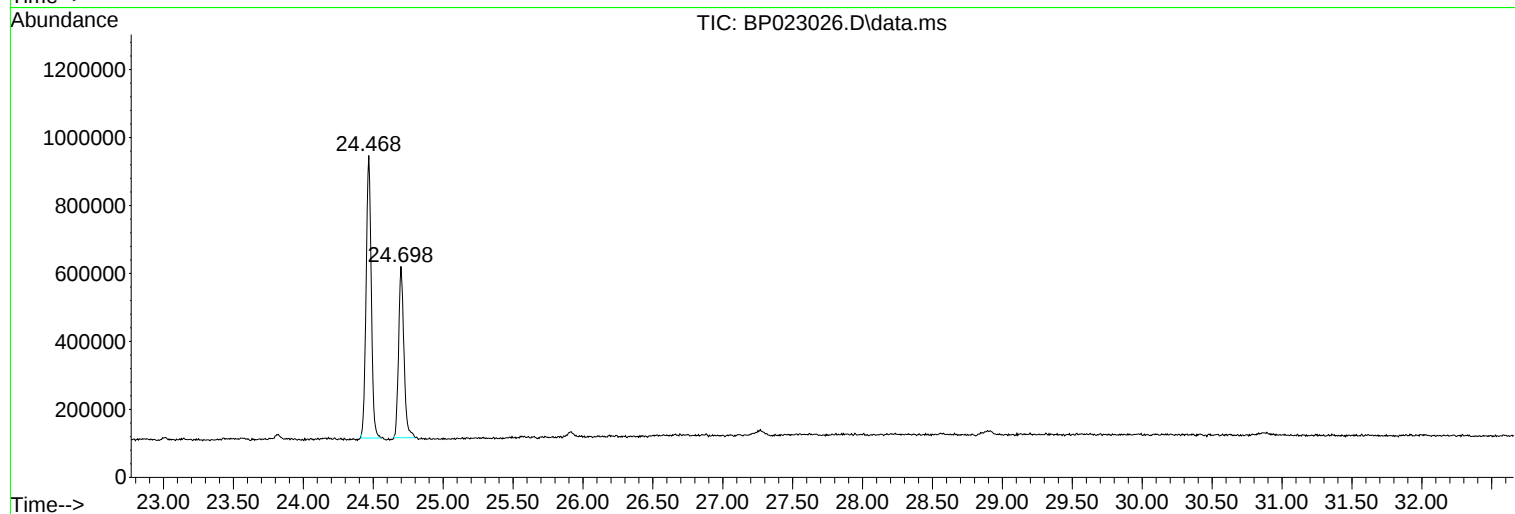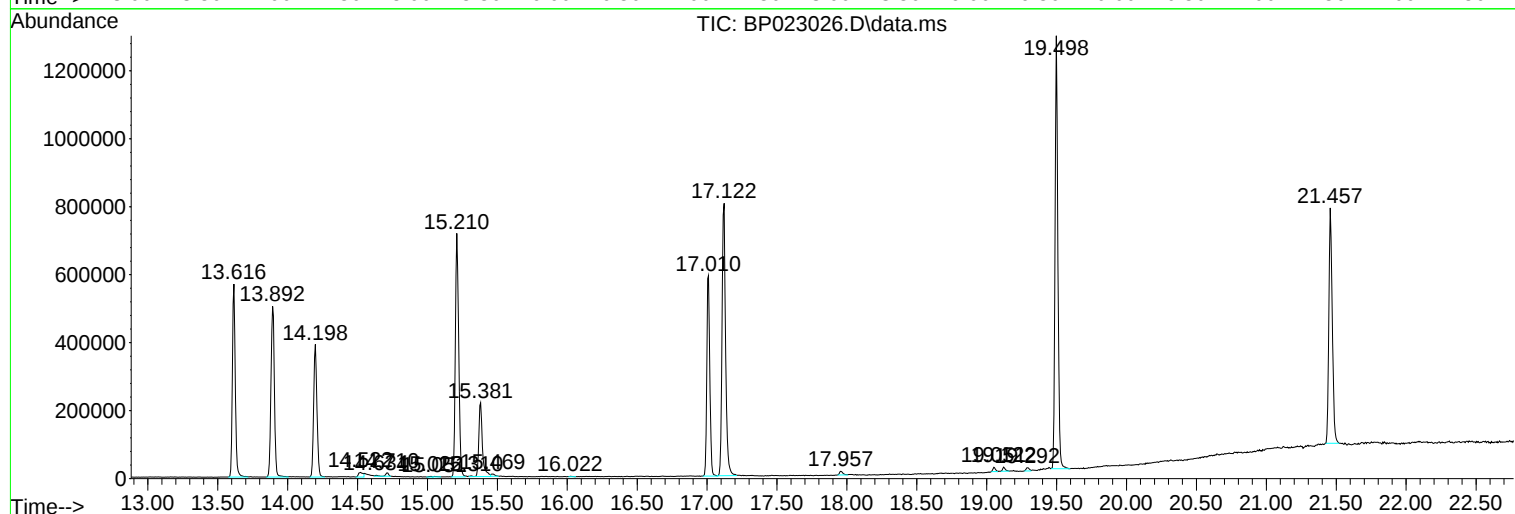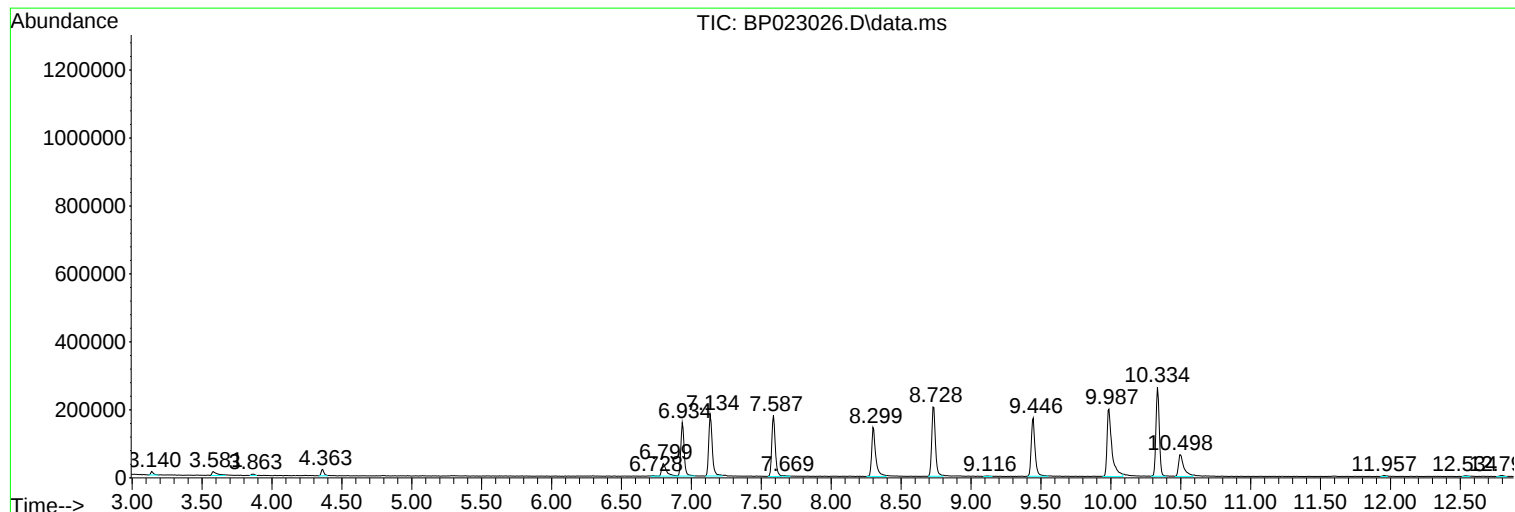

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023026.D
Acq On : 11 Nov 2024 23:09
Operator : RC/JU
Sample : P4668-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023026.D
Acq On : 11 Nov 2024 23:09
Operator : RC/JU
Sample : P4668-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
