

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023033.D
 Acq On : 12 Nov 2024 04:34
 Operator : RC/JU
 Sample : P4717-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	30	rBV	12117	16608	0.61%	0.087%
2	3.170	30	31	36	rVB2	4517	5328	0.20%	0.028%
3	3.564	94	98	113	rBV	37846	74142	2.73%	0.387%
4	3.864	145	149	155	rVB5	3433	4398	0.16%	0.023%
5	4.364	230	234	239	rBV3	6192	9354	0.34%	0.049%
6	6.799	642	648	666	rBV	45857	104787	3.86%	0.547%
7	6.934	666	671	680	rBV	168165	269964	9.93%	1.408%
8	7.134	697	705	724	rBV	194221	348370	12.82%	1.818%
9	7.587	774	782	793	rBV	209662	355049	13.06%	1.852%
10	8.305	897	904	928	rBV	141406	296353	10.90%	1.546%
11	8.728	969	976	992	rBV	219373	403740	14.85%	2.106%
12	9.122	1037	1043	1049	rVB9	1757	3806	0.14%	0.020%
13	9.440	1091	1097	1118	rBV	179546	363141	13.36%	1.895%
14	9.987	1183	1190	1211	rBV	235749	520118	19.14%	2.714%
15	10.334	1242	1249	1257	rBV	321183	490965	18.06%	2.561%
16	10.493	1268	1276	1298	rBV	144017	373723	13.75%	1.950%
17	10.646	1300	1302	1311	rVB9	1589	3096	0.11%	0.016%
18	11.963	1519	1526	1532	rBV6	2705	7014	0.26%	0.037%
19	13.604	1799	1805	1820	rBV	709313	934188	34.37%	4.874%
20	13.898	1848	1855	1871	rBV	713872	930792	34.24%	4.856%
21	14.210	1900	1908	1919	rBV	483238	763290	28.08%	3.982%
22	14.510	1953	1959	1974	rBV7	18835	84491	3.11%	0.441%
23	15.222	2071	2080	2089	rBV	756742	1344690	49.47%	7.016%
24	15.369	2100	2105	2117	rBV	311471	501684	18.46%	2.617%
25	15.457	2117	2120	2127	rVB6	6182	12966	0.48%	0.068%
26	17.022	2378	2386	2396	rVV	634482	1035926	38.11%	5.405%
27	17.122	2396	2403	2422	rVB	1216751	1748486	64.33%	9.122%
28	17.428	2451	2455	2458	rBV6	1677	2842	0.10%	0.015%
29	17.586	2479	2482	2487	rVB6	2492	3655	0.13%	0.019%
30	17.957	2540	2545	2553	rBV4	22476	38612	1.42%	0.201%
31	18.498	2633	2637	2639	rBV4	3630	5040	0.19%	0.026%
32	18.575	2648	2650	2655	rVB6	3836	5258	0.19%	0.027%
33	18.633	2655	2660	2663	rBV6	2493	4807	0.18%	0.025%
34	18.845	2692	2696	2699	rBV5	3129	5605	0.21%	0.029%
35	19.039	2725	2729	2734	rBV3	13964	23326	0.86%	0.122%
36	19.133	2740	2745	2747	rBV2	13002	21020	0.77%	0.110%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023033.D
Acq On : 12 Nov 2024 04:34
Operator : RC/JU
Sample : P4717-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	19.163	2747	2750	2759	rVB4	40989	59716	2.20%	0.312%
38	19.292	2768	2772	2777	rBV4	30306	42007	1.55%	0.219%
39	19.404	2789	2791	2795	rBV5	5172	5698	0.21%	0.030%
40	19.504	2801	2808	2817	rBV	1596895	2267966	83.44%	11.833%
41	21.457	3134	3140	3150	rBV	857535	1399375	51.48%	7.301%
42	24.468	3642	3652	3664	rVB	1054451	2718120	100.00%	14.181%
43	24.686	3680	3689	3707	rVB	486774	1557737	57.31%	8.127%




Sum of corrected areas: 19167253

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023033.D
Acq On : 12 Nov 2024 04:34
Operator : RC/JU
Sample : P4717-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

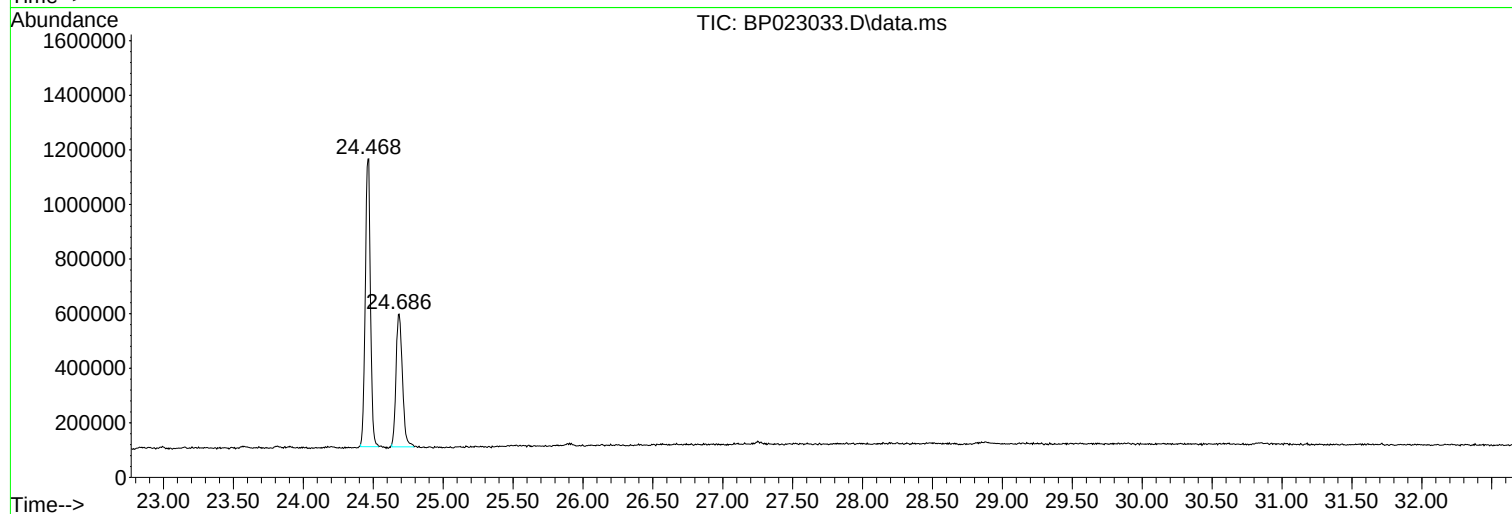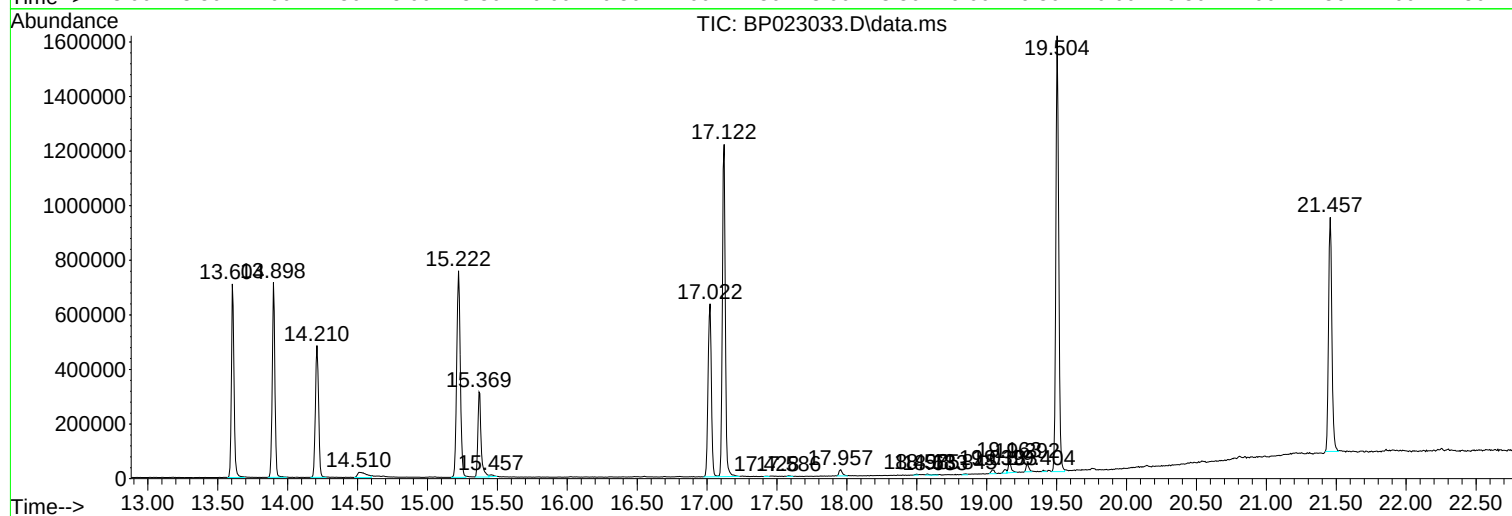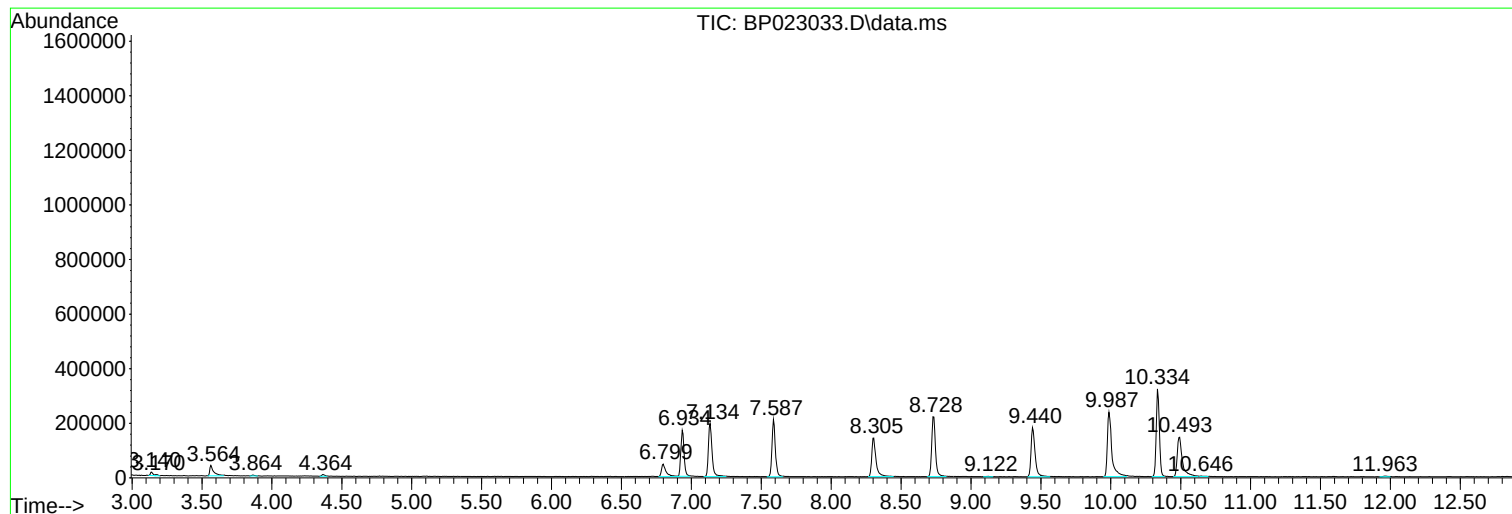

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023033.D
Acq On : 12 Nov 2024 04:34
Operator : RC/JU
Sample : P4717-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023033.D
Acq On : 12 Nov 2024 04:34
Operator : RC/JU
Sample : P4717-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
