

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023034.D
 Acq On : 12 Nov 2024 05:14
 Operator : RC/JU
 Sample : P4717-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	23	26	30	rBV2	12018	13717	0.54%	0.082%
2	3.569	96	99	111	rBV	27205	56203	2.19%	0.334%
3	3.864	145	149	156	rVB4	3430	6257	0.24%	0.037%
4	4.369	229	235	240	rBV	8383	13781	0.54%	0.082%
5	6.799	641	648	661	rBV	39061	95254	3.72%	0.566%
6	6.940	666	672	684	rVB	157915	255876	9.98%	1.522%
7	7.134	699	705	716	rBV	177341	321297	12.54%	1.911%
8	7.587	775	782	798	rBV	175548	297708	11.62%	1.770%
9	8.299	897	903	923	rVV	144217	293110	11.44%	1.743%
10	8.734	970	977	990	rBV	210227	381671	14.89%	2.270%
11	9.110	1038	1041	1047	rBV8	1386	3206	0.13%	0.019%
12	9.440	1089	1097	1116	rBV	187563	338997	13.23%	2.016%
13	9.987	1183	1190	1224	rBV	220072	504972	19.70%	3.003%
14	10.334	1242	1249	1262	rBV	231189	388269	15.15%	2.309%
15	10.487	1269	1275	1295	rBV	164756	361148	14.09%	2.148%
16	11.969	1521	1527	1533	rBV6	3130	6421	0.25%	0.038%
17	13.610	1801	1806	1822	rBV	657767	885063	34.53%	5.263%
18	13.898	1848	1855	1864	rBV2	546328	852873	33.28%	5.072%
19	14.210	1901	1908	1919	rBV	394719	587282	22.91%	3.492%
20	14.522	1955	1961	1962	rBV4	15885	24506	0.96%	0.146%
21	14.692	1988	1990	1994	rVB5	2417	3066	0.12%	0.018%
22	15.222	2072	2080	2096	rBV	651964	1218993	47.56%	7.249%
23	15.369	2099	2105	2119	rBV	249268	444382	17.34%	2.643%
24	16.486	2290	2295	2297	rBV5	1724	2939	0.11%	0.017%
25	17.016	2378	2385	2394	rBV	472478	795229	31.03%	4.729%
26	17.116	2396	2402	2421	rVB	1066483	1544631	60.27%	9.186%
27	17.575	2477	2480	2484	rVB4	2500	3702	0.14%	0.022%
28	17.957	2539	2545	2551	rBV10	9240	16253	0.63%	0.097%
29	18.580	2646	2651	2655	rBV8	2768	4685	0.18%	0.028%
30	19.045	2725	2730	2734	rBV3	13499	20946	0.82%	0.125%
31	19.122	2739	2743	2749	rVB4	8724	17494	0.68%	0.104%
32	19.298	2769	2773	2776	rBV6	10895	17697	0.69%	0.105%
33	19.433	2794	2796	2800	rVB4	4777	4784	0.19%	0.028%
34	19.492	2800	2806	2819	rBV2	1305907	2076556	81.02%	12.349%
35	21.457	3134	3140	3151	rBV	742498	1162283	45.35%	6.912%
36	24.474	3642	3653	3665	rVB	998700	2563017	100.00%	15.242%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023034.D
Acq On : 12 Nov 2024 05:14
Operator : RC/JU
Sample : P4717-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	24.692	3681	3690	3700	rBV	455387	1231568	48.05%	7.324%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 16815836

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023034.D
Acq On : 12 Nov 2024 05:14
Operator : RC/JU
Sample : P4717-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

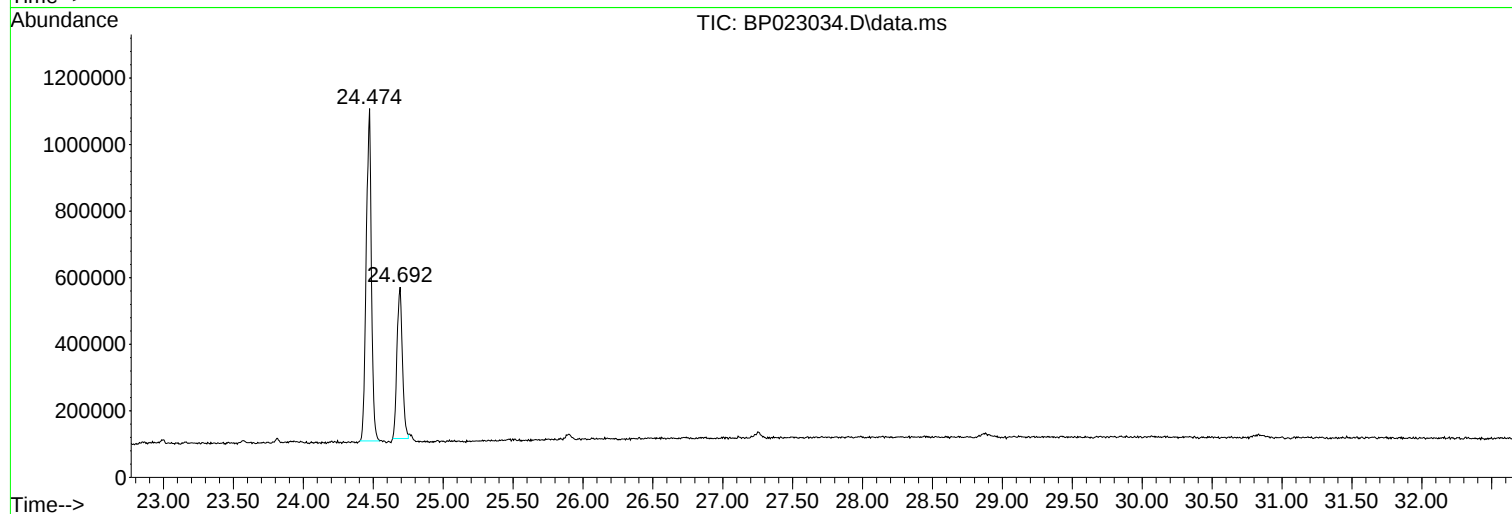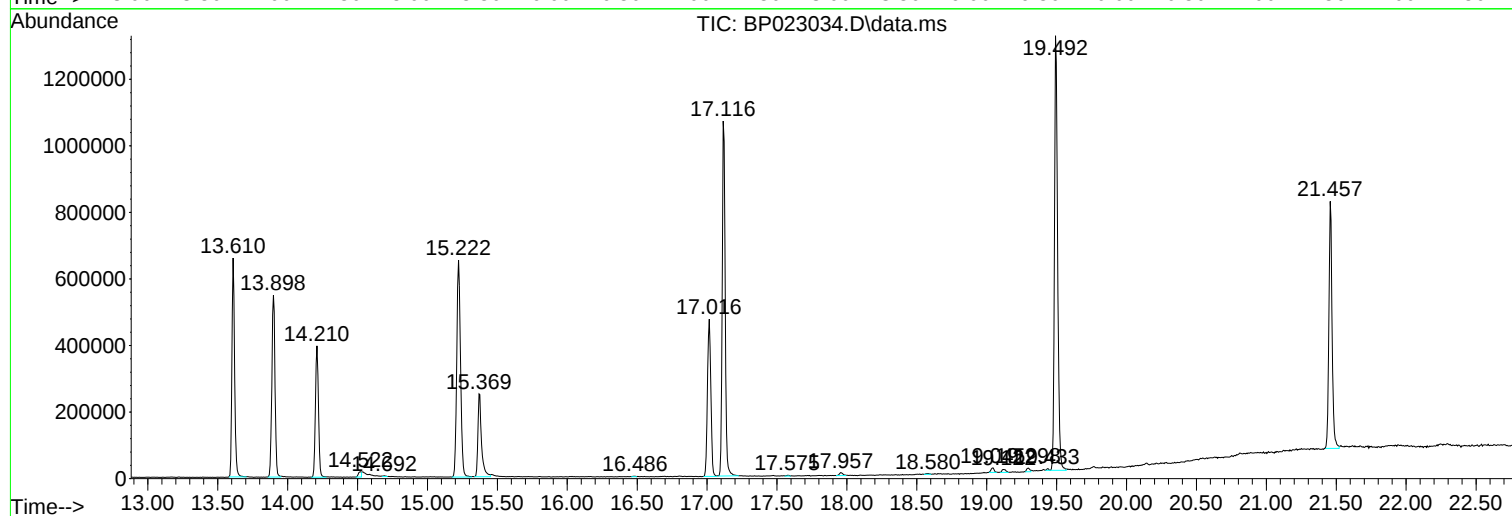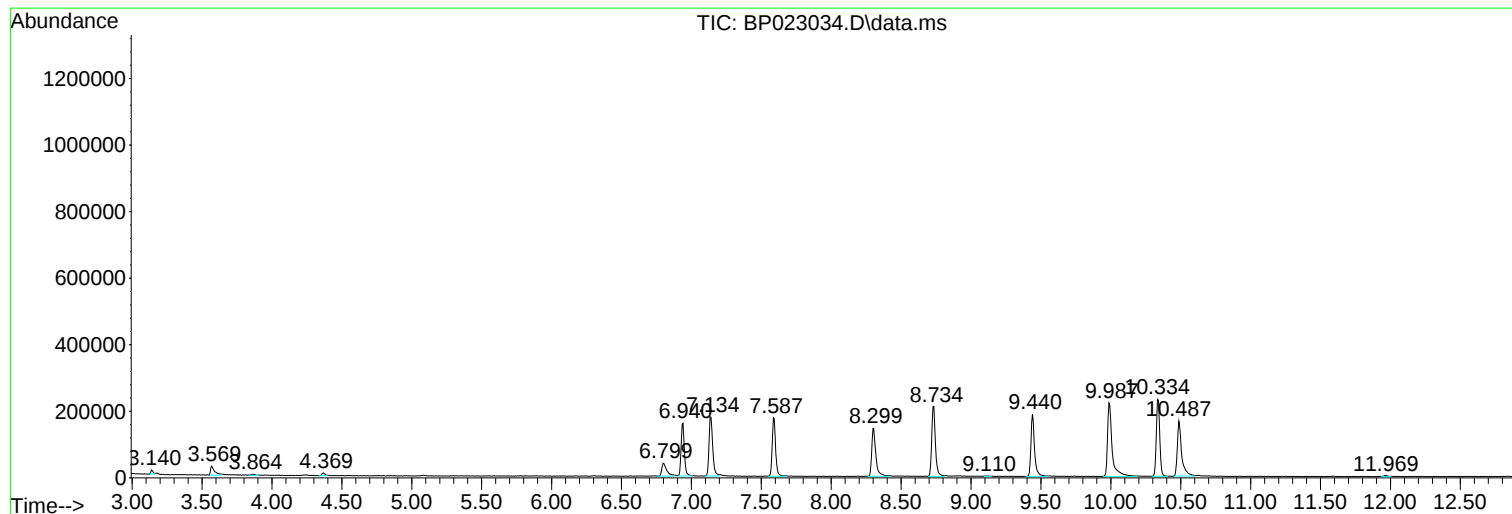

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023034.D
Acq On : 12 Nov 2024 05:14
Operator : RC/JU
Sample : P4717-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023034.D
Acq On : 12 Nov 2024 05:14
Operator : RC/JU
Sample : P4717-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
