

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023035.D
 Acq On : 12 Nov 2024 05:55
 Operator : RC/JU
 Sample : P4717-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	30	rBV	10369	12466	0.43%	0.063%
2	3.564	95	98	111	rBV	35320	69644	2.41%	0.350%
3	3.864	146	149	153	rVB6	2674	3477	0.12%	0.017%
4	4.364	230	234	241	rBV2	8200	13084	0.45%	0.066%
5	4.940	328	332	338	rBV4	5612	9707	0.34%	0.049%
6	5.093	352	358	360	rVB6	2030	3065	0.11%	0.015%
7	6.793	642	647	662	rBV	48611	105386	3.65%	0.530%
8	6.934	665	671	687	rVB	183150	288914	10.01%	1.452%
9	7.134	698	705	720	rBV	207467	360674	12.49%	1.813%
10	7.587	774	782	800	rBV	189281	326192	11.30%	1.639%
11	8.299	896	903	921	rBV2	157517	331324	11.48%	1.665%
12	8.728	968	976	987	rBV	237048	426617	14.78%	2.144%
13	9.440	1090	1097	1111	rBV	218986	395304	13.69%	1.987%
14	9.987	1183	1190	1218	rBV2	252710	580514	20.11%	2.917%
15	10.340	1242	1250	1258	rBV	246812	438353	15.18%	2.203%
16	10.487	1268	1275	1299	rBV	197418	441357	15.29%	2.218%
17	11.205	1390	1397	1412	rBV	4667	14977	0.52%	0.075%
18	11.952	1519	1524	1530	rBV5	2779	6068	0.21%	0.030%
19	13.616	1799	1807	1818	rBV	805322	1106457	38.33%	5.561%
20	13.904	1848	1856	1866	rBV	670513	1052937	36.47%	5.292%
21	14.216	1902	1909	1919	rBV	491875	694565	24.06%	3.491%
22	14.522	1953	1961	1975	rBV4	20878	84974	2.94%	0.427%
23	14.687	1986	1989	1997	rVB9	3785	6417	0.22%	0.032%
24	15.222	2071	2080	2092	rBV	949915	1553727	53.82%	7.808%
25	15.304	2092	2094	2098	rVB4	2876	2966	0.10%	0.015%
26	15.369	2098	2105	2118	rBV	292001	543621	18.83%	2.732%
27	15.463	2118	2121	2128	rVB6	5986	11475	0.40%	0.058%
28	16.687	2323	2329	2331	rBV6	1781	3436	0.12%	0.017%
29	17.022	2379	2386	2396	rVV	653293	978801	33.90%	4.919%
30	17.116	2396	2402	2416	rVV	1330952	1899207	65.78%	9.545%
31	17.963	2542	2546	2550	rBV5	7754	11418	0.40%	0.057%
32	19.045	2725	2730	2735	rVB2	17640	27823	0.96%	0.140%
33	19.134	2740	2745	2749	rBV	14316	23207	0.80%	0.117%
34	19.298	2770	2773	2777	rBV4	6570	10744	0.37%	0.054%
35	19.439	2794	2797	2800	rBV5	4209	5036	0.17%	0.025%
36	19.498	2801	2807	2822	rVV	1544619	2463687	85.34%	12.382%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023035.D
Acq On : 12 Nov 2024 05:55
Operator : RC/JU
Sample : P4717-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	21.457	3133	3140	3151	rBV	653085	1287134	44.58%	6.469%
38	24.463	3641	3651	3665	rVB	1290987	2887035	100.00%	14.509%
39	24.686	3679	3689	3707	rVB	486540	1416266	49.06%	7.118%




Sum of corrected areas: 19898056

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023035.D
Acq On : 12 Nov 2024 05:55
Operator : RC/JU
Sample : P4717-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

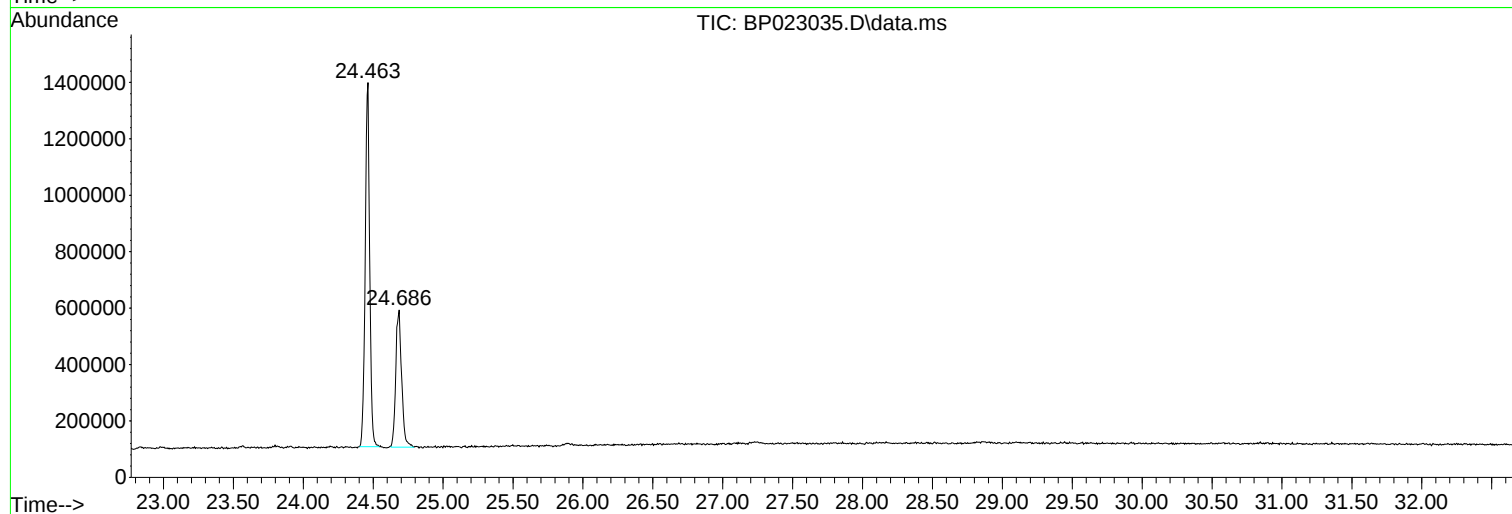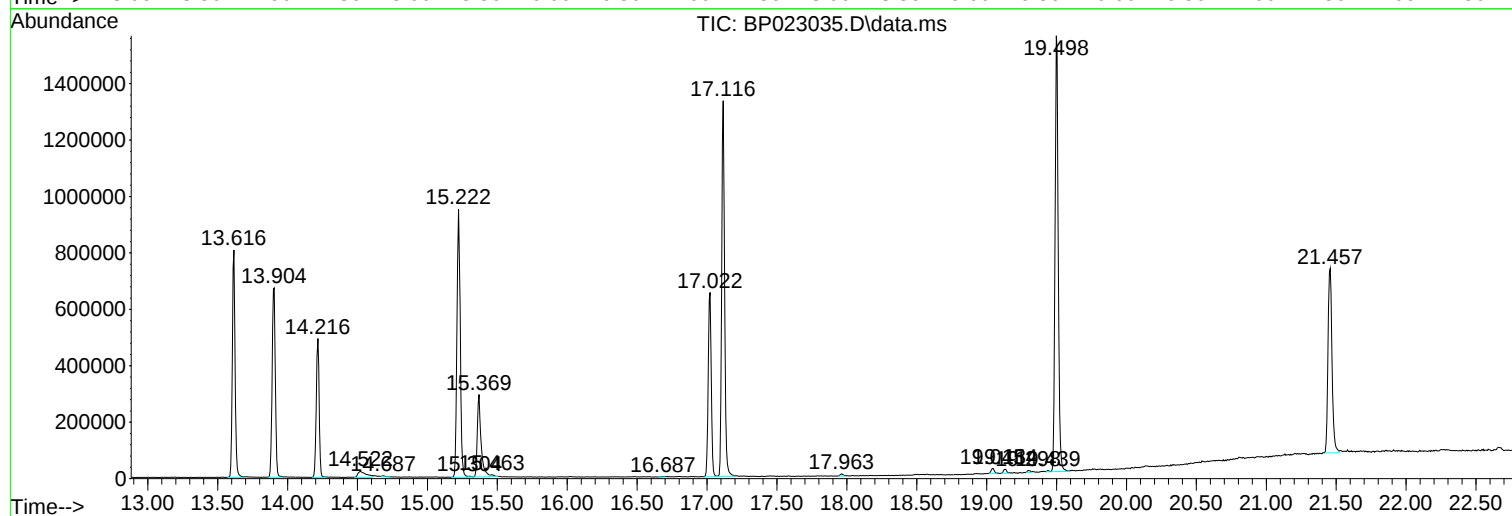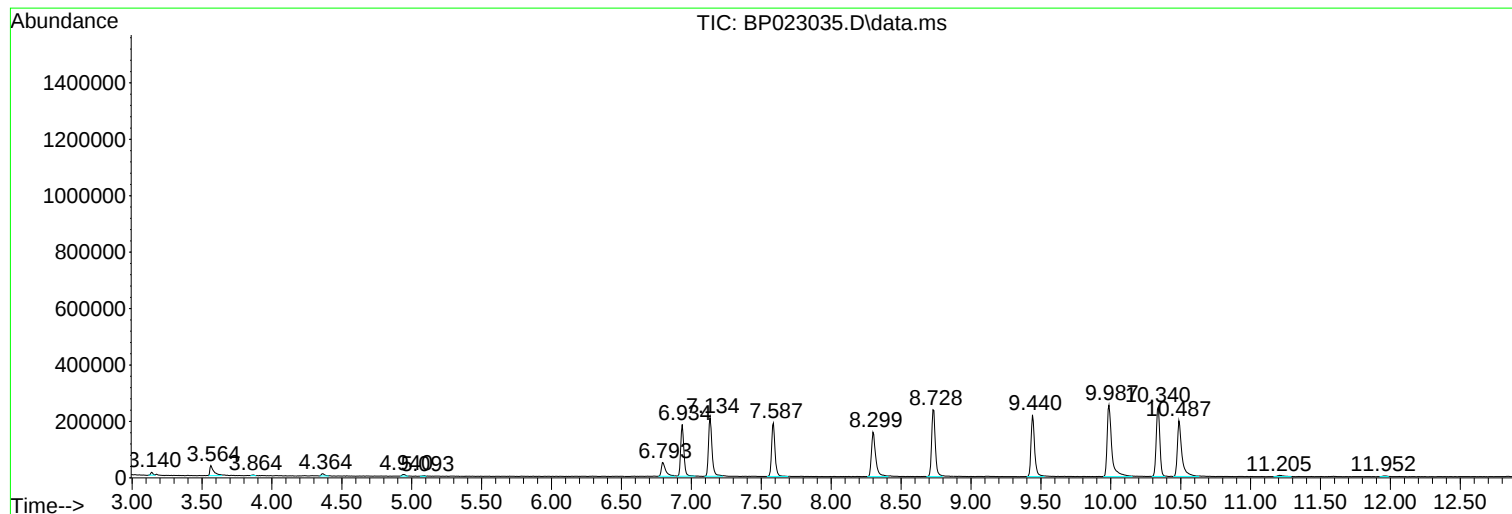

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023035.D
Acq On : 12 Nov 2024 05:55
Operator : RC/JU
Sample : P4717-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023035.D
Acq On : 12 Nov 2024 05:55
Operator : RC/JU
Sample : P4717-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc