

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023045.D
 Acq On : 12 Nov 2024 13:52
 Operator : RC/JU
 Sample : P4741-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E27L8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	33	rVB	13260	17635	0.59%	0.078%
2	3.564	95	98	112	rBV	37916	73887	2.49%	0.326%
3	3.864	146	149	154	rBV5	3156	5277	0.18%	0.023%
4	4.293	218	222	227	rVB5	2331	4190	0.14%	0.019%
5	6.728	632	636	641	rBV4	2184	3375	0.11%	0.015%
6	6.793	641	647	665	rBV2	99692	217541	7.32%	0.961%
7	6.934	665	671	684	rVB	208272	337259	11.35%	1.490%
8	7.134	698	705	716	rBV	273365	475236	16.00%	2.099%
9	7.587	772	782	794	rBV	241299	411778	13.86%	1.819%
10	8.293	894	902	924	rBV	282960	530413	17.85%	2.343%
11	8.728	969	976	989	rBV	275331	495212	16.67%	2.187%
12	9.128	1037	1044	1049	rVB7	3318	6553	0.22%	0.029%
13	9.446	1090	1098	1111	rBV	232967	452429	15.23%	1.998%
14	9.981	1183	1189	1218	rBV	310460	698513	23.51%	3.086%
15	10.334	1242	1249	1257	rBV	338613	564227	18.99%	2.492%
16	10.487	1268	1275	1292	rBV	223679	507002	17.07%	2.240%
17	11.957	1520	1525	1532	rBV7	3701	8878	0.30%	0.039%
18	12.481	1610	1614	1619	rBV7	2162	3260	0.11%	0.014%
19	13.598	1797	1804	1821	rBV	643913	1136493	38.25%	5.020%
20	13.740	1823	1828	1837	rVB7	10637	19282	0.65%	0.085%
21	13.887	1843	1853	1866	rBV	831567	1199558	40.38%	5.299%
22	14.128	1890	1894	1899	rBV7	5170	8494	0.29%	0.038%
23	14.198	1899	1906	1924	rVB	584764	883535	29.74%	3.903%
24	14.487	1946	1955	1976	rBV2	56065	206331	6.94%	0.911%
25	14.628	1978	1979	1983	rVV4	6774	8396	0.28%	0.037%
26	14.675	1985	1987	1994	rVB8	3756	6824	0.23%	0.030%
27	14.869	2015	2020	2024	rBV	64277	86760	2.92%	0.383%
28	14.904	2024	2026	2033	rVV3	20212	25372	0.85%	0.112%
29	15.222	2073	2080	2090	rVV	1197167	1626344	54.74%	7.184%
30	15.363	2097	2104	2120	rBV	317563	568933	19.15%	2.513%
31	15.475	2121	2123	2128	rVB5	6923	9454	0.32%	0.042%
32	15.745	2162	2169	2175	rBV5	3368	8406	0.28%	0.037%
33	15.804	2175	2179	2185	rVB8	2826	5357	0.18%	0.024%
34	16.534	2298	2303	2304	rBV5	2713	3446	0.12%	0.015%
35	16.581	2308	2311	2316	rVB3	5847	7453	0.25%	0.033%
36	17.010	2370	2384	2393	rBV	924930	1250340	42.09%	5.523%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023045.D
Acq On : 12 Nov 2024 13:52
Operator : RC/JU
Sample : P4741-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27L8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	17.098	2393	2399	2417	rVB	1288904	1935223	65.14%	8.548%
38	17.704	2498	2502	2506	rVB6	7766	10836	0.36%	0.048%
39	17.892	2532	2534	2538	rVB5	4213	4452	0.15%	0.020%
40	17.945	2538	2543	2548	rBV7	11113	17491	0.59%	0.077%
41	18.157	2575	2579	2582	rBV6	2784	3826	0.13%	0.017%
42	19.033	2724	2728	2732	rBV5	15974	23820	0.80%	0.105%
43	19.128	2739	2744	2748	rBV2	14720	22449	0.76%	0.099%
44	19.286	2767	2771	2776	rBV7	13584	23713	0.80%	0.105%
45	19.492	2800	2806	2823	rVB	1517376	2443972	82.26%	10.796%
46	21.445	3132	3138	3150	rBV2	1033330	1552529	52.26%	6.858%
47	24.439	3638	3647	3661	rVB	1295476	2970968	100.00%	13.124%
48	24.663	3675	3685	3705	rVB	577854	1755764	59.10%	7.756%




Sum of corrected areas: 22638486

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023045.D
Acq On : 12 Nov 2024 13:52
Operator : RC/JU
Sample : P4741-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27L8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

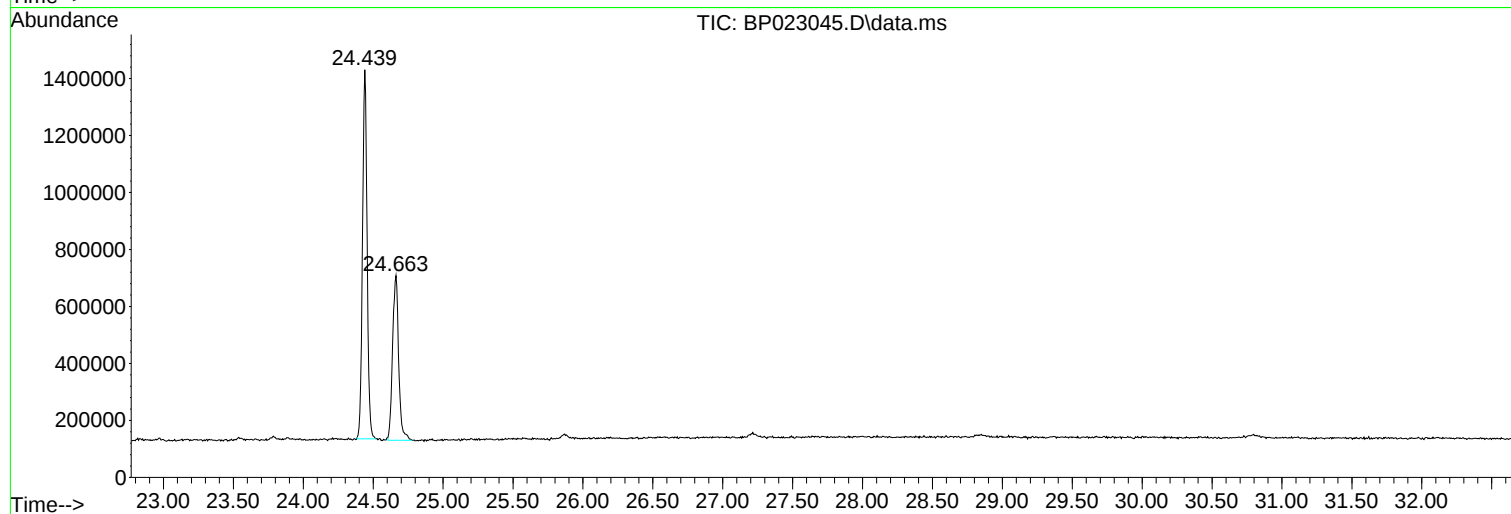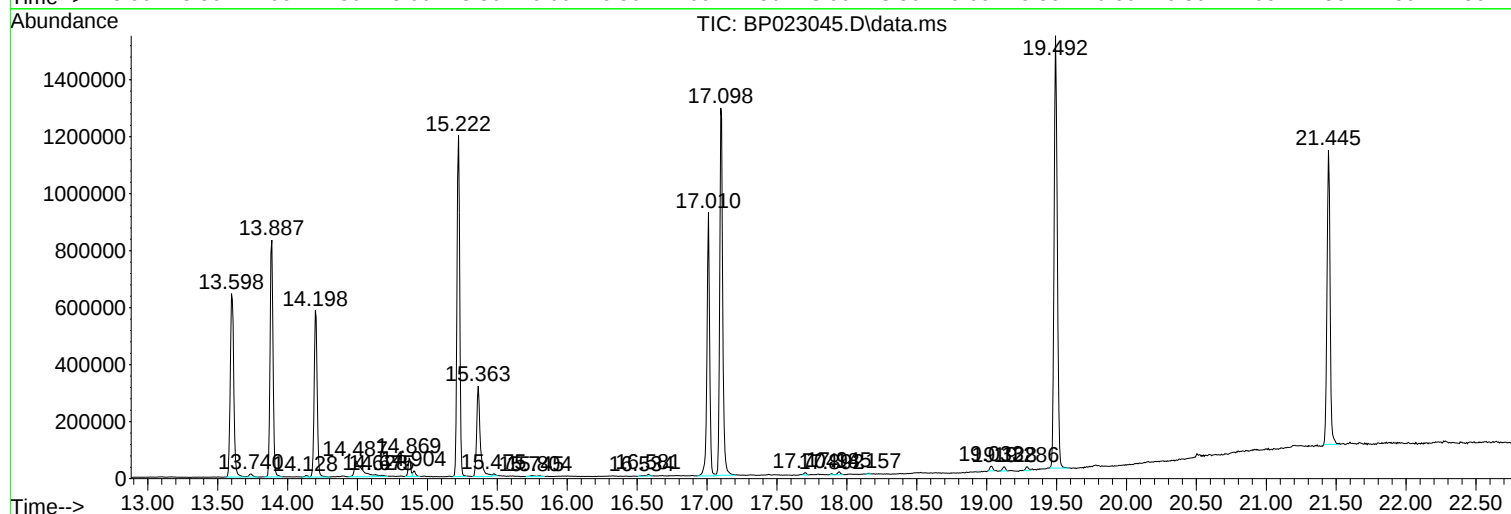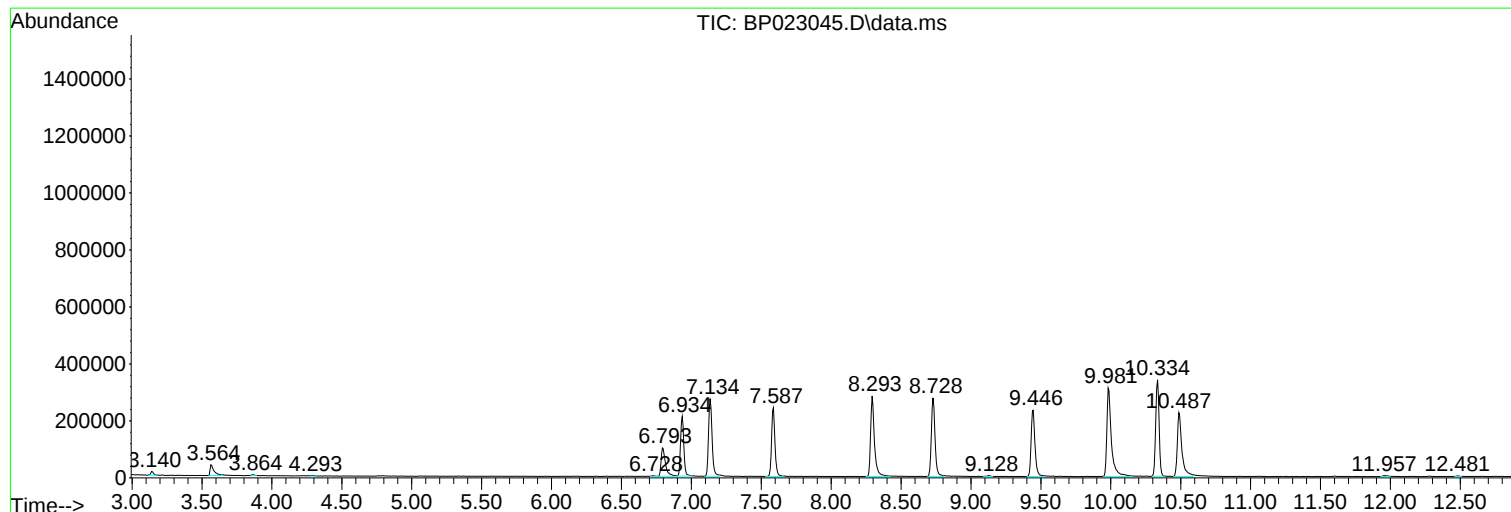

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023045.D
Acq On : 12 Nov 2024 13:52
Operator : RC/JU
Sample : P4741-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27L8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023045.D
Acq On : 12 Nov 2024 13:52
Operator : RC/JU
Sample : P4741-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27L8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------