

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023057.D
 Acq On : 12 Nov 2024 21:59
 Operator : RC/JU
 Sample : P4687-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	23	26	32	rBV	8965	12494	0.52%	0.070%
2	3.387	65	68	74	rVB8	2268	3867	0.16%	0.022%
3	3.563	95	98	113	rBV	45071	86720	3.62%	0.487%
4	3.863	145	149	154	rVB2	7396	10895	0.45%	0.061%
5	4.381	231	237	243	rBV9	3191	5463	0.23%	0.031%
6	5.157	364	369	373	rVV7	1496	2475	0.10%	0.014%
7	5.287	386	391	396	rBV6	3049	5706	0.24%	0.032%
8	5.646	446	452	460	rBV4	3678	6568	0.27%	0.037%
9	6.693	625	630	634	rBV7	3958	8855	0.37%	0.050%
10	6.728	634	636	640	rVV4	1890	2487	0.10%	0.014%
11	6.804	644	649	661	rBV	33999	80691	3.37%	0.453%
12	6.934	666	671	686	rVB	140064	223272	9.31%	1.253%
13	7.134	698	705	720	rBV	158462	284957	11.89%	1.599%
14	7.587	774	782	790	rBV	223937	370038	15.43%	2.076%
15	7.657	790	794	802	rVB2	9118	18294	0.76%	0.103%
16	8.298	896	903	922	rVV	121453	254292	10.61%	1.427%
17	8.728	969	976	993	rVV	179253	327032	13.64%	1.835%
18	8.869	994	1000	1011	rVB5	6445	16130	0.67%	0.090%
19	9.439	1090	1097	1113	rBV	154327	283730	11.83%	1.592%
20	9.745	1142	1149	1156	rBV	3561	8639	0.36%	0.048%
21	9.986	1181	1190	1210	rBV2	182895	444808	18.55%	2.496%
22	10.334	1241	1249	1256	rBV	286228	506713	21.13%	2.843%
23	10.381	1256	1257	1264	rVB3	6652	9191	0.38%	0.052%
24	10.486	1267	1275	1296	rBV	187737	396029	16.52%	2.222%
25	11.010	1359	1364	1374	rVV2	8805	22641	0.94%	0.127%
26	11.610	1459	1466	1474	rBV6	3196	8130	0.34%	0.046%
27	11.933	1516	1521	1528	rVB5	3533	6201	0.26%	0.035%
28	12.010	1528	1534	1544	rBV6	3455	7672	0.32%	0.043%
29	12.233	1568	1572	1580	rVB8	3267	6145	0.26%	0.034%
30	13.527	1784	1792	1796	rBV8	2080	4428	0.18%	0.025%
31	13.622	1796	1808	1820	rBV	495686	768849	32.07%	4.314%
32	13.898	1844	1855	1870	rBV	399856	753583	31.43%	4.228%
33	14.204	1899	1907	1918	rBV	456073	776151	32.37%	4.355%
34	14.439	1940	1947	1954	rVB5	7396	14295	0.60%	0.080%
35	14.522	1954	1961	1968	rBV4	17883	53924	2.25%	0.303%
36	14.986	2036	2040	2043	rBV6	1714	2995	0.12%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023057.D
 Acq On : 12 Nov 2024 21:59
 Operator : RC/JU
 Sample : P4687-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

37	15.057	2049	2052	2058	rVB6	3422	5672	0.24%	0.032%
38	15.204	2067	2077	2094	rBV	732904	1115835	46.54%	6.261%
39	15.374	2098	2106	2116	rBV	198278	404659	16.88%	2.270%
40	15.445	2116	2118	2130	rVB3	15944	33327	1.39%	0.187%
41	15.586	2136	2142	2149	rBV	89692	127039	5.30%	0.713%
42	15.816	2175	2181	2183	rBV7	1434	2517	0.10%	0.014%
43	15.974	2206	2208	2212	rVB5	2211	2664	0.11%	0.015%
44	16.168	2236	2241	2247	rBV2	14587	21456	0.89%	0.120%
45	16.416	2278	2283	2284	rBV5	4267	5480	0.23%	0.031%
46	16.998	2376	2382	2393	rBV	721342	1080650	45.07%	6.063%
47	17.110	2393	2401	2414	rVV	883323	1459113	60.86%	8.187%
48	17.386	2443	2448	2452	rBV2	10283	18456	0.77%	0.104%
49	17.810	2517	2520	2523	rVB5	3699	4702	0.20%	0.026%
50	17.939	2538	2542	2548	rBV3	48245	69450	2.90%	0.390%
51	18.245	2590	2594	2597	rBV5	5420	9420	0.39%	0.053%
52	18.351	2608	2612	2616	rBV2	8538	16249	0.68%	0.091%
53	18.815	2687	2691	2695	rVB3	10929	16553	0.69%	0.093%
54	19.045	2726	2730	2735	rBV4	15098	19697	0.82%	0.111%
55	19.115	2740	2742	2746	rVB	12117	15295	0.64%	0.086%
56	19.274	2765	2769	2776	rVB7	18616	28479	1.19%	0.160%
57	19.380	2782	2787	2794	rBV2	27071	56957	2.38%	0.320%
58	19.492	2800	2806	2816	rBV	1492832	1995241	83.22%	11.195%
59	21.439	3131	3137	3149	rBV2	914656	1471305	61.37%	8.255%
60	24.433	3636	3646	3658	rVB	941769	2397600	100.00%	13.452%
61	24.662	3676	3685	3702	rVB	632728	1651214	68.87%	9.264%




Sum of corrected areas: 17823390

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023057.D
Acq On : 12 Nov 2024 21:59
Operator : RC/JU
Sample : P4687-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

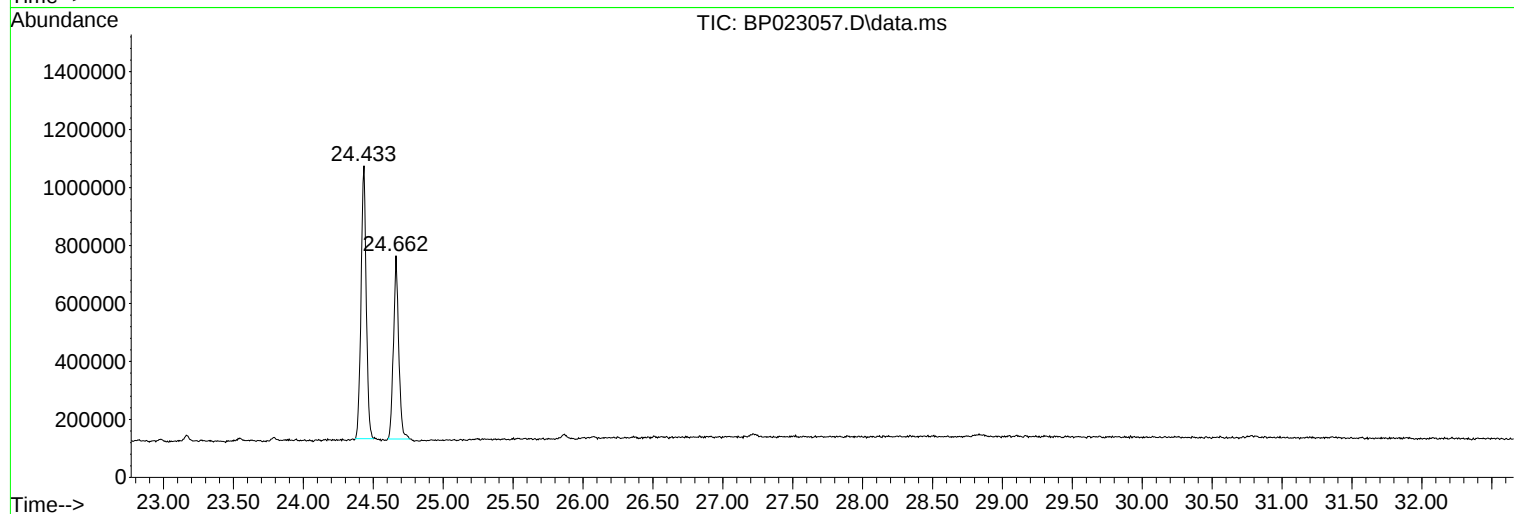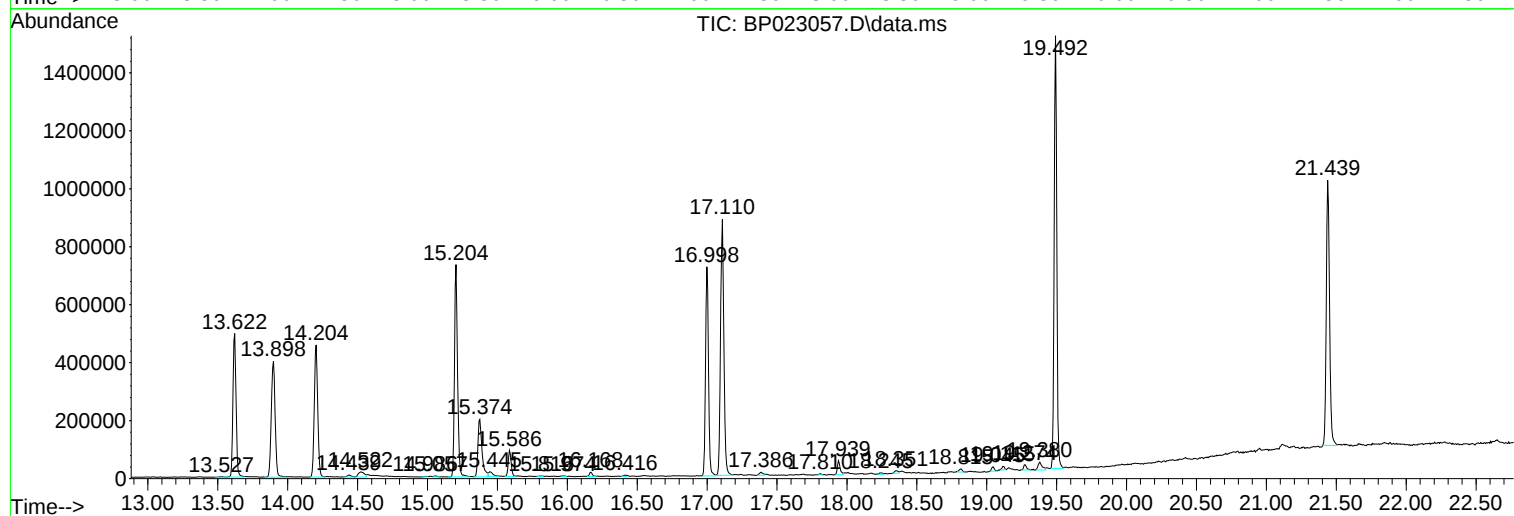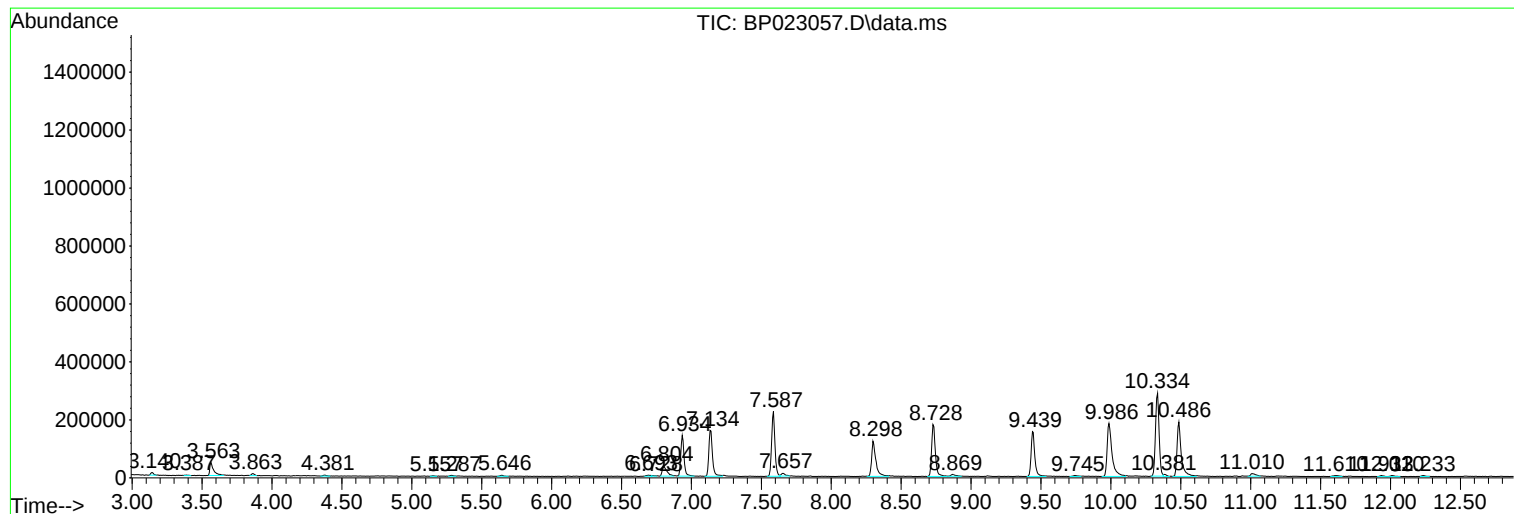

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023057.D
Acq On : 12 Nov 2024 21:59
Operator : RC/JU
Sample : P4687-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CG4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.586	3.27 ng/ul	127039	Acenaphthene-d10	14.204

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	95
3			Benzophenone	182	C13H10O	000119-61-9	95
4			Benzophenone	182	C13H10O	000119-61-9	93
5			Benzophenone	182	C13H10O	000119-61-9	91

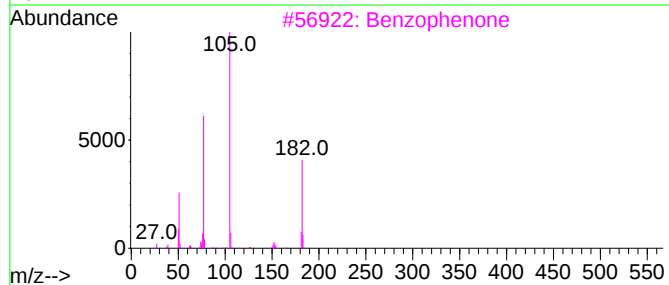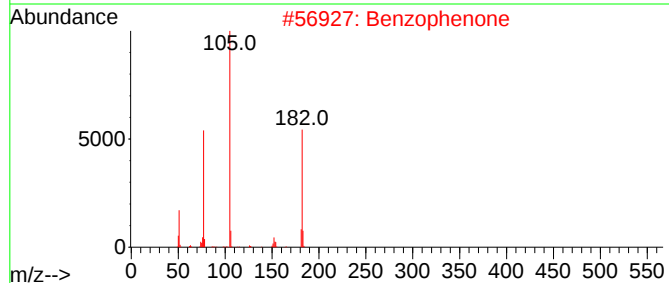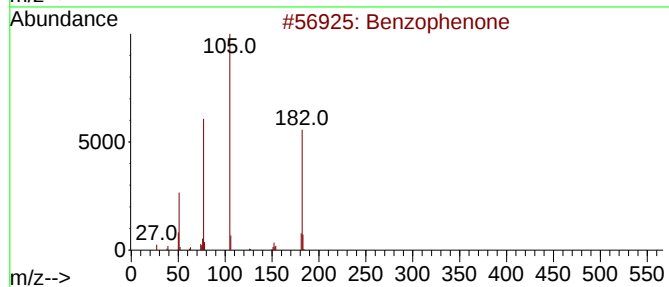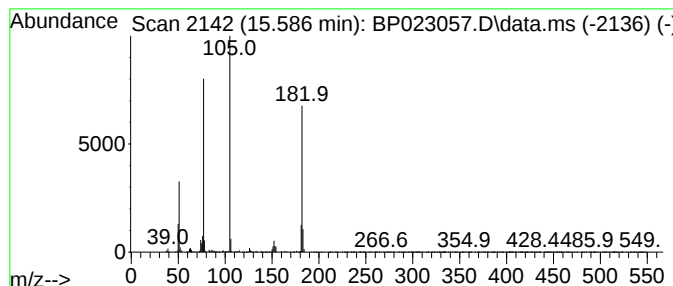

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023057.D
Acq On : 12 Nov 2024 21:59
Operator : RC/JU
Sample : P4687-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.586	3.3	ng/u1	127039	3	14.204	776151	20.0