

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023059.D
 Acq On : 12 Nov 2024 23:20
 Operator : RC/JU
 Sample : P4687-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.575	96	100	111	rBV	19234	42144	0.11%	0.070%
2	4.387	230	238	260	rBV	24060538	37691968	100.00%	62.640%
3	6.804	641	649	666	rBV2	63735	167066	0.44%	0.278%
4	6.940	666	672	681	rVV	200803	313122	0.83%	0.520%
5	7.140	699	706	716	rBV	218194	380043	1.01%	0.632%
6	7.587	775	782	794	rBV	249396	421596	1.12%	0.701%
7	8.298	897	903	923	rBV	204379	411538	1.09%	0.684%
8	8.734	969	977	990	rBV	247115	459694	1.22%	0.764%
9	9.445	1091	1098	1111	rBV	212089	399190	1.06%	0.663%
10	9.986	1181	1190	1204	rBV	258064	600196	1.59%	0.997%
11	10.334	1240	1249	1261	rVB	328940	588420	1.56%	0.978%
12	10.498	1267	1277	1298	rBV	145309	334801	0.89%	0.556%
13	13.616	1799	1807	1821	rBV	727869	1116371	2.96%	1.855%
14	13.886	1842	1853	1866	rBV	633675	1066495	2.83%	1.772%
15	14.192	1896	1905	1918	rBV	534279	918502	2.44%	1.526%
16	15.204	2071	2077	2086	rBV	1135114	1585201	4.21%	2.634%
17	15.369	2098	2105	2119	rBV	332512	601592	1.60%	1.000%
18	15.592	2136	2143	2151	rBV	46861	72123	0.19%	0.120%
19	16.992	2375	2381	2392	rBV	911257	1272150	3.38%	2.114%
20	17.104	2392	2400	2415	rBV2	1259914	2109737	5.60%	3.506%
21	17.939	2537	2542	2548	rBV3	34616	54078	0.14%	0.090%
22	19.033	2724	2728	2734	rBV3	20537	38068	0.10%	0.063%
23	19.486	2799	2805	2814	rBV	2224596	2767739	7.34%	4.600%
24	21.439	3131	3137	3149	rVB2	1003992	1658493	4.40%	2.756%
25	24.427	3635	3645	3662	rVB	1319466	3247877	8.62%	5.398%
26	24.650	3674	3683	3706	rVB	666971	1853684	4.92%	3.081%




Sum of corrected areas: 60171888

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023059.D
Acq On : 12 Nov 2024 23:20
Operator : RC/JU
Sample : P4687-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

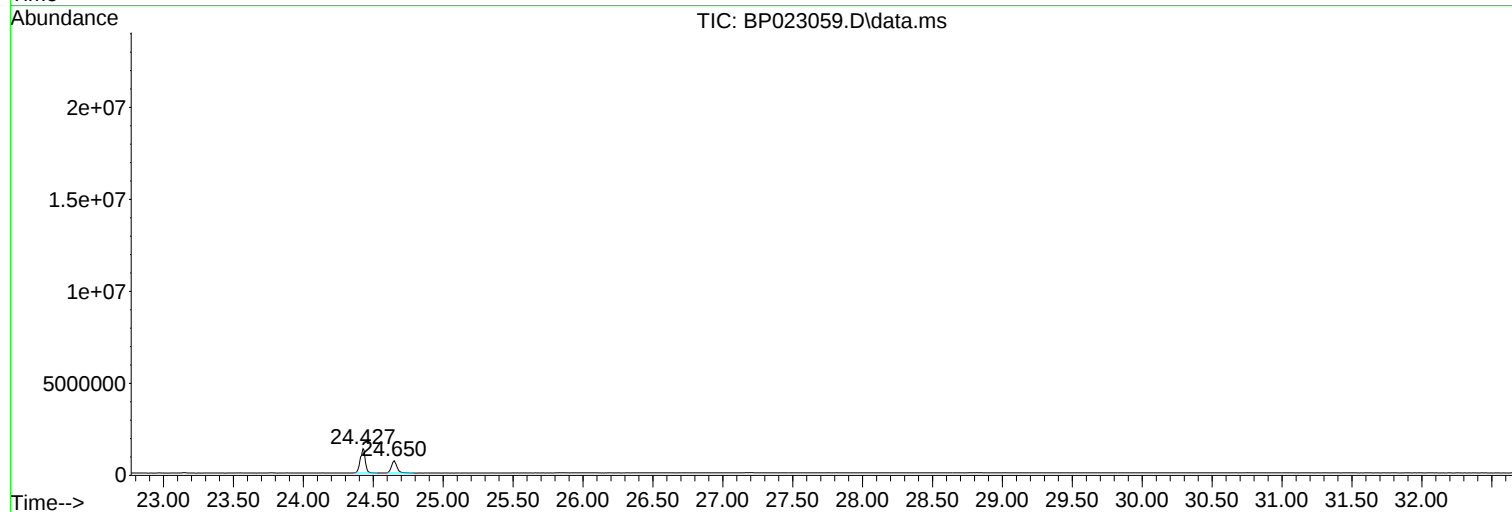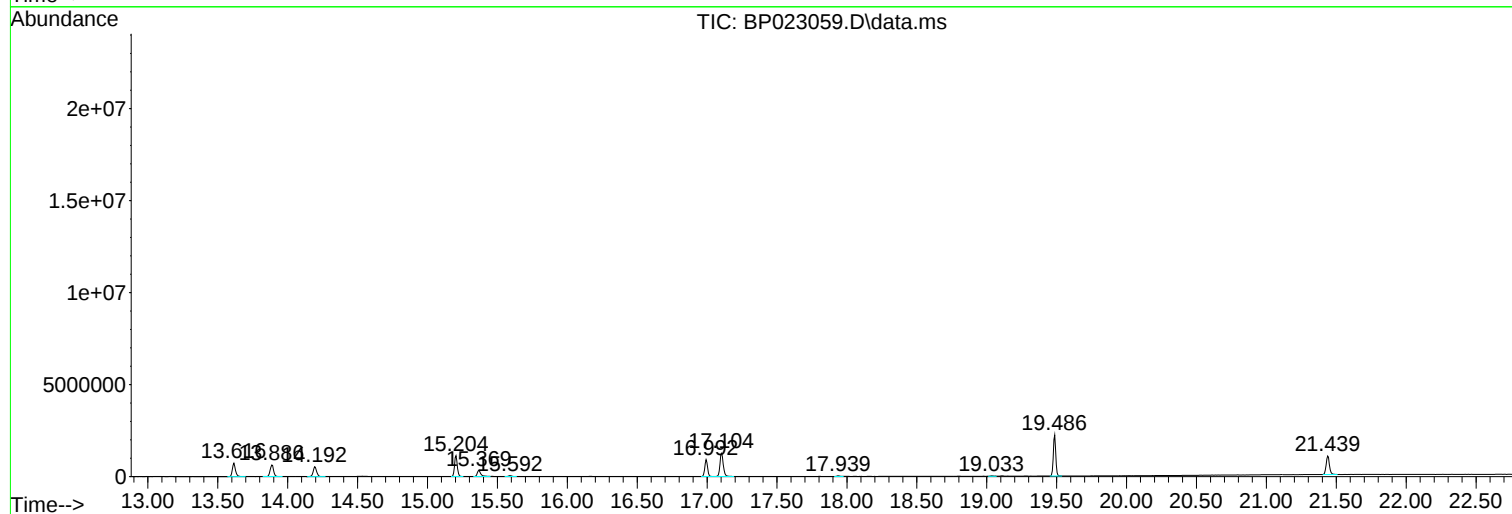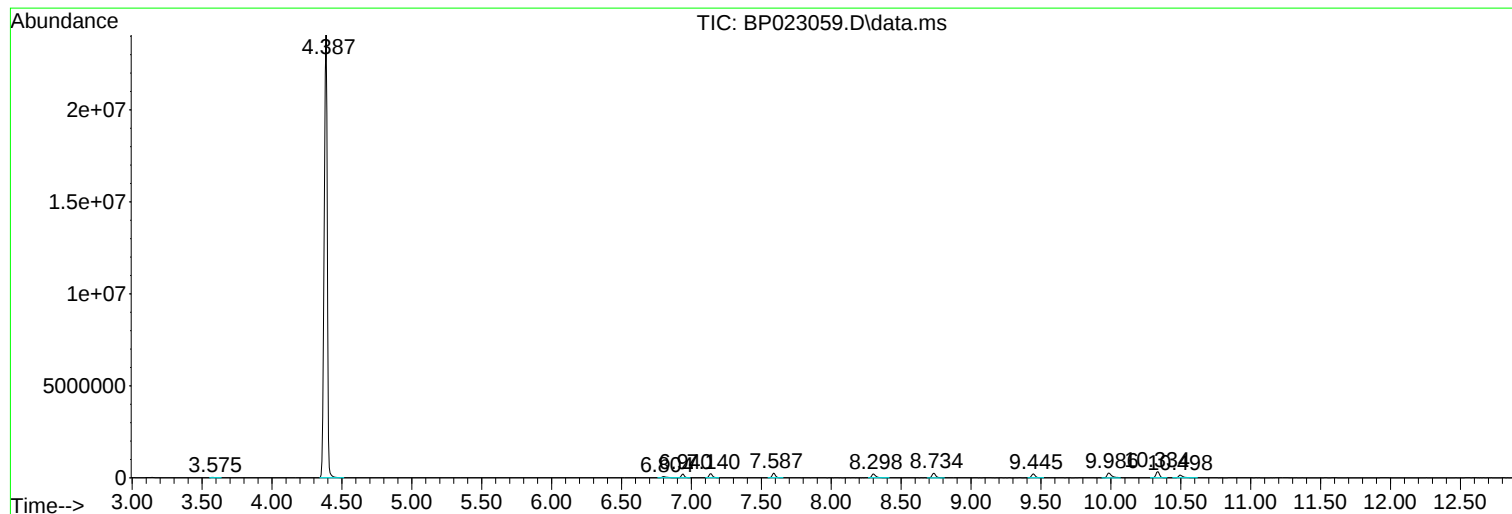

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023059.D
Acq On : 12 Nov 2024 23:20
Operator : RC/JU
Sample : P4687-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.387	1788.06 ng/ul	37692000	1,4-Dichlorobenzene-d4	7.592

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	43

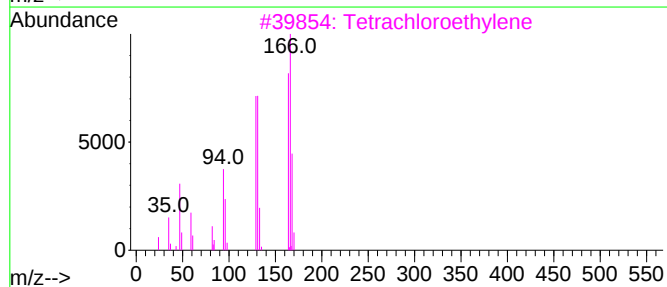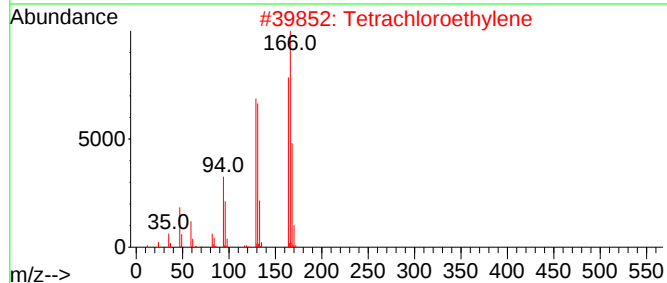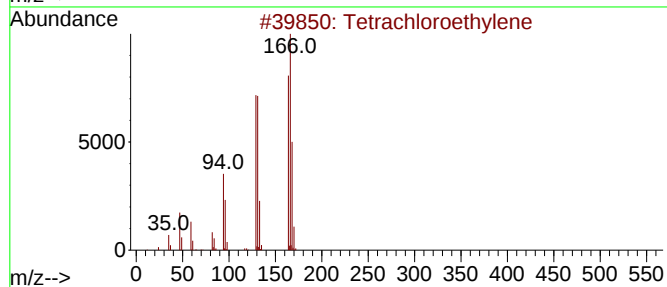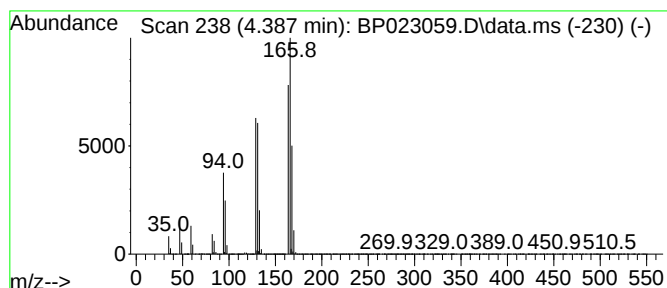

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023059.D
Acq On : 12 Nov 2024 23:20
Operator : RC/JU
Sample : P4687-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.387	1788.1	ng/ul	37692000	1	7.592	421596	20.0