

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023060.D
 Acq On : 13 Nov 2024 00:00
 Operator : RC/JU
 Sample : P4687-20
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	31	rVB	14160	17405	0.57%	0.074%
2	3.563	95	98	114	rBV	42351	78914	2.61%	0.338%
3	3.863	144	149	153	rBV4	3755	5667	0.19%	0.024%
4	4.375	231	236	241	rBV3	16384	25428	0.84%	0.109%
5	6.798	641	648	664	rBV	52590	126899	4.19%	0.543%
6	6.934	665	671	683	rVV	199089	306888	10.14%	1.313%
7	7.134	698	705	715	rBV	225012	392188	12.95%	1.678%
8	7.587	775	782	796	rBV	288347	465182	15.36%	1.991%
9	8.298	896	903	920	rBV	201269	377074	12.45%	1.614%
10	8.728	968	976	991	rBV	250630	463647	15.31%	1.984%
11	9.122	1039	1043	1047	rVB6	3268	5103	0.17%	0.022%
12	9.439	1089	1097	1113	rBV	220259	413317	13.65%	1.769%
13	9.981	1182	1189	1209	rBV	257658	629745	20.80%	2.695%
14	10.334	1241	1249	1264	rVB	363042	649311	21.45%	2.779%
15	10.486	1268	1275	1297	rBV	238947	524292	17.32%	2.244%
16	11.957	1518	1525	1534	rBV5	3938	9535	0.31%	0.041%
17	13.610	1797	1806	1819	rBV	654487	1175525	38.83%	5.031%
18	13.880	1845	1852	1867	rBV	768586	1147638	37.90%	4.911%
19	14.198	1899	1906	1916	rBV	678347	1002832	33.12%	4.292%
20	14.516	1949	1960	1971	rBV5	27757	102732	3.39%	0.440%
21	14.622	1976	1978	1984	rVV7	5178	9721	0.32%	0.042%
22	14.686	1987	1989	1994	rVB6	2774	3856	0.13%	0.017%
23	15.210	2072	2078	2089	rBV	1249260	1704396	56.29%	7.294%
24	15.280	2089	2090	2098	rVB7	4078	6182	0.20%	0.026%
25	15.369	2098	2105	2120	rBV	293294	602991	19.92%	2.580%
26	15.469	2120	2122	2128	rVB5	8212	11033	0.36%	0.047%
27	15.586	2136	2142	2151	rVB	56164	74626	2.46%	0.319%
28	16.998	2376	2382	2392	rBV	1138834	1403206	46.35%	6.005%
29	17.104	2392	2400	2418	rVV2	1196665	2127405	70.26%	9.104%
30	17.392	2444	2449	2453	rBV8	3587	6498	0.21%	0.028%
31	17.510	2465	2469	2477	rVB3	5931	11132	0.37%	0.048%
32	17.692	2498	2500	2507	rVB8	3993	6060	0.20%	0.026%
33	17.939	2537	2542	2551	rBV2	27973	51792	1.71%	0.222%
34	18.157	2576	2579	2585	rVB6	2955	4730	0.16%	0.020%
35	18.480	2627	2634	2637	rBV9	3362	7793	0.26%	0.033%
36	19.039	2725	2729	2738	rBV2	17105	30227	1.00%	0.129%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023060.D
Acq On : 13 Nov 2024 00:00
Operator : RC/JU
Sample : P4687-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CD6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	19.121	2738	2743	2747	rBV3	17596	27340	0.90%	0.117%
38	19.268	2765	2768	2771	rBV4	11432	13778	0.46%	0.059%
39	19.386	2783	2788	2790	rBV5	6322	11649	0.38%	0.050%
40	19.492	2799	2806	2818	rBV	1701164	2677770	88.44%	11.459%
41	21.439	3131	3137	3148	rBV2	1022319	1774739	58.62%	7.595%
42	24.433	3636	3646	3663	rVB	1270285	3027723	100.00%	12.957%
43	24.656	3675	3684	3697	rBV	693516	1853549	61.22%	7.932%




Sum of corrected areas: 23367518

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023060.D
Acq On : 13 Nov 2024 00:00
Operator : RC/JU
Sample : P4687-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

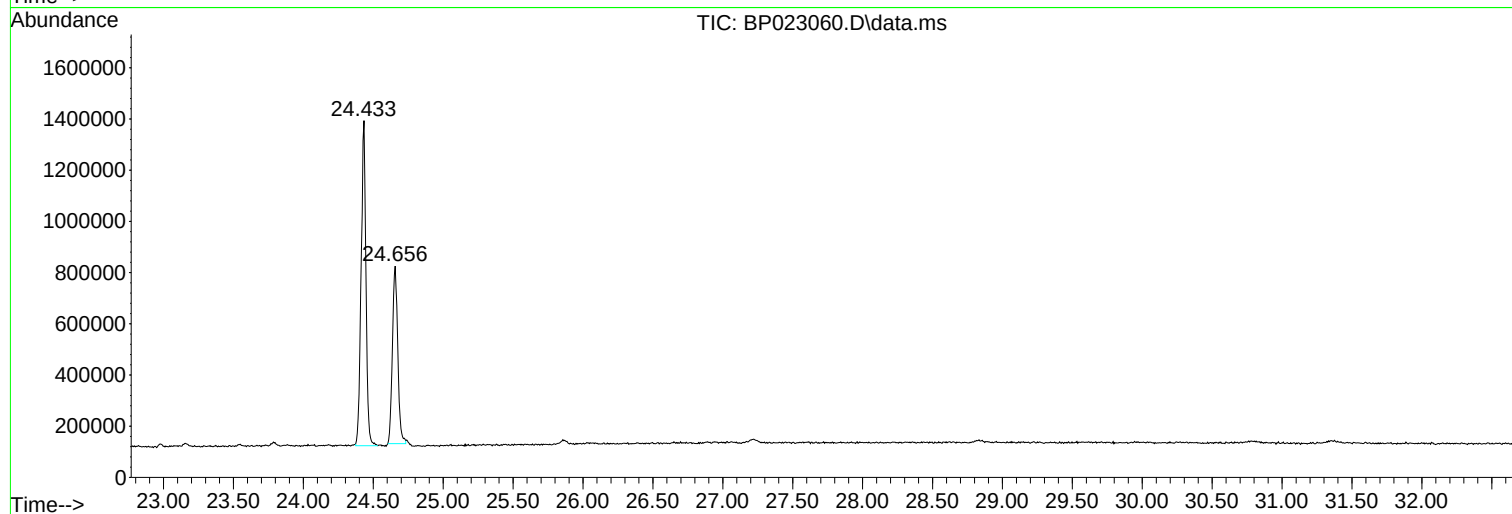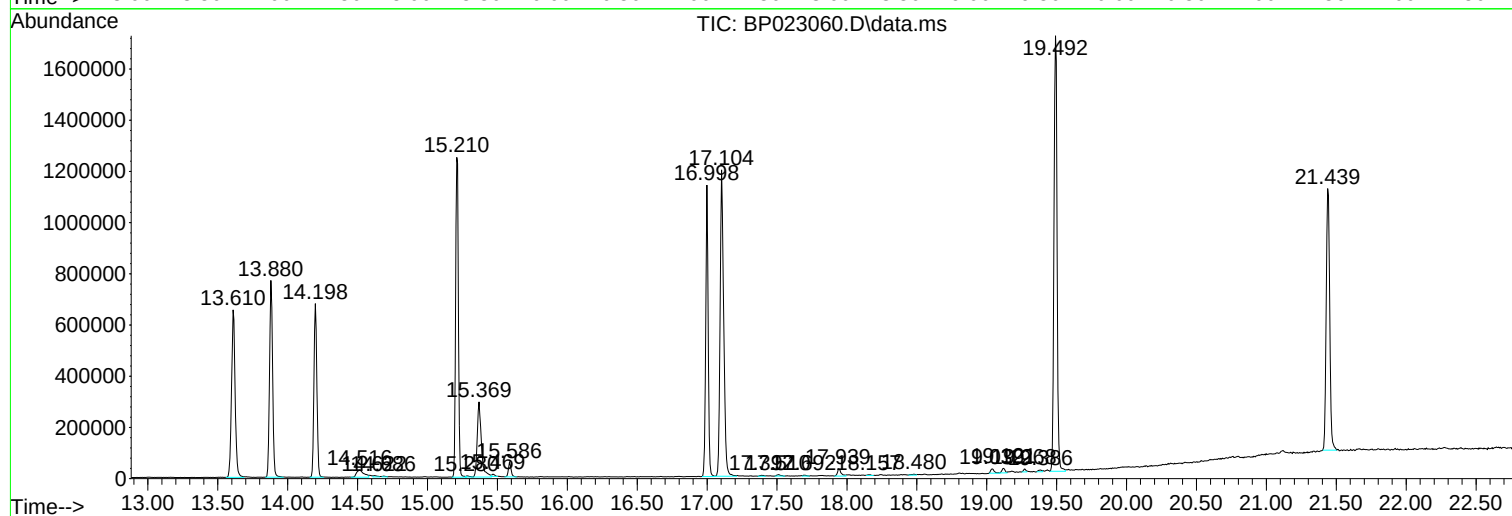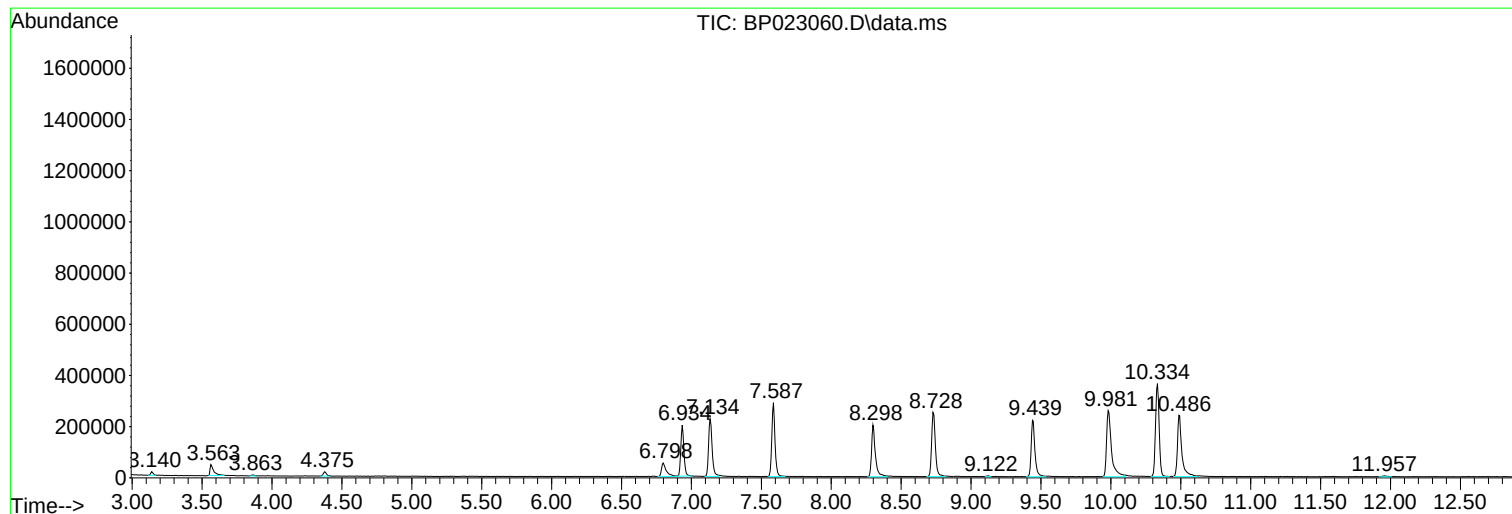

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023060.D
Acq On : 13 Nov 2024 00:00
Operator : RC/JU
Sample : P4687-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023060.D
Acq On : 13 Nov 2024 00:00
Operator : RC/JU
Sample : P4687-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------