

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023061.D
 Acq On : 13 Nov 2024 00:41
 Operator : RC/JU
 Sample : P4687-17
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	34	rVB	15331	20398	0.70%	0.097%
2	3.575	98	100	114	rBV	14187	32891	1.13%	0.156%
3	3.864	145	149	153	rBV3	2672	3576	0.12%	0.017%
4	4.375	231	236	245	rVB6	6440	9666	0.33%	0.046%
5	6.799	642	648	665	rBV	49997	124518	4.27%	0.589%
6	6.934	666	671	686	rVB	208784	303203	10.41%	1.435%
7	7.134	698	705	716	rBV	211892	388047	13.32%	1.836%
8	7.587	774	782	792	rBV	239857	387018	13.28%	1.832%
9	7.657	792	794	805	rVB	2967	5889	0.20%	0.028%
10	8.305	894	904	921	rBV	190219	361341	12.40%	1.710%
11	8.728	970	976	991	rBV	278245	453325	15.56%	2.145%
12	9.116	1036	1042	1047	rBV7	3150	5705	0.20%	0.027%
13	9.316	1074	1076	1083	rBV7	1577	2952	0.10%	0.014%
14	9.440	1090	1097	1114	rBV	229660	403734	13.86%	1.911%
15	9.981	1181	1189	1211	rBV	236534	608963	20.90%	2.882%
16	10.340	1241	1250	1259	rBV	335185	541769	18.59%	2.564%
17	10.499	1269	1277	1302	rBV	97844	248366	8.52%	1.175%
18	11.963	1520	1526	1530	rBV4	2773	5811	0.20%	0.028%
19	13.610	1800	1806	1820	rBV	906689	1080279	37.07%	5.113%
20	13.898	1848	1855	1869	rBV	731949	1064110	36.52%	5.036%
21	14.204	1897	1907	1917	rBV	531260	824799	28.30%	3.903%
22	14.510	1954	1959	1964	rBV4	25065	56154	1.93%	0.266%
23	15.204	2070	2077	2091	rBV	858852	1535014	52.68%	7.265%
24	15.298	2091	2093	2099	rVV7	3561	5379	0.18%	0.025%
25	15.375	2099	2106	2117	rVV	332190	553328	18.99%	2.619%
26	15.457	2117	2120	2126	rVB5	8154	13753	0.47%	0.065%
27	15.598	2137	2144	2152	rBV	125007	183357	6.29%	0.868%
28	16.128	2229	2234	2237	rBV7	2417	3185	0.11%	0.015%
29	16.539	2299	2304	2306	rBV5	2450	4825	0.17%	0.023%
30	16.798	2344	2348	2353	rVB6	2247	3656	0.13%	0.017%
31	17.004	2376	2383	2395	rBV	661871	1142028	39.19%	5.405%
32	17.116	2395	2402	2415	rBV	1345020	1941764	66.64%	9.190%
33	17.304	2432	2434	2443	rVB7	3298	5491	0.19%	0.026%
34	17.392	2445	2449	2451	rBV3	3491	4678	0.16%	0.022%
35	17.698	2496	2501	2507	rVB9	4693	8811	0.30%	0.042%
36	17.939	2537	2542	2549	rBV2	49118	79720	2.74%	0.377%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023061.D
Acq On : 13 Nov 2024 00:41
Operator : RC/JU
Sample : P4687-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CD4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	18.157	2575	2579	2584	rBV2	9804	14809	0.51%	0.070%
38	18.233	2589	2592	2600	rVB9	4216	6495	0.22%	0.031%
39	18.392	2615	2619	2621	rBV4	3125	3875	0.13%	0.018%
40	19.033	2724	2728	2735	rBV2	16237	24382	0.84%	0.115%
41	19.122	2737	2743	2746	rBV2	15915	28851	0.99%	0.137%
42	19.275	2765	2769	2774	rBV7	21608	32797	1.13%	0.155%
43	19.492	2799	2806	2819	rBV	1593813	2487217	85.35%	11.771%
44	21.433	3131	3136	3147	rBV	961738	1508373	51.76%	7.139%
45	24.433	3636	3646	3661	rVB	1074995	2913976	100.00%	13.791%
46	24.645	3674	3682	3704	rVB	629245	1691655	58.05%	8.006%




Sum of corrected areas: 21129933

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023061.D
Acq On : 13 Nov 2024 00:41
Operator : RC/JU
Sample : P4687-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

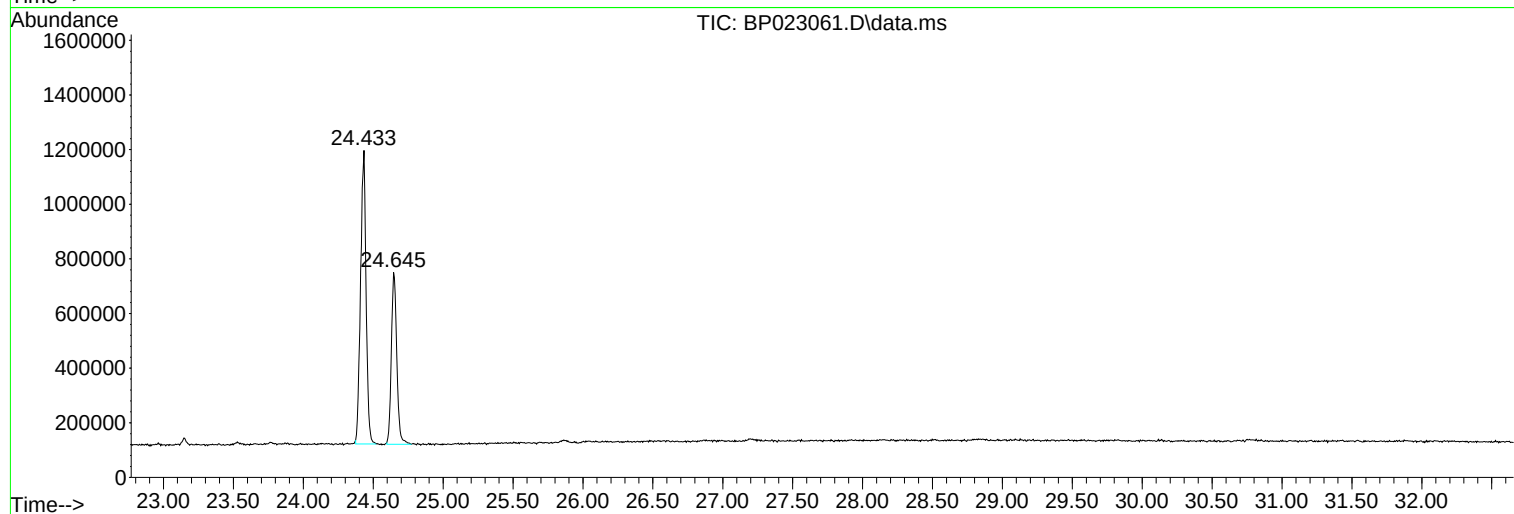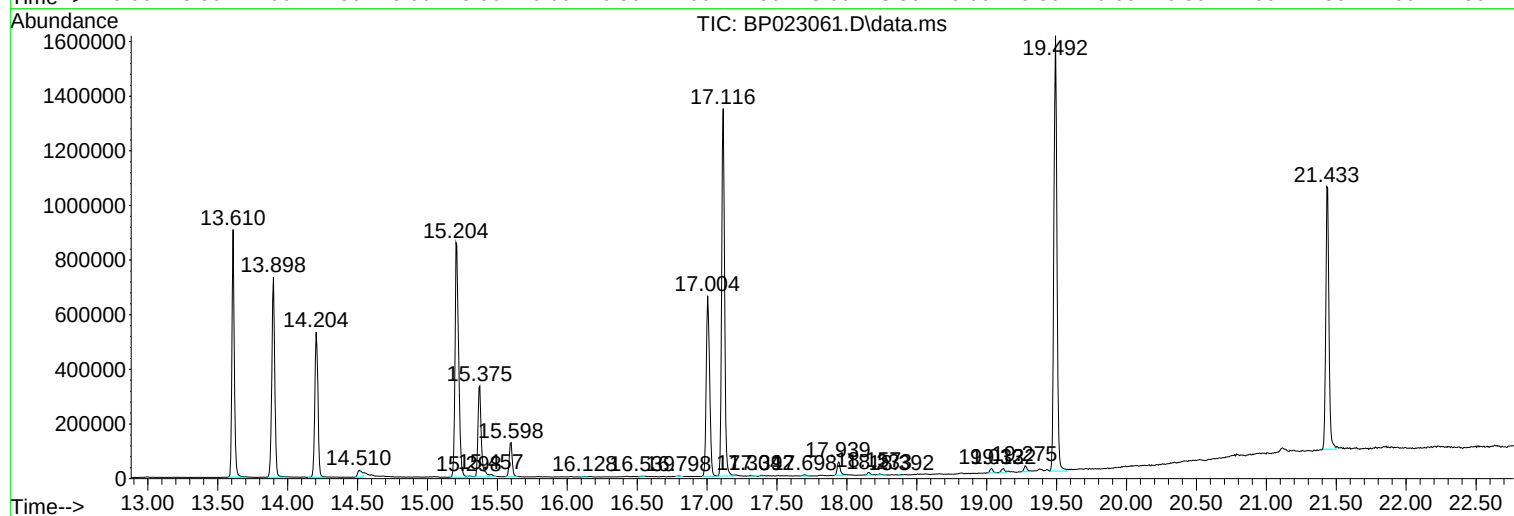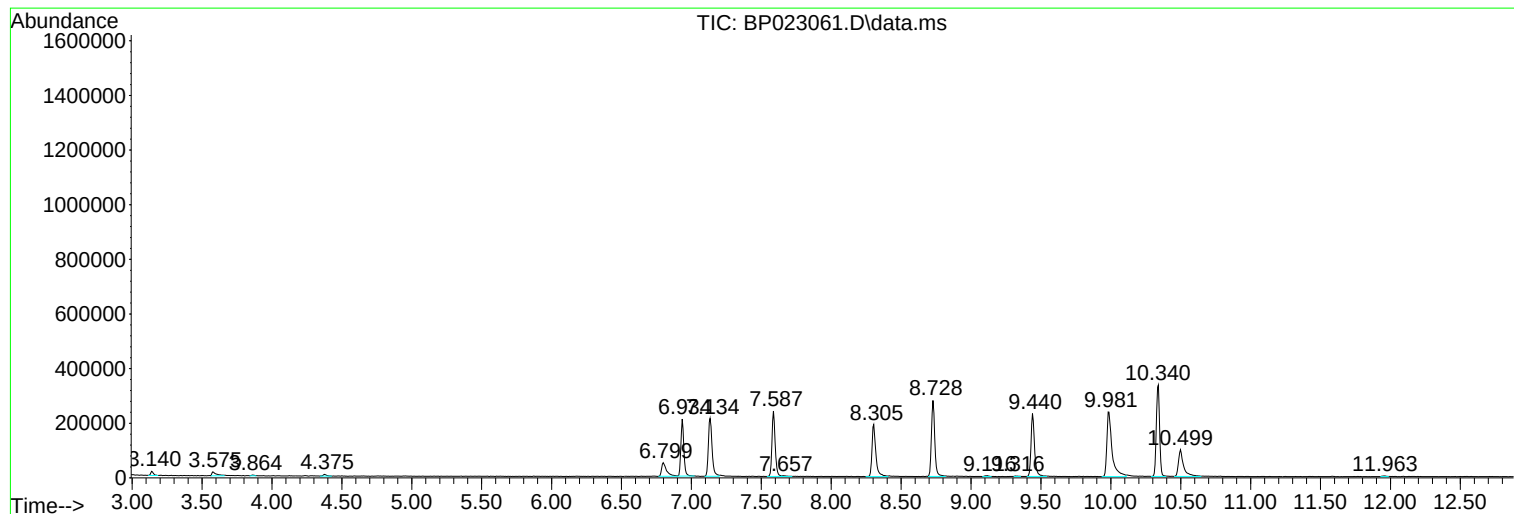

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023061.D
Acq On : 13 Nov 2024 00:41
Operator : RC/JU
Sample : P4687-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CD4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.598	4.45 ng/ul	183357	Acenaphthene-d10	14.204

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	97
3			Benzophenone	182	C13H10O	000119-61-9	96
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	87

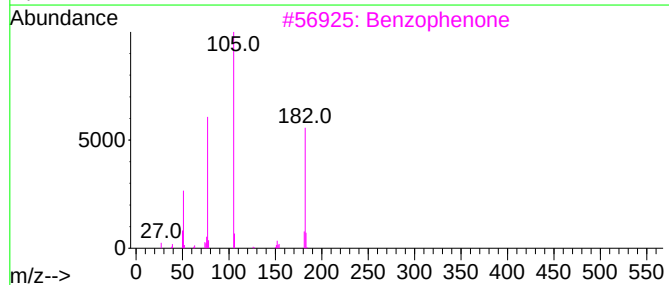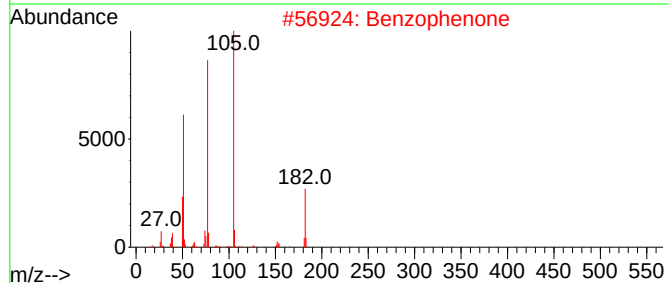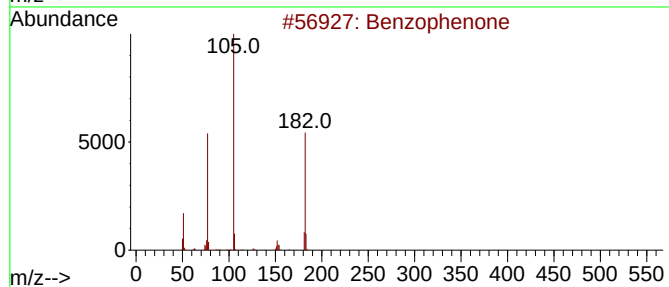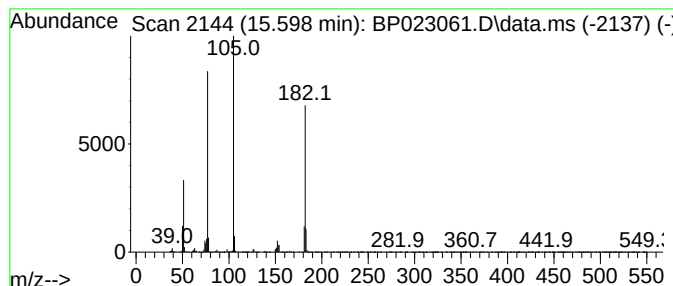

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023061.D
Acq On : 13 Nov 2024 00:41
Operator : RC/JU
Sample : P4687-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CD4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.598	4.5	ng/u1	183357	3	14.204	824799	20.0