

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023068.D
 Acq On : 13 Nov 2024 06:04
 Operator : RC/JU
 Sample : P4687-22
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023068.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	31	rBV	16463	20568	0.44%	0.076%
2	3.563	95	98	113	rBV	46150	92844	2.00%	0.344%
3	4.375	230	236	254	rBV	3322092	4640853	100.00%	17.218%
4	6.793	641	647	665	rBV	115025	237166	5.11%	0.880%
5	6.934	665	671	686	rVB	215135	329240	7.09%	1.222%
6	7.134	698	705	724	rBV	255738	457707	9.86%	1.698%
7	7.587	775	782	796	rBV	230502	377047	8.12%	1.399%
8	8.299	897	903	920	rBV	256274	504457	10.87%	1.872%
9	8.734	969	977	997	rBV	263123	486076	10.47%	1.803%
10	9.446	1090	1098	1113	rBV	231478	438535	9.45%	1.627%
11	9.987	1183	1190	1223	rBV	295344	658515	14.19%	2.443%
12	10.340	1241	1250	1261	rBV	296769	527933	11.38%	1.959%
13	10.493	1268	1276	1293	rBV	194642	463268	9.98%	1.719%
14	11.969	1518	1527	1532	rBV5	4176	9037	0.19%	0.034%
15	13.604	1798	1805	1825	rBV	645198	1129478	24.34%	4.191%
16	13.886	1846	1853	1865	rBV	798583	1163399	25.07%	4.316%
17	14.198	1900	1906	1914	rBV	601649	822371	17.72%	3.051%
18	14.481	1949	1954	1970	rBV	64553	217413	4.68%	0.807%
19	14.669	1983	1986	1997	rVB	3988	9457	0.20%	0.035%
20	15.216	2073	2079	2095	rBV	1168676	1622377	34.96%	6.019%
21	15.357	2097	2103	2117	rBV	312502	559531	12.06%	2.076%
22	15.586	2137	2142	2151	rBV	22122	32899	0.71%	0.122%
23	16.169	2236	2241	2246	rVB5	4435	7672	0.17%	0.028%
24	17.004	2376	2383	2392	rBV	792372	1155879	24.91%	4.289%
25	17.098	2393	2399	2415	rVV	1274013	1990053	42.88%	7.383%
26	17.945	2538	2543	2548	rBV4	16205	25913	0.56%	0.096%
27	18.151	2574	2578	2583	rBV2	9463	16279	0.35%	0.060%
28	19.039	2724	2729	2736	rBV4	14820	25358	0.55%	0.094%
29	19.121	2739	2743	2747	rBV	18297	25141	0.54%	0.093%
30	19.280	2767	2770	2777	rBV6	11546	18114	0.39%	0.067%
31	19.492	2800	2806	2820	rBV	1798958	2600360	56.03%	9.648%
32	21.439	3131	3137	3150	rVB	967404	1529792	32.96%	5.676%
33	24.427	3636	3645	3663	rVB	1369745	3048549	65.69%	11.311%
34	24.639	3673	3681	3702	rVB	580863	1709706	36.84%	6.343%

Sum of corrected areas: 26952987




Instrument :
BNA_P
ClientSampleId :
C0CC8

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023068.D
Acq On : 13 Nov 2024 06:04
Operator : RC/JU
Sample : P4687-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

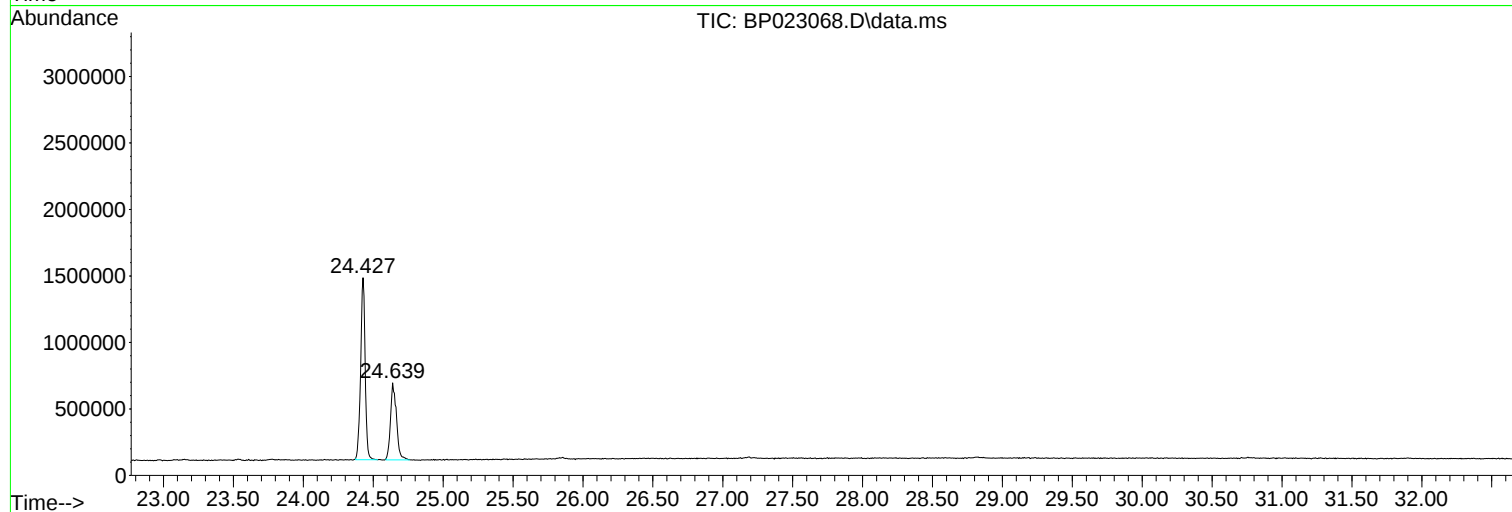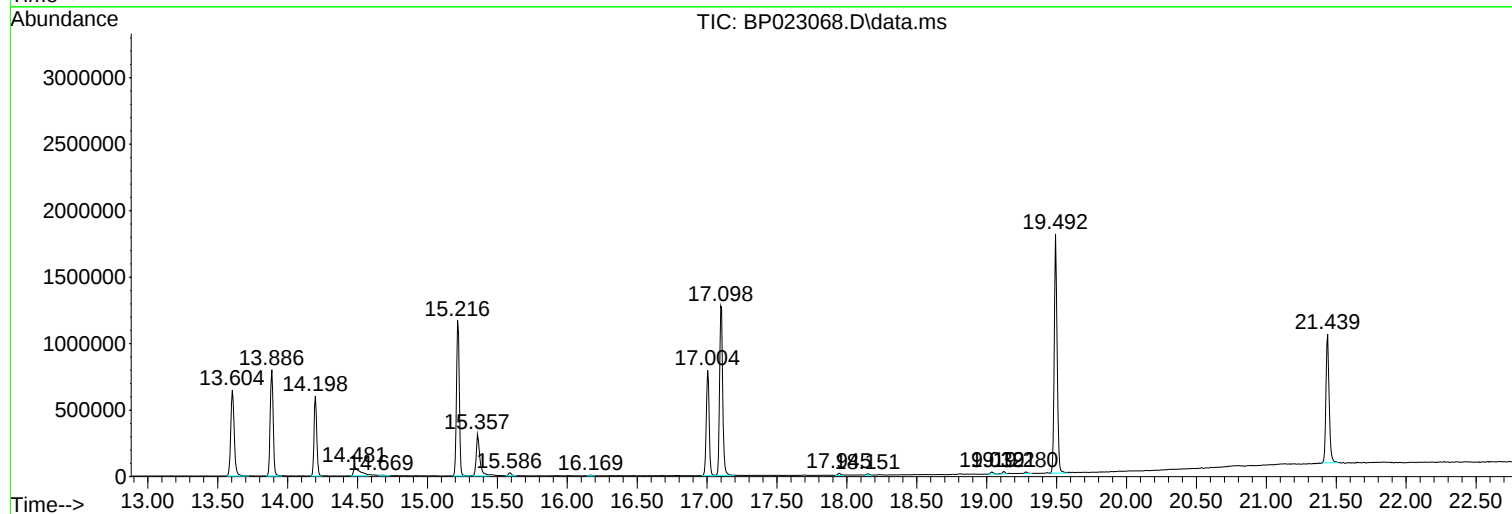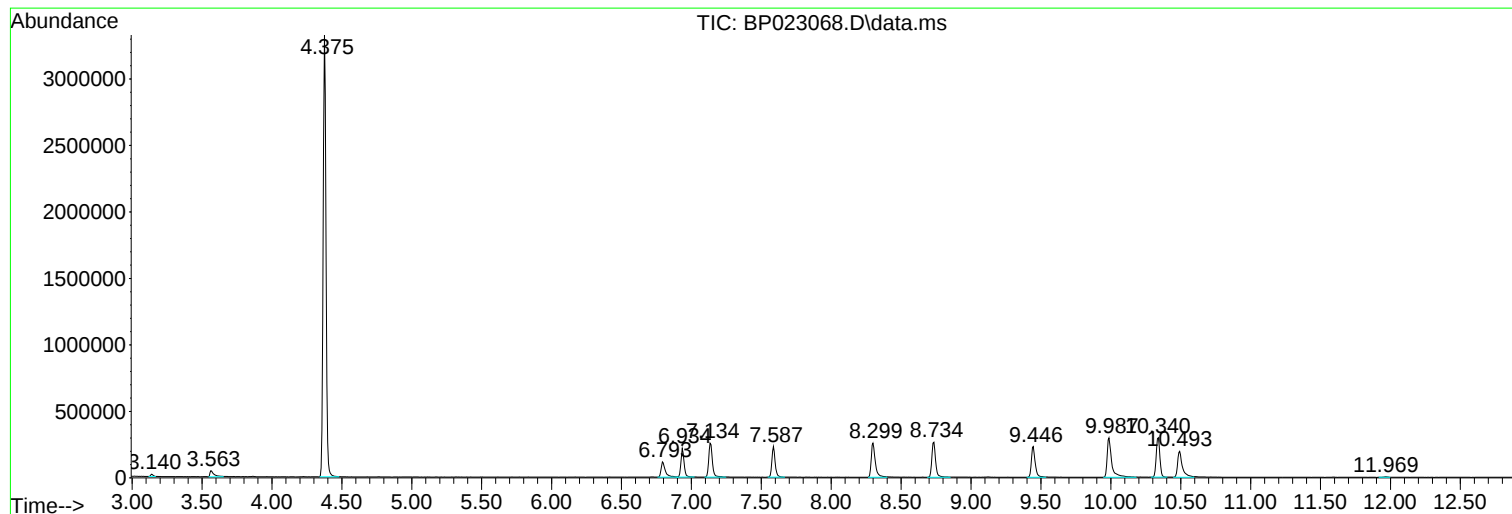

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023068.D
Acq On : 13 Nov 2024 06:04
Operator : RC/JU
Sample : P4687-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.375	246.17 ng/ul	4640850	1,4-Dichlorobenzene-d4	7.587

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	64
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

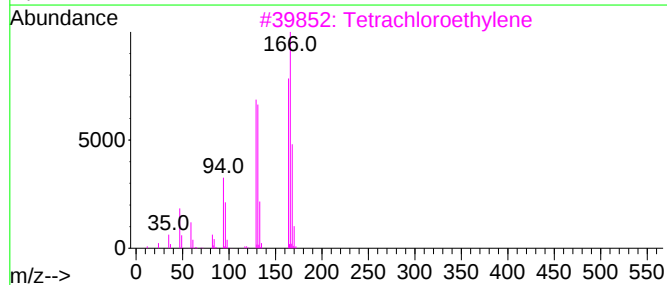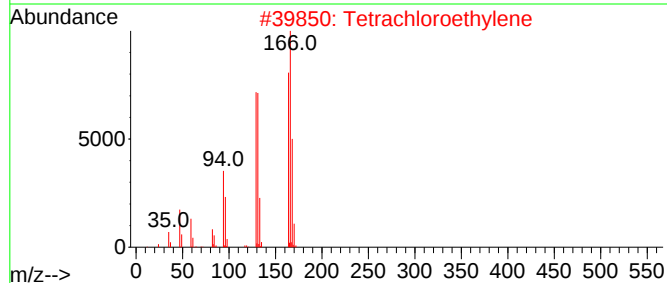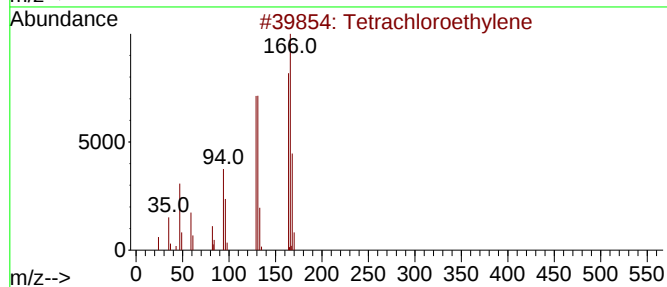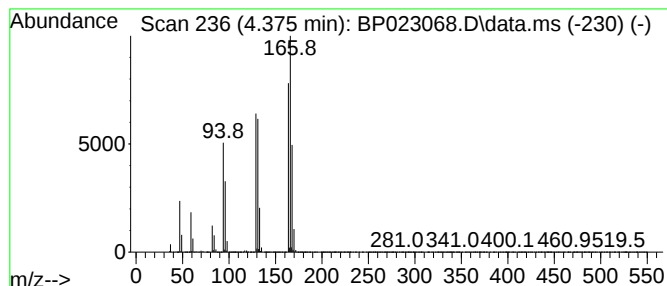

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023068.D
Acq On : 13 Nov 2024 06:04
Operator : RC/JU
Sample : P4687-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.375	246.2	ng/ul	4640850	1	7.587	377047	20.0