

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023071.D
 Acq On : 13 Nov 2024 08:06
 Operator : RC/JU
 Sample : P4687-09
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023071.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	34	rBV	13762	19455	0.67%	0.084%
2	3.564	95	98	110	rBV	45425	85222	2.95%	0.368%
3	3.869	144	150	154	rBV4	3321	5387	0.19%	0.023%
4	6.793	641	647	663	rBV	78862	167553	5.80%	0.724%
5	6.934	665	671	681	rVV	188740	296910	10.28%	1.282%
6	7.134	698	705	715	rBV	223005	396869	13.74%	1.714%
7	7.587	774	782	800	rBV	269389	481284	16.67%	2.079%
8	8.305	897	904	922	rBV	224936	434326	15.04%	1.876%
9	8.728	969	976	991	rBV	245625	428751	14.85%	1.852%
10	8.875	997	1001	1008	rVB9	3407	7811	0.27%	0.034%
11	9.116	1038	1042	1049	rBV10	2920	5521	0.19%	0.024%
12	9.440	1090	1097	1113	rBV	212407	385475	13.35%	1.665%
13	9.987	1183	1190	1213	rBV	274068	590916	20.46%	2.552%
14	10.334	1240	1249	1262	rBV	408418	672521	23.29%	2.904%
15	10.481	1268	1274	1294	rBV	245963	531951	18.42%	2.297%
16	10.887	1337	1343	1348	rBV5	2966	6036	0.21%	0.026%
17	10.951	1348	1354	1358	rBV6	2780	5901	0.20%	0.025%
18	11.193	1388	1395	1403	rBV6	7602	21373	0.74%	0.092%
19	11.940	1518	1522	1529	rVB4	4063	7690	0.27%	0.033%
20	13.045	1704	1710	1713	rBV6	1529	3328	0.12%	0.014%
21	13.087	1715	1717	1725	rVB7	2926	5026	0.17%	0.022%
22	13.610	1798	1806	1816	rBV	911339	1070428	37.07%	4.623%
23	13.898	1844	1855	1868	rBV	700155	1046369	36.24%	4.519%
24	14.204	1899	1907	1919	rBV	700305	1055450	36.55%	4.558%
25	14.504	1954	1958	1959	rBV	20551	22417	0.78%	0.097%
26	14.681	1985	1988	1992	rVB6	4387	6003	0.21%	0.026%
27	15.039	2046	2049	2055	rVB5	4056	5645	0.20%	0.024%
28	15.204	2069	2077	2088	rBV2	727115	1512513	52.38%	6.532%
29	15.292	2088	2092	2098	rVB4	10338	17308	0.60%	0.075%
30	15.369	2098	2105	2115	rBV	329078	548438	18.99%	2.369%
31	15.581	2136	2141	2152	rVB	50113	81802	2.83%	0.353%
32	16.157	2234	2239	2244	rVB	12731	17677	0.61%	0.076%
33	16.404	2278	2281	2287	rVB8	3401	4964	0.17%	0.021%
34	16.675	2322	2327	2332	rBV8	2121	3660	0.13%	0.016%
35	16.786	2336	2346	2351	rBV6	3007	9543	0.33%	0.041%
36	16.992	2373	2381	2393	rBV	870750	1474167	51.05%	6.366%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
 Data File : BP023071.D
 Acq On : 13 Nov 2024 08:06
 Operator : RC/JU
 Sample : P4687-09
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CE4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

37	17.110	2393	2401	2413	rVV	1208523	2005157	69.44%	8.660%
38	17.192	2413	2415	2421	rVB7	5234	7719	0.27%	0.033%
39	17.392	2444	2449	2451	rBV6	3021	5082	0.18%	0.022%
40	17.522	2466	2471	2474	rBV6	2322	3904	0.14%	0.017%
41	17.804	2515	2519	2526	rBV8	8396	15091	0.52%	0.065%
42	17.857	2526	2528	2533	rVV6	2165	3076	0.11%	0.013%
43	17.933	2536	2541	2550	rBV3	59646	90836	3.15%	0.392%
44	18.010	2550	2554	2557	rVB2	5309	8313	0.29%	0.036%
45	18.233	2589	2592	2597	rBV6	3313	4997	0.17%	0.022%
46	19.033	2723	2728	2732	rBV2	19986	30700	1.06%	0.133%
47	19.104	2737	2740	2745	rVV	16789	27168	0.94%	0.117%
48	19.151	2745	2748	2750	rVV4	6871	7542	0.26%	0.033%
49	19.269	2763	2768	2773	rBV6	21896	35702	1.24%	0.154%
50	19.486	2799	2805	2818	rBV	1680754	2572176	89.07%	11.108%
51	21.433	3130	3136	3147	rBV	1272699	1928014	66.77%	8.326%
52	24.421	3634	3644	3660	rVB	1064560	2887662	100.00%	12.471%
53	24.645	3674	3682	3702	rVB	748608	2053339	71.11%	8.868%
54	30.356	4651	4653	4656	rBV2	25473	33106	1.15%	0.143%




Sum of corrected areas: 23155274

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023071.D
Acq On : 13 Nov 2024 08:06
Operator : RC/JU
Sample : P4687-09
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

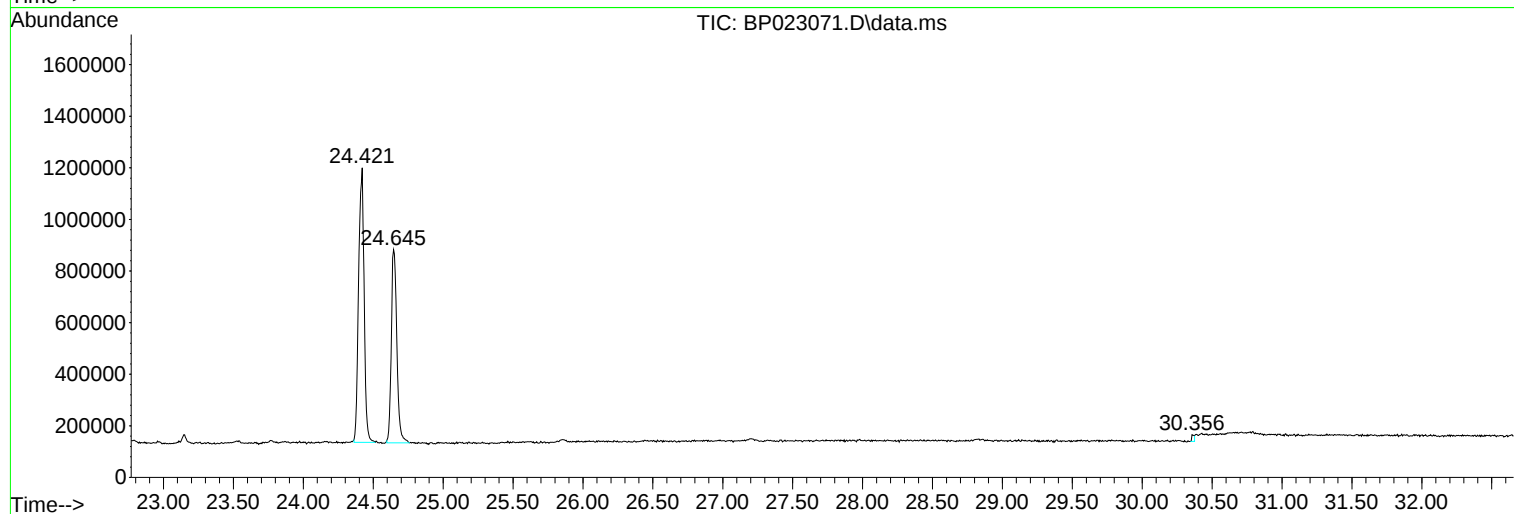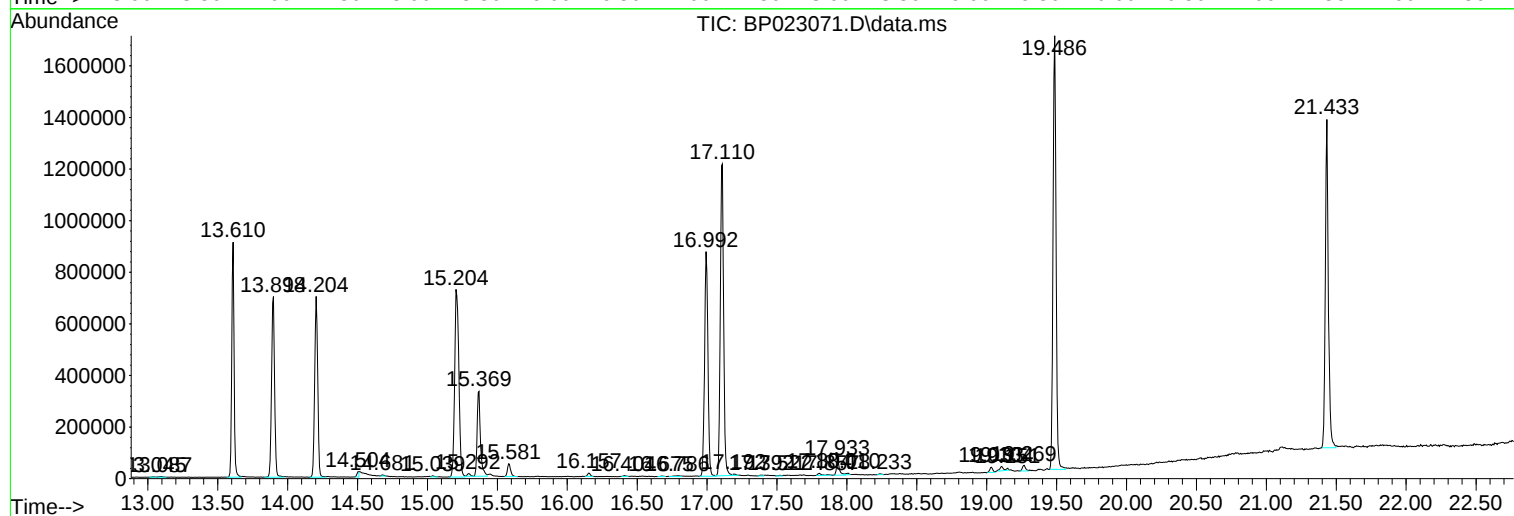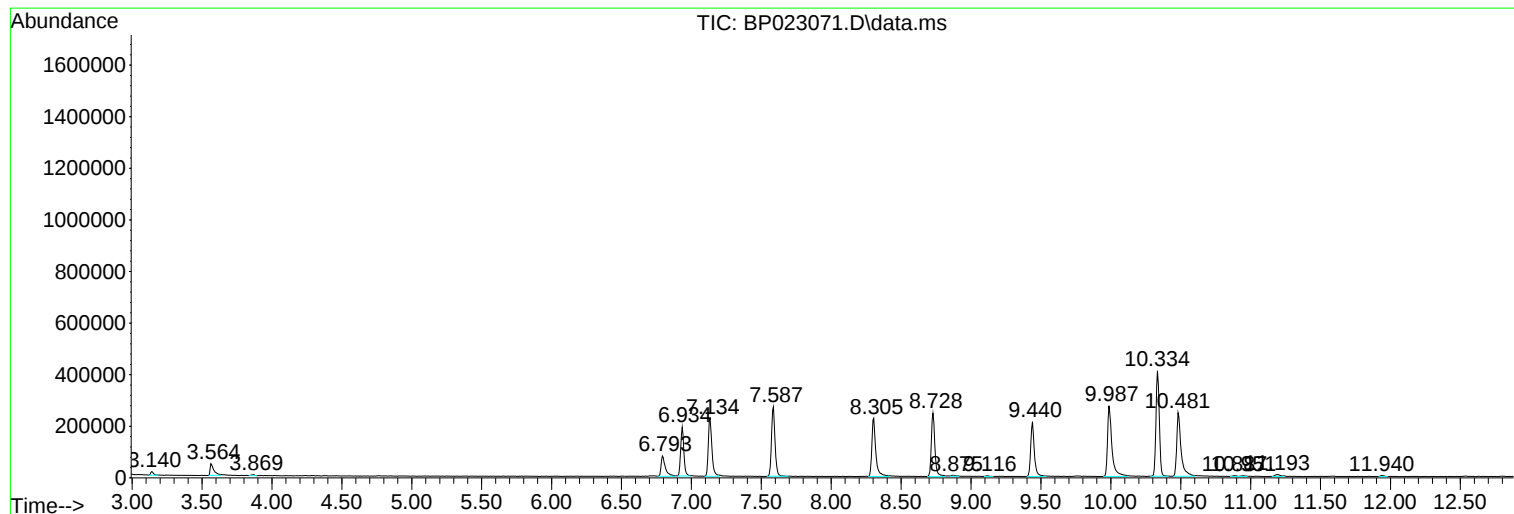

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023071.D
Acq On : 13 Nov 2024 08:06
Operator : RC/JU
Sample : P4687-09
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111224\
Data File : BP023071.D
Acq On : 13 Nov 2024 08:06
Operator : RC/JU
Sample : P4687-09
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
